

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030991.D
 Acq On : 18 Apr 2024 01:23
 Operator : MA/JU
 Sample : P2036-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030991.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	18	22	25	rBV	52355	73435	1.11%	0.145%
2	3.146	25	27	39	rVB	38650	71275	1.08%	0.141%
3	3.564	96	98	114	rBV	93257	191808	2.89%	0.379%
4	3.875	147	151	154	rVB3	6556	8820	0.13%	0.017%
5	4.387	233	238	253	rVB	161200	283110	4.27%	0.560%
6	6.816	644	651	659	rBV	104025	172632	2.60%	0.341%
7	6.981	673	679	691	rBV	465468	752556	11.35%	1.489%
8	7.169	705	711	722	rBV	405339	661856	9.99%	1.309%
9	7.640	784	791	800	rBV	690822	1111617	16.77%	2.199%
10	8.346	903	911	922	rBV	339741	547839	8.27%	1.084%
11	8.793	980	987	998	rBV	553153	910704	13.74%	1.801%
12	8.905	1002	1006	1009	rVV6	4448	6670	0.10%	0.013%
13	9.510	1100	1109	1124	rBV	417839	662084	9.99%	1.310%
14	10.040	1193	1199	1215	rBV	628781	1050508	15.85%	2.078%
15	10.422	1256	1264	1275	rBV	1061354	1778389	26.83%	3.518%
16	10.563	1281	1288	1308	rBV	673616	1146668	17.30%	2.268%
17	12.016	1530	1535	1544	rBV	11610	19367	0.29%	0.038%
18	13.181	1729	1733	1740	rVB4	9548	14724	0.22%	0.029%
19	13.704	1813	1822	1836	rBV	1602342	2185703	32.98%	4.324%
20	13.975	1860	1868	1879	rBV	1783983	2475259	37.35%	4.896%
21	14.287	1914	1921	1932	rBV	1830156	2683299	40.48%	5.308%
22	14.498	1951	1957	1967	rBV	98502	185960	2.81%	0.368%
23	15.145	2064	2067	2071	rVB4	5435	6671	0.10%	0.013%
24	15.281	2083	2090	2103	rBV	2359493	3336408	50.34%	6.600%
25	15.404	2105	2111	2122	rBV	675784	897689	13.54%	1.776%
26	15.522	2128	2131	2135	rVB3	8673	9826	0.15%	0.019%
27	16.010	2208	2214	2217	rBV4	10080	14023	0.21%	0.028%
28	16.069	2220	2224	2228	rVB5	7212	9797	0.15%	0.019%
29	16.798	2345	2348	2354	rBV5	9760	17088	0.26%	0.034%
30	17.034	2382	2388	2399	rBV	2501860	3454606	52.12%	6.834%
31	17.134	2399	2405	2421	rVV2	2816310	4046051	61.04%	8.004%
32	17.533	2470	2473	2480	rVB3	8937	11032	0.17%	0.022%
33	17.933	2536	2541	2547	rBV5	26602	39853	0.60%	0.079%
34	18.233	2588	2592	2595	rBV3	9472	13255	0.20%	0.026%
35	18.263	2595	2597	2607	rVB5	11488	21534	0.32%	0.043%
36	18.998	2718	2722	2729	rVB2	39613	51116	0.77%	0.101%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030991.D
Acq On : 18 Apr 2024 01:23
Operator : MA/JU
Sample : P2036-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSY7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	19.069	2730	2734	2739	rBV	35439	49665	0.75%	0.098%
38	19.222	2756	2760	2769	rBV6	24213	40877	0.62%	0.081%
39	19.433	2790	2796	2812	rVV2	3757895	5162757	77.89%	10.213%
40	21.269	3102	3108	3118	rBV	3085012	4371380	65.95%	8.647%
41	23.974	3558	3568	3590	rVB2	2709962	6628043	100.00%	13.111%
42	24.168	3593	3601	3616	rVB2	2190194	5377263	81.13%	10.637%




Sum of corrected areas: 50553217

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030991.D
Acq On : 18 Apr 2024 01:23
Operator : MA/JU
Sample : P2036-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSY7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

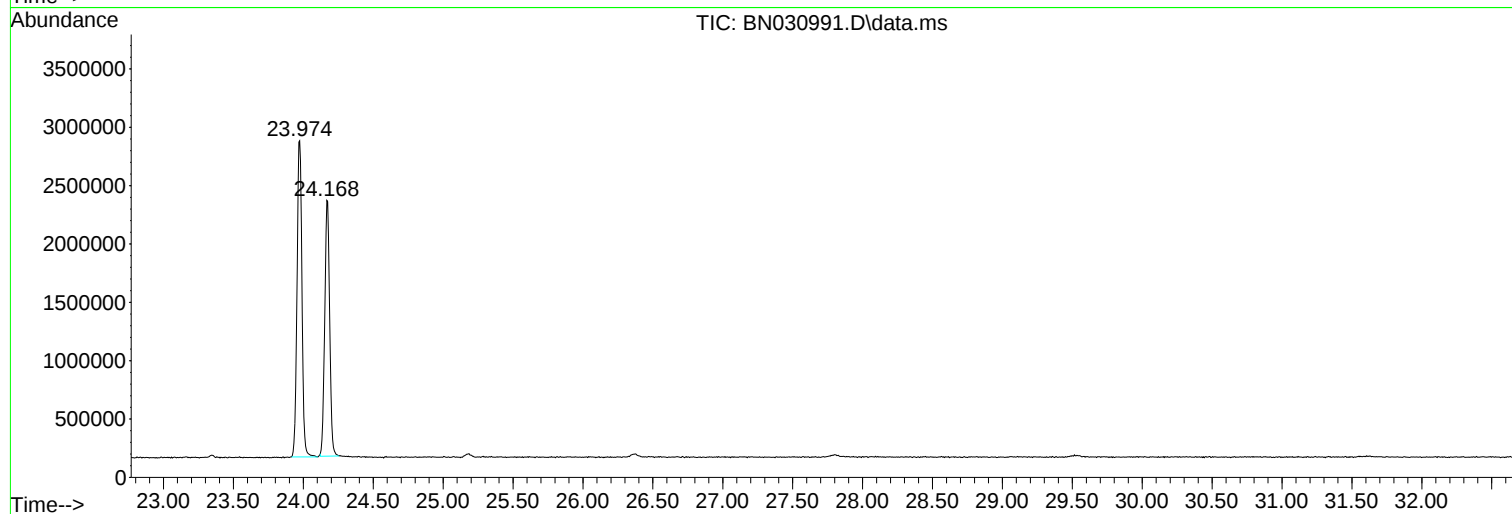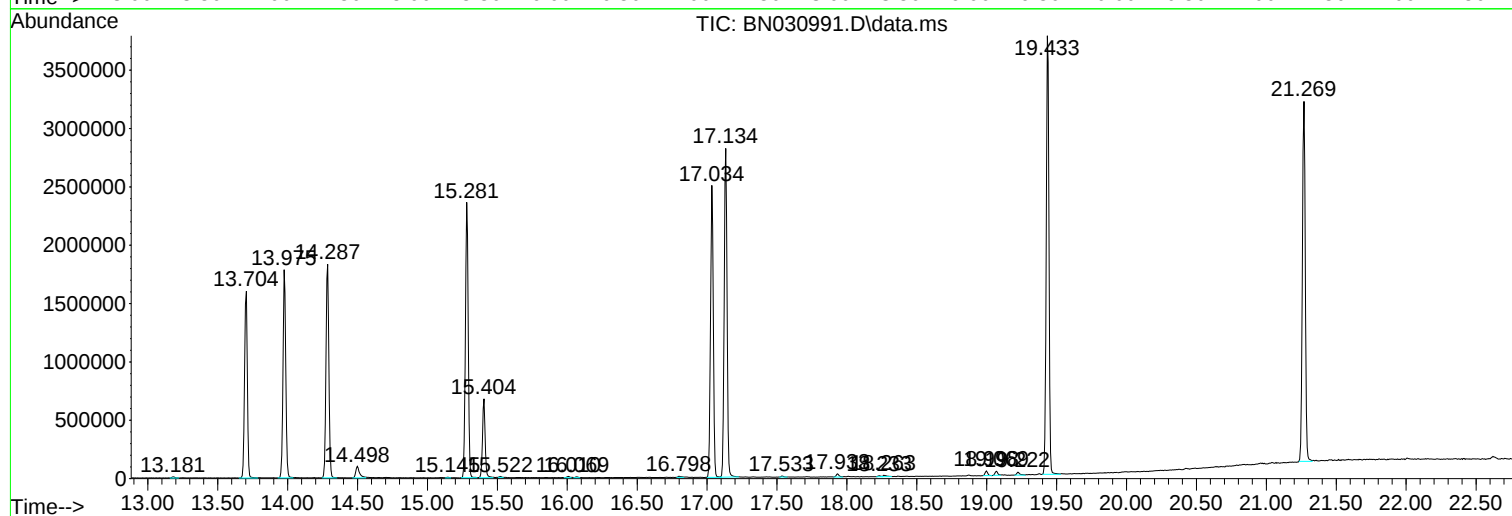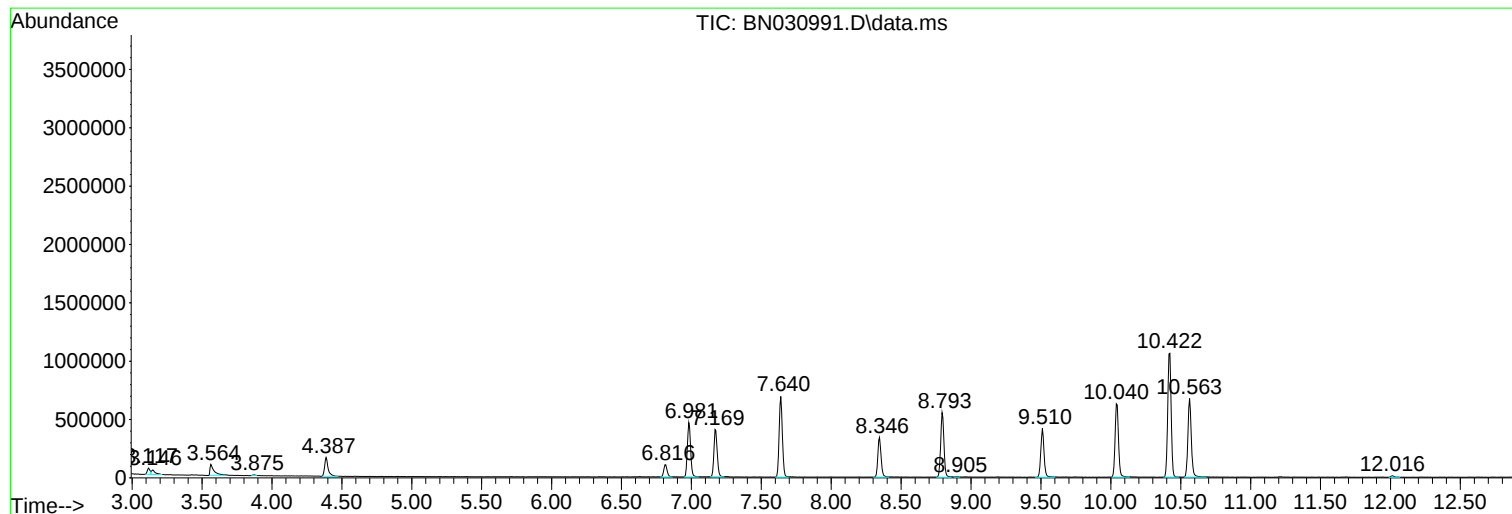

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030991.D
Acq On : 18 Apr 2024 01:23
Operator : MA/JU
Sample : P2036-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSY7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.387	5.09 ng/ul	283110	1,4-Dichlorobenzene-d4	7.640

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			2,4-Dichloro-6-fluoropyrimidine	166	C4HC12FN2	003833-57-6	27

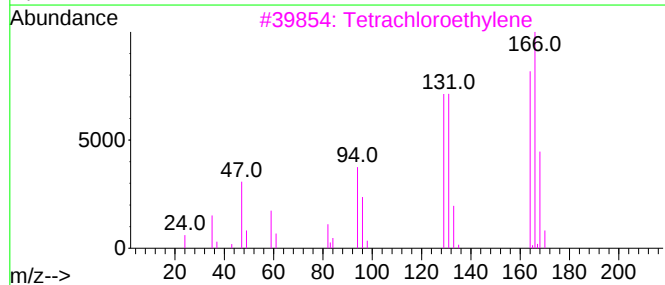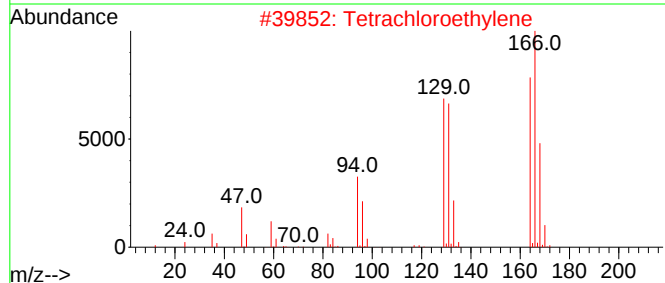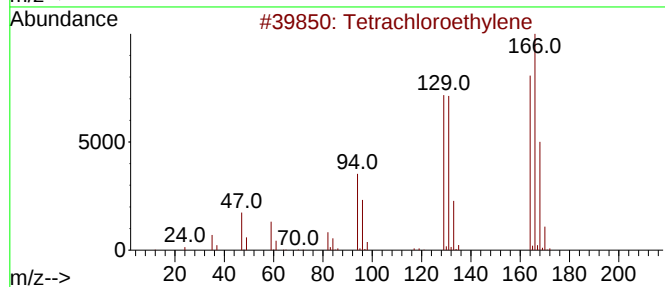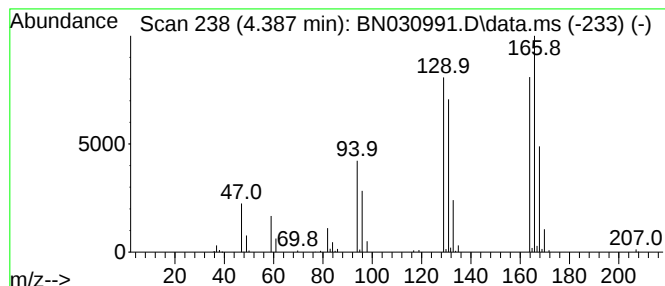

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030991.D
Acq On : 18 Apr 2024 01:23
Operator : MA/JU
Sample : P2036-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSY7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.387	5.1	ng/ul	283110	1	7.640	1111620	20.0