

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030993.D
 Acq On : 18 Apr 2024 02:42
 Operator : MA/JU
 Sample : P2053-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030993.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	17	22	32	rBV	342511	592461	9.74%	1.373%
2	3.564	96	98	117	rBV	89752	190407	3.13%	0.441%
3	3.870	145	150	159	rVB4	5683	11788	0.19%	0.027%
4	4.387	232	238	250	rVB	87509	148493	2.44%	0.344%
5	6.811	645	650	660	rVB	73997	125302	2.06%	0.290%
6	6.981	673	679	691	rBV	391078	621958	10.23%	1.442%
7	7.169	705	711	722	rBV	317360	513207	8.44%	1.190%
8	7.640	783	791	798	rBV	484568	775261	12.75%	1.797%
9	8.346	904	911	921	rBV	233083	378915	6.23%	0.878%
10	8.793	980	987	1000	rBV	449826	749360	12.32%	1.737%
11	8.957	1009	1015	1020	rBV4	10174	18234	0.30%	0.042%
12	9.510	1102	1109	1118	rBV	314280	508571	8.36%	1.179%
13	10.040	1192	1199	1215	rBV	586236	943693	15.52%	2.188%
14	10.416	1256	1263	1272	rBV	760551	1258608	20.70%	2.918%
15	10.563	1281	1288	1306	rBV	526336	933480	15.35%	2.164%
16	11.210	1393	1398	1402	rVB6	5309	7766	0.13%	0.018%
17	12.016	1528	1535	1543	rBV3	10740	18214	0.30%	0.042%
18	13.175	1729	1732	1737	rBV3	7271	10888	0.18%	0.025%
19	13.698	1815	1821	1834	rBV	1451474	1987287	32.69%	4.607%
20	13.975	1860	1868	1879	rBV	1570412	2283275	37.55%	5.293%
21	14.287	1914	1921	1932	rBV	1253582	1864131	30.66%	4.321%
22	14.498	1948	1957	1970	rBV	68399	137411	2.26%	0.319%
23	14.651	1980	1983	1989	rBV6	7207	12330	0.20%	0.029%
24	14.710	1989	1993	1999	rVB5	5907	9581	0.16%	0.022%
25	15.116	2058	2062	2065	rBV	14053	15580	0.26%	0.036%
26	15.281	2084	2090	2101	rBV	2211760	3084767	50.74%	7.151%
27	15.404	2105	2111	2124	rVV	524967	709406	11.67%	1.645%
28	15.522	2127	2131	2140	rVB6	9443	15464	0.25%	0.036%
29	16.069	2219	2224	2227	rVB4	6258	8302	0.14%	0.019%
30	16.445	2284	2288	2294	rBV6	6564	11236	0.18%	0.026%
31	16.586	2305	2312	2319	rBV6	4976	8736	0.14%	0.020%
32	16.804	2345	2349	2356	rBV5	7937	18435	0.30%	0.043%
33	16.963	2372	2376	2381	rVB4	15385	16609	0.27%	0.039%
34	17.034	2382	2388	2398	rBV	1810741	2463631	40.52%	5.711%
35	17.134	2398	2405	2417	rBV	2585081	3592087	59.08%	8.327%
36	17.428	2451	2455	2462	rVB8	4419	9266	0.15%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030993.D
 Acq On : 18 Apr 2024 02:42
 Operator : MA/JU
 Sample : P2053-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	17.810	2513	2520	2526	rBV9	7564	18495	0.30%	0.043%
38	17.933	2536	2541	2542	rBV	100799	111047	1.83%	0.257%
39	17.957	2542	2545	2559	rVV	215197	323483	5.32%	0.750%
40	18.081	2563	2566	2570	rVV2	12356	17385	0.29%	0.040%
41	18.181	2581	2583	2586	rVV3	7405	8144	0.13%	0.019%
42	18.233	2586	2592	2595	rVV	13931	23505	0.39%	0.054%
43	18.269	2596	2598	2607	rVB7	10663	18517	0.30%	0.043%
44	18.363	2612	2614	2619	rVB5	7495	10331	0.17%	0.024%
45	18.804	2687	2689	2697	rVB9	9694	17184	0.28%	0.040%
46	18.998	2717	2722	2727	rBV2	34928	54316	0.89%	0.126%
47	19.069	2730	2734	2737	rBV	37712	57805	0.95%	0.134%
48	19.104	2737	2740	2748	rVB4	38781	58647	0.96%	0.136%
49	19.222	2756	2760	2766	rBV4	50526	71190	1.17%	0.165%
50	19.375	2783	2786	2790	rBV3	16033	18230	0.30%	0.042%
51	19.433	2790	2796	2804	rBV	3493110	4723413	77.69%	10.950%
52	19.904	2873	2876	2881	rBV6	16978	20872	0.34%	0.048%
53	20.963	3052	3056	3067	rBV4	77248	132752	2.18%	0.308%
54	21.269	3102	3108	3120	rBV	2243839	3244098	53.36%	7.520%
55	23.974	3558	3568	3583	rBV2	2517985	6080098	100.00%	14.095%
56	24.168	3592	3601	3614	rBV2	1674967	4074123	67.01%	9.444%




Sum of corrected areas: 43137775

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030993.D
Acq On : 18 Apr 2024 02:42
Operator : MA/JU
Sample : P2053-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YC556

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

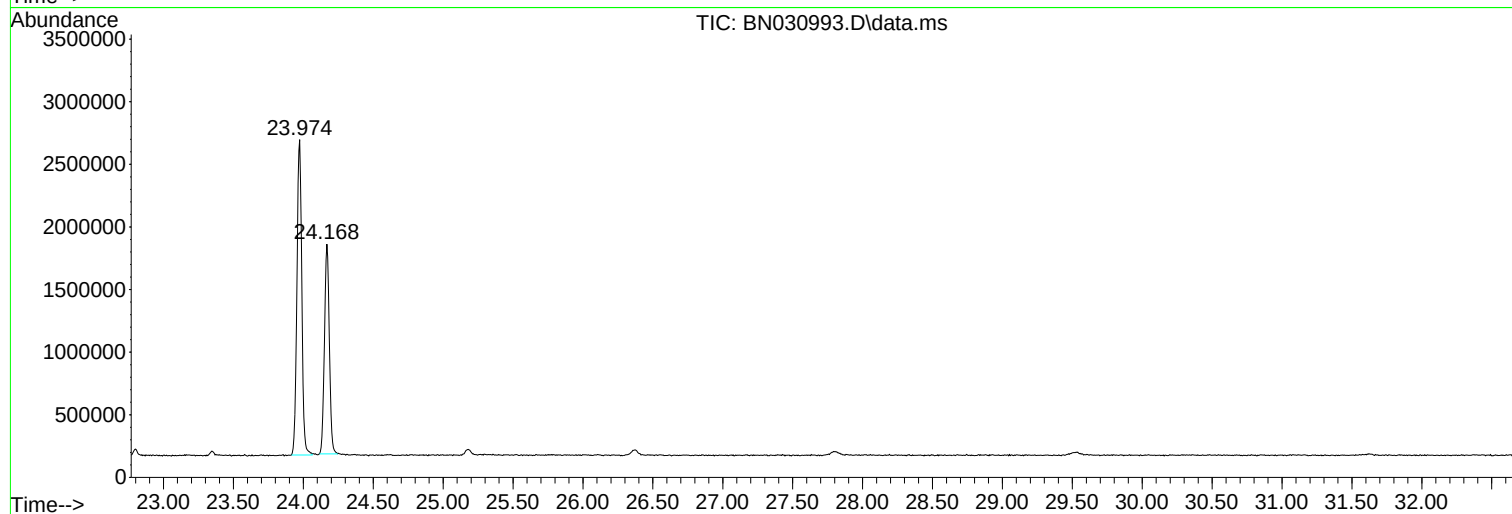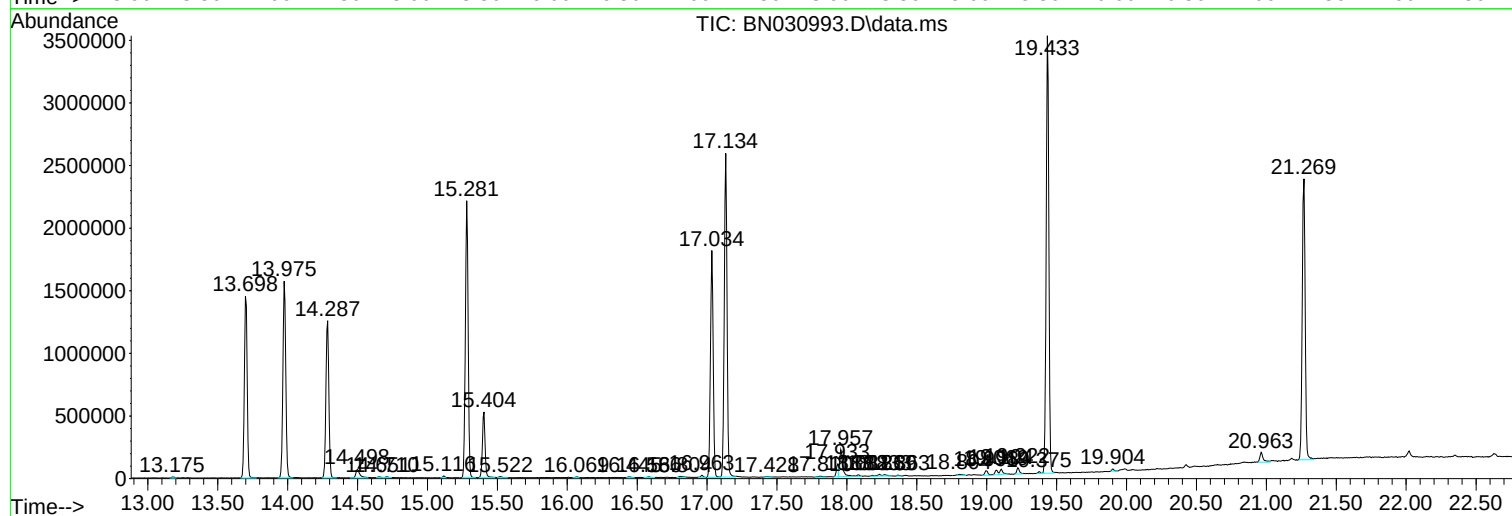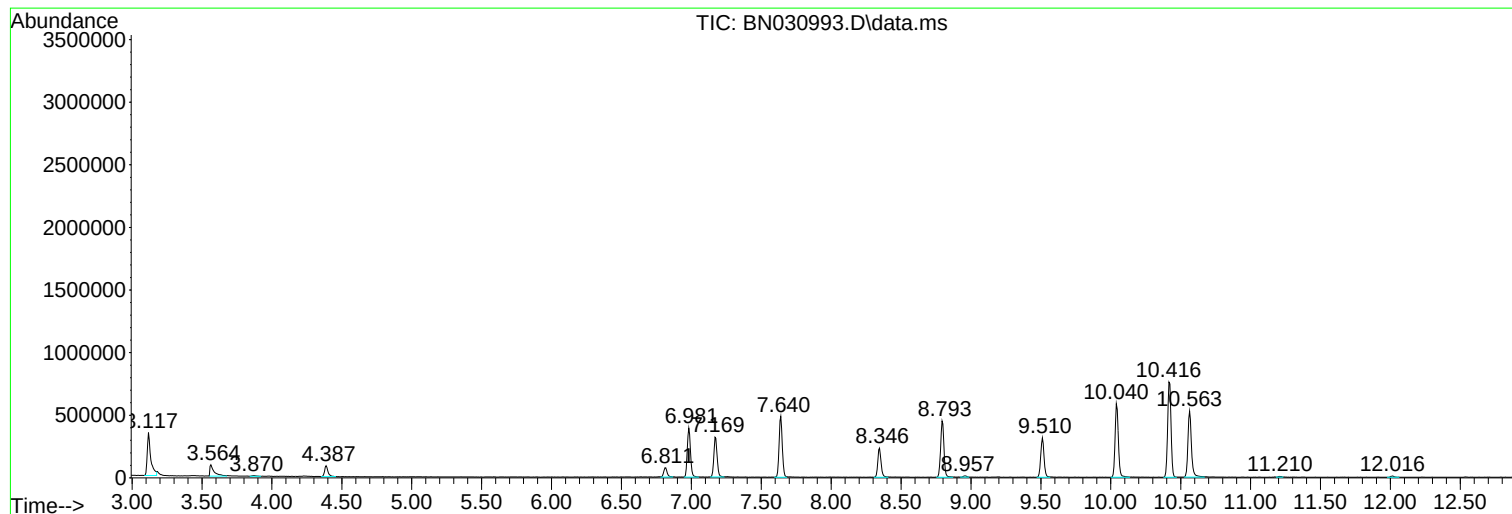

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030993.D
Acq On : 18 Apr 2024 02:42
Operator : MA/JU
Sample : P2053-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSS6









Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.387	3.83 ng/ul	148493	1,4-Dichlorobenzene-d4	7.640

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	25

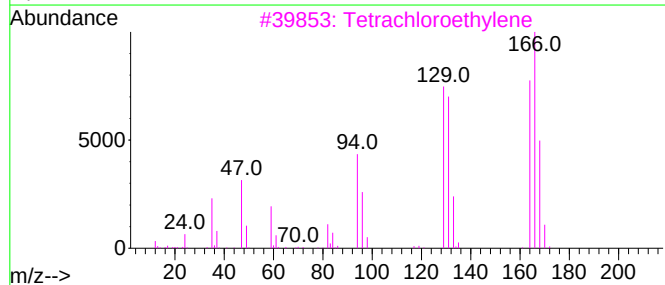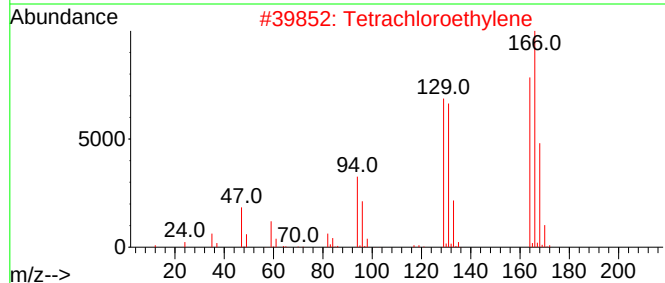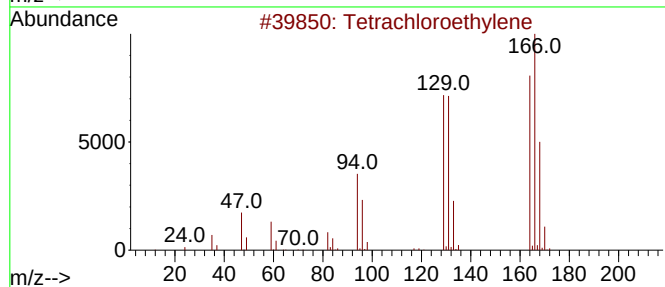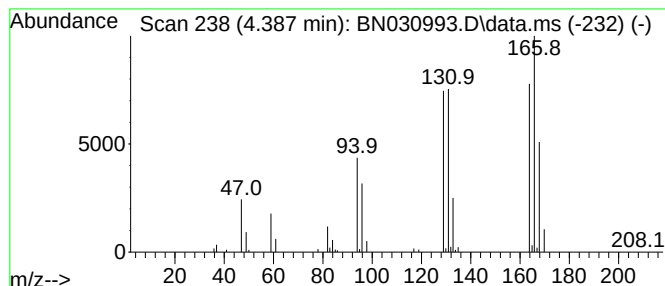

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030993.D
Acq On : 18 Apr 2024 02:42
Operator : MA/JU
Sample : P2053-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YC556










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Cyclic17.957 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.957	2.63 ng/ul	323483	Phenanthrene-d10	17.034

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclotetradecane	196	C14H28	000295-17-0	58
2			4-Heptafluorobutyroxytridecane	396	C17H27F7O2	1000245-49-6	58
3			1-Heptadecene	238	C17H34	006765-39-5	58
4			5-Octadecene, (E)-	252	C18H36	007206-21-5	58
5			7-Hexadecene, (Z)-	224	C16H32	035507-09-6	58

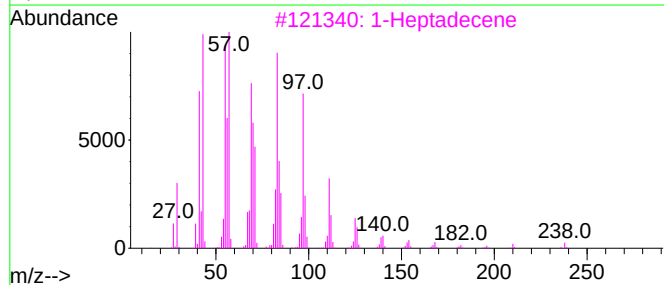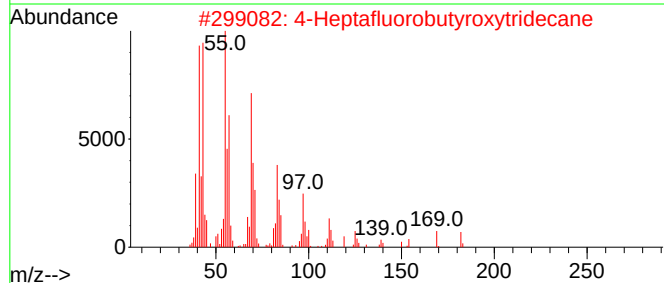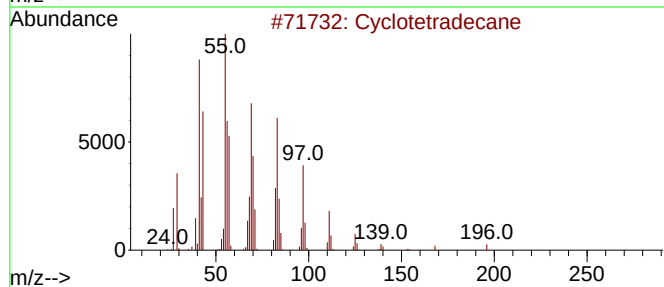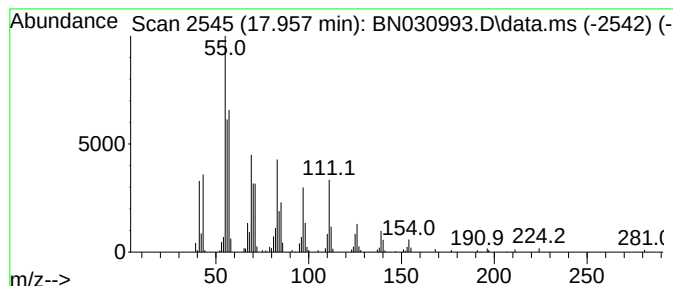

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030993.D
Acq On : 18 Apr 2024 02:42
Operator : MA/JU
Sample : P2053-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YCSS6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.387	3.8	ng/u1	148493	1	7.640	775261	20.0
(DEL) Alkane: C...	17.957	2.6	ng/u1	323483	4	17.034	2463630	20.0