

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030994.D
 Acq On : 18 Apr 2024 03:21
 Operator : MA/JU
 Sample : P2053-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YCSS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030994.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	18	22	38	rVB2	119718	240474	3.92%	0.547%
2	3.564	95	98	122	rBV	89698	187137	3.05%	0.425%
3	3.870	146	150	158	rVB4	8297	15879	0.26%	0.036%
4	4.387	233	238	251	rVB	112535	188421	3.07%	0.428%
5	6.811	644	650	659	rBV	101486	167423	2.73%	0.381%
6	6.981	673	679	692	rVB	457805	707566	11.55%	1.608%
7	7.169	702	711	723	rBV	394696	633234	10.33%	1.439%
8	7.640	784	791	803	rBV	520316	823391	13.44%	1.872%
9	8.346	903	911	925	rBV	334256	533703	8.71%	1.213%
10	8.793	979	987	1000	rBV	531338	864027	14.10%	1.964%
11	9.510	1102	1109	1117	rBV	378742	598624	9.77%	1.361%
12	10.040	1192	1199	1214	rBV	614605	1011512	16.50%	2.299%
13	10.416	1253	1263	1273	rBV	776970	1321064	21.56%	3.003%
14	10.563	1281	1288	1300	rBV	665101	1088174	17.76%	2.473%
15	11.828	1498	1503	1509	rVB3	4621	7339	0.12%	0.017%
16	12.016	1529	1535	1541	rBV2	11511	18962	0.31%	0.043%
17	13.128	1718	1724	1728	rBV	63577	89680	1.46%	0.204%
18	13.181	1729	1733	1739	rVB2	11574	17050	0.28%	0.039%
19	13.698	1814	1821	1832	rBV	1497294	2029398	33.11%	4.613%
20	13.975	1861	1868	1880	rBV	1626086	2357066	38.46%	5.358%
21	14.287	1914	1921	1934	rBV	1356744	1960890	32.00%	4.457%
22	14.498	1949	1957	1967	rBV2	93283	172733	2.82%	0.393%
23	14.587	1967	1972	1976	rVB7	6414	12306	0.20%	0.028%
24	14.698	1989	1991	1999	rVB7	4082	9333	0.15%	0.021%
25	15.116	2055	2062	2068	rBV	25288	33528	0.55%	0.076%
26	15.281	2083	2090	2099	rBV	2240519	3165614	51.65%	7.195%
27	15.404	2104	2111	2121	rBV	595783	787826	12.85%	1.791%
28	15.522	2127	2131	2136	rVB2	10109	14445	0.24%	0.033%
29	15.910	2193	2197	2201	rBV	14825	17860	0.29%	0.041%
30	16.069	2220	2224	2230	rVB3	7153	9935	0.16%	0.023%
31	17.034	2381	2388	2398	rBV	1859613	2540685	41.46%	5.775%
32	17.134	2398	2405	2418	rVV	2701861	3741865	61.06%	8.505%
33	17.539	2470	2474	2477	rVB4	6081	6746	0.11%	0.015%
34	17.934	2536	2541	2550	rBV2	50824	78897	1.29%	0.179%
35	18.228	2588	2591	2594	rBV4	5180	7882	0.13%	0.018%
36	18.263	2595	2597	2602	rVB2	7067	10212	0.17%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030994.D
Acq On : 18 Apr 2024 03:21
Operator : MA/JU
Sample : P2053-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YC557

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	18.998	2717	2722	2728	rBV3	33902	49888	0.81%	0.113%
38	19.069	2729	2734	2739	rBV	38000	55024	0.90%	0.125%
39	19.222	2756	2760	2770	rBV2	55317	81227	1.33%	0.185%
40	19.433	2790	2796	2805	rBV	3655705	4869790	79.46%	11.069%
41	21.269	3102	3108	3118	rBV2	2353279	3302850	53.89%	7.507%
42	23.974	3559	3568	3588	rVB2	2650218	6128566	100.00%	13.930%
43	24.168	3593	3601	3616	rVB	1653093	4036721	65.87%	9.175%




Sum of corrected areas: 43994947

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030994.D
Acq On : 18 Apr 2024 03:21
Operator : MA/JU
Sample : P2053-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YC557

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

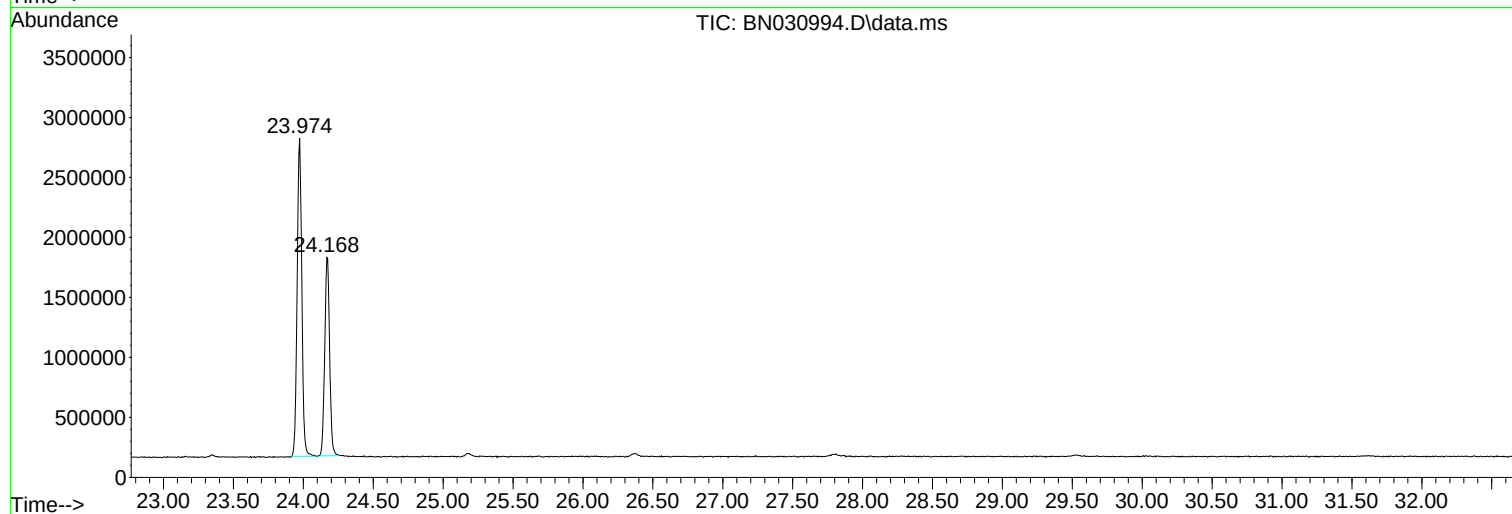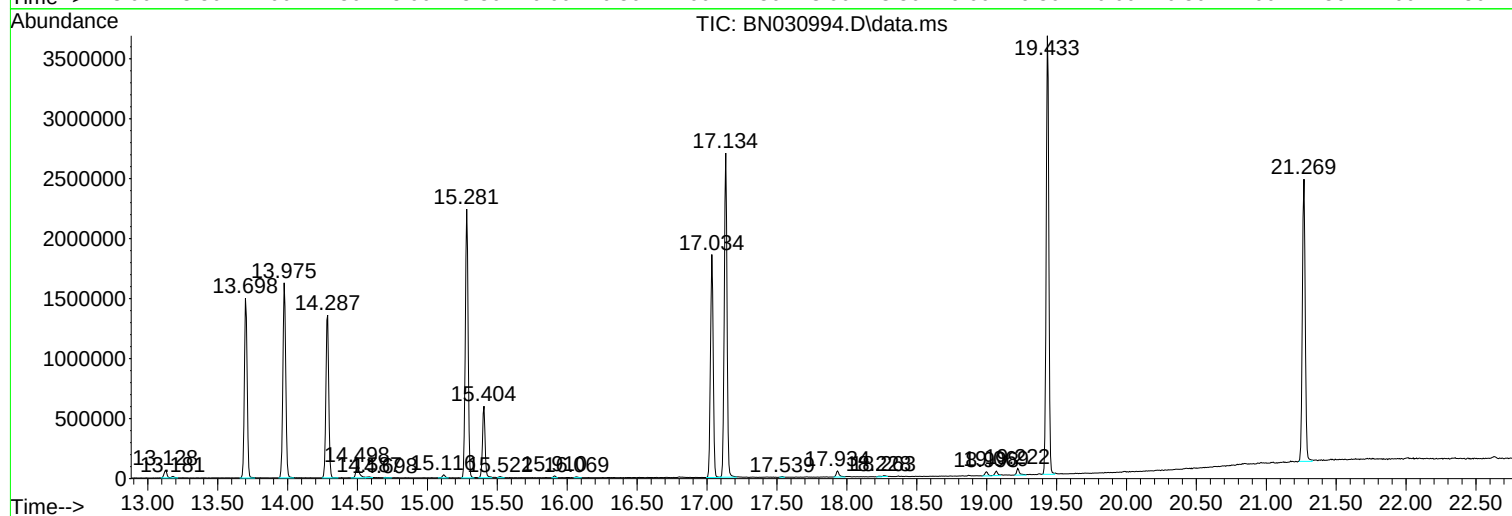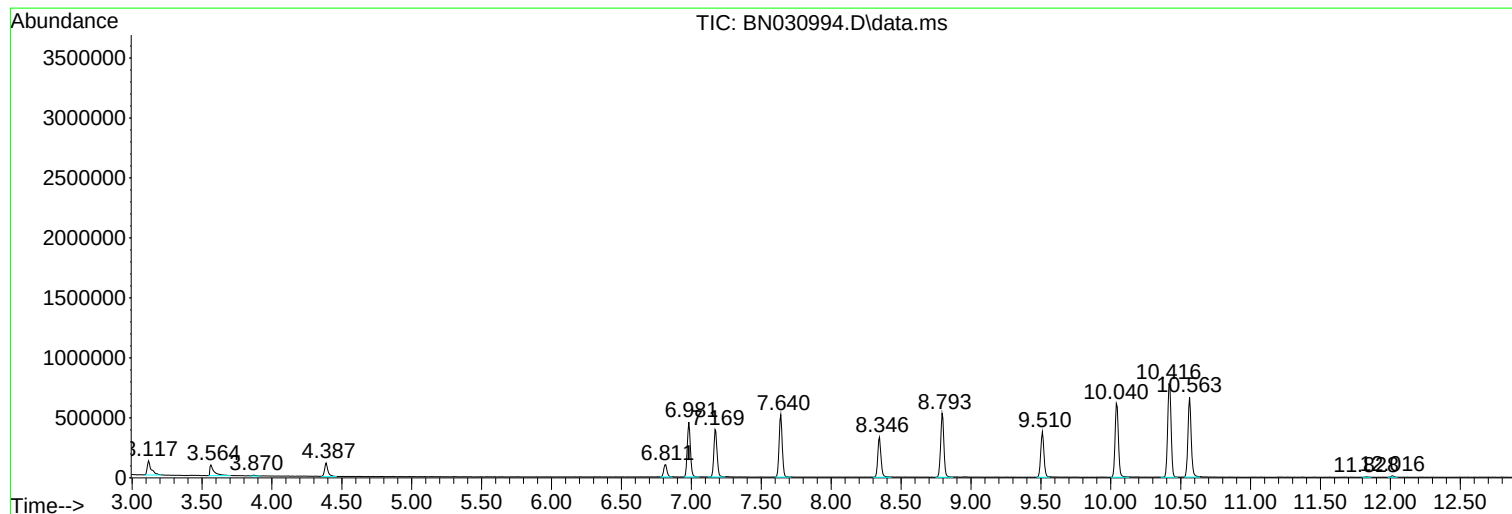

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030994.D
Acq On : 18 Apr 2024 03:21
Operator : MA/JU
Sample : P2053-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YC557









Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.387	4.58 ng/ul	188421	1,4-Dichlorobenzene-d4	7.640

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	35

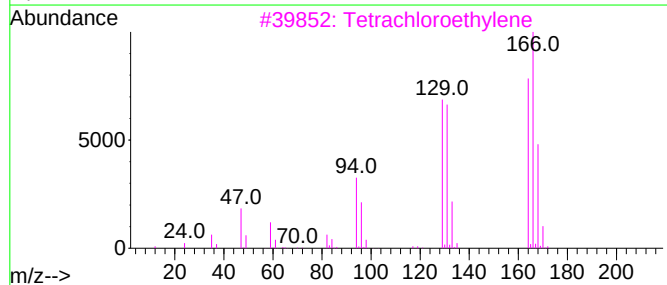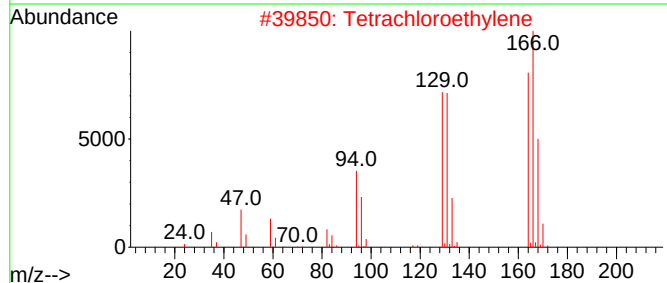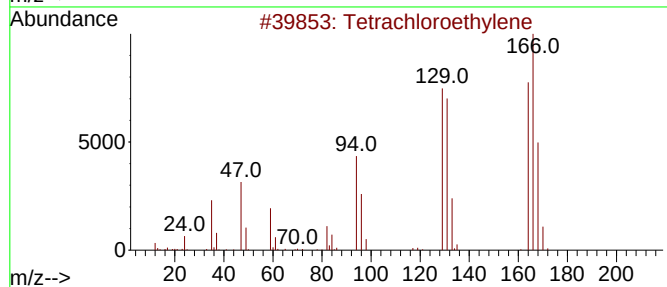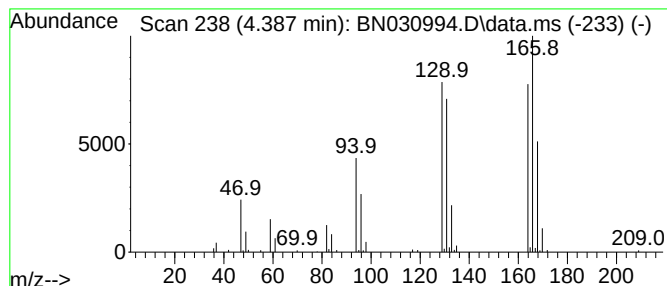

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030994.D
Acq On : 18 Apr 2024 03:21
Operator : MA/JU
Sample : P2053-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YC557

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.387	4.6	ng/ul	188421	1	7.640	823391	20.0