

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030996.D
 Acq On : 18 Apr 2024 04:40
 Operator : MA/JU
 Sample : P2077-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030996.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	25	28	33	rVB2	13543	16724	0.31%	0.042%
2	3.570	97	99	110	rBV	40544	75347	1.38%	0.191%
3	3.875	147	151	155	rVB4	5932	9438	0.17%	0.024%
4	6.816	644	651	662	rVB	73085	124850	2.29%	0.317%
5	6.981	673	679	690	rBV	404717	630296	11.56%	1.600%
6	7.169	705	711	721	rBV	329022	535286	9.82%	1.358%
7	7.640	784	791	799	rBV	525970	833320	15.28%	2.115%
8	8.346	905	911	922	rBV	255690	410501	7.53%	1.042%
9	8.793	979	987	996	rBV	452372	748164	13.72%	1.899%
10	8.957	1010	1015	1019	rBB5	5650	7198	0.13%	0.018%
11	9.199	1049	1056	1061	rVB7	4993	9070	0.17%	0.023%
12	9.363	1078	1084	1090	rVB3	5415	8107	0.15%	0.021%
13	9.510	1102	1109	1119	rBV	310793	499191	9.15%	1.267%
14	9.916	1175	1178	1188	rBV5	3300	7185	0.13%	0.018%
15	10.040	1191	1199	1218	rBV	522272	866025	15.88%	2.198%
16	10.416	1255	1263	1274	rBV	815184	1348536	24.73%	3.422%
17	10.563	1280	1288	1304	rBV	435642	752979	13.81%	1.911%
18	11.169	1386	1391	1396	rBV6	3897	7838	0.14%	0.020%
19	12.010	1530	1534	1540	rBV3	9150	14816	0.27%	0.038%
20	13.181	1728	1733	1739	rVB5	8668	13808	0.25%	0.035%
21	13.698	1814	1821	1832	rBV	1264213	1738394	31.88%	4.412%
22	13.975	1861	1868	1878	rBV	1363177	2002191	36.72%	5.081%
23	14.040	1878	1879	1888	rVB6	3728	6145	0.11%	0.016%
24	14.287	1914	1921	1928	rBV	1360726	1984910	36.40%	5.037%
25	14.498	1951	1957	1967	rBV2	49088	104172	1.91%	0.264%
26	15.281	2083	2090	2102	rBV	1942576	2730021	50.07%	6.928%
27	15.404	2105	2111	2124	rVV	362878	522608	9.58%	1.326%
28	15.516	2127	2130	2136	rVB4	8335	11993	0.22%	0.030%
29	16.069	2220	2224	2229	rVB4	5565	8020	0.15%	0.020%
30	16.910	2365	2367	2372	rVB4	4856	5888	0.11%	0.015%
31	16.963	2372	2376	2381	rBV5	15181	19722	0.36%	0.050%
32	17.034	2381	2388	2398	rBV	1859175	2570674	47.14%	6.524%
33	17.134	2398	2405	2415	rBV	2364039	3244609	59.50%	8.234%
34	17.422	2449	2454	2458	rBV6	4959	9724	0.18%	0.025%
35	17.804	2515	2519	2522	rBV6	5904	7490	0.14%	0.019%
36	17.934	2536	2541	2550	rBV2	48985	73035	1.34%	0.185%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030996.D
 Acq On : 18 Apr 2024 04:40
 Operator : MA/JU
 Sample : P2077-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	18.269	2594	2598	2603	rVB3	11092	17773	0.33%	0.045%
38	18.369	2612	2615	2619	rVB5	8824	8322	0.15%	0.021%
39	18.422	2621	2624	2627	rVB5	4509	5662	0.10%	0.014%
40	18.804	2685	2689	2694	rBV5	10240	17503	0.32%	0.044%
41	18.998	2717	2722	2726	rBV2	31586	45062	0.83%	0.114%
42	19.069	2730	2734	2738	rBV	33353	42997	0.79%	0.109%
43	19.222	2756	2760	2765	rBV2	25855	35109	0.64%	0.089%
44	19.375	2784	2786	2788	rBV2	6038	6522	0.12%	0.017%
45	19.433	2790	2796	2803	rVV	3140093	4223039	77.45%	10.717%
46	20.963	3053	3056	3060	rBV6	38530	46679	0.86%	0.118%
47	21.269	3102	3108	3115	rBV2	2342265	3359879	61.62%	8.527%
48	23.968	3558	3567	3585	rBV2	2306959	5452737	100.00%	13.838%
49	24.168	3592	3601	3617	rVB2	1649055	4183898	76.73%	10.618%




Sum of corrected areas: 39403457

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030996.D
Acq On : 18 Apr 2024 04:40
Operator : MA/JU
Sample : P2077-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

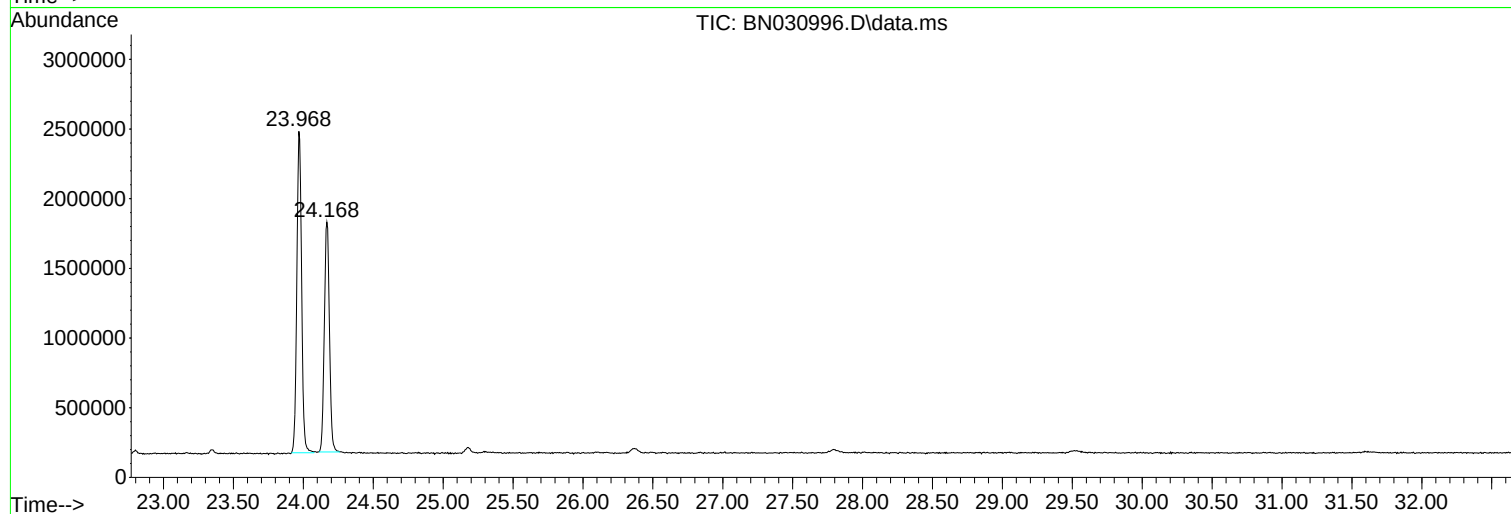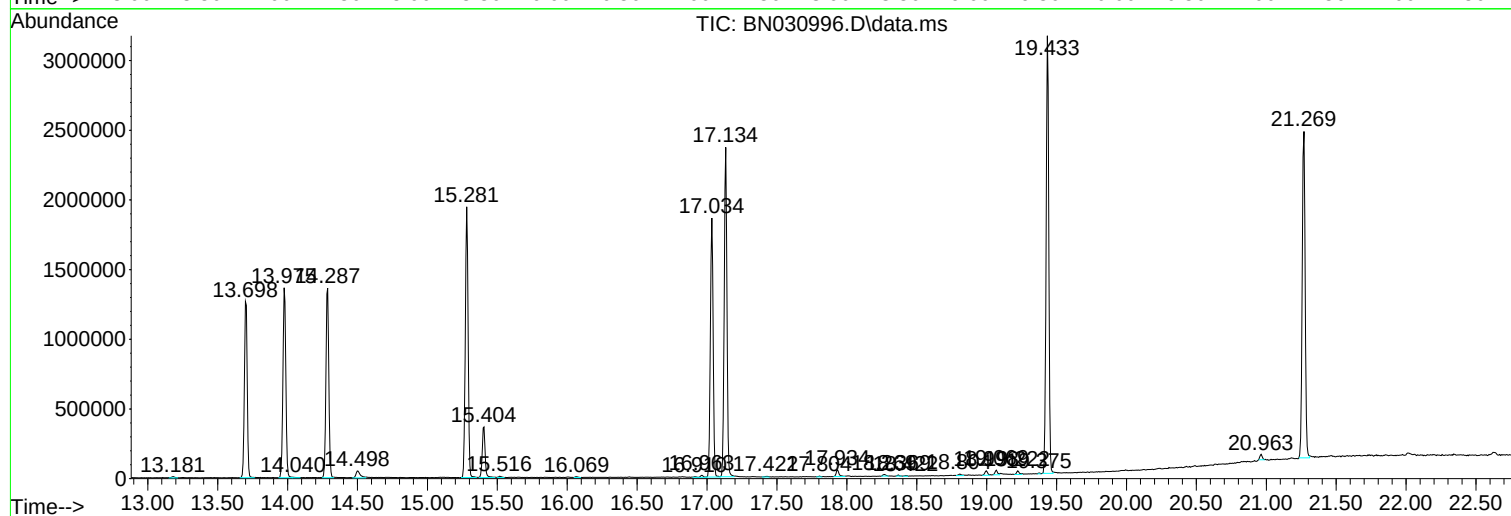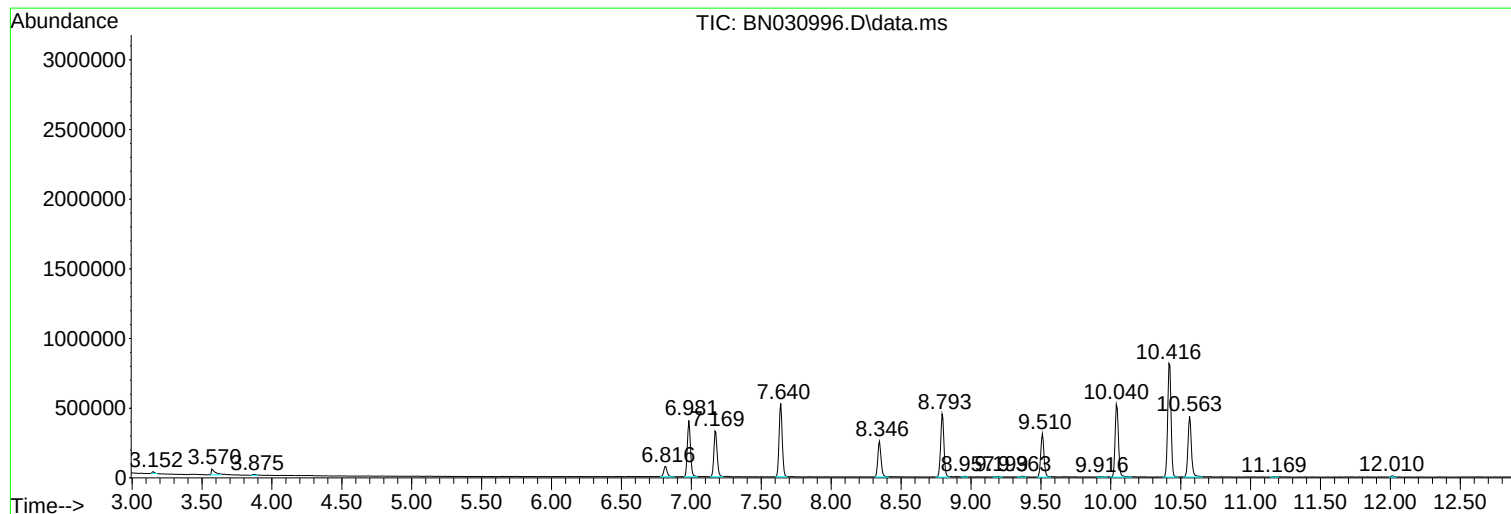

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030996.D
Acq On : 18 Apr 2024 04:40
Operator : MA/JU
Sample : P2077-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030996.D
Acq On : 18 Apr 2024 04:40
Operator : MA/JU
Sample : P2077-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------