

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN030997.D
 Acq On : 18 Apr 2024 05:19
 Operator : MA/JU
 Sample : PB160279BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK279

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	23	27	39	rVB	23641	41778	0.86%	0.113%
2	3.557	94	97	123	rBV	283545	553272	11.32%	1.501%
3	3.875	147	151	156	rVB4	4548	7480	0.15%	0.020%
4	6.810	644	650	661	rBV	453985	711512	14.56%	1.930%
5	6.981	673	679	693	rVB	392353	609407	12.47%	1.653%
6	7.169	705	711	721	rBV	436211	710367	14.54%	1.927%
7	7.639	782	791	799	rBV	404161	636873	13.03%	1.728%
8	8.345	903	911	930	rBV	580205	941464	19.27%	2.554%
9	8.792	979	987	1001	rBV	444035	717749	14.69%	1.947%
10	9.510	1102	1109	1119	rBV	335595	531969	10.89%	1.443%
11	10.039	1193	1199	1213	rBV	574085	938471	19.21%	2.546%
12	10.416	1257	1263	1274	rVB	610611	1012162	20.72%	2.746%
13	10.563	1279	1288	1303	rBV	647965	1087670	22.26%	2.951%
14	12.016	1529	1535	1541	rBV2	8337	14325	0.29%	0.039%
15	13.180	1727	1733	1738	rBV2	9840	14274	0.29%	0.039%
16	13.698	1815	1821	1837	rBV	1188941	1675415	34.29%	4.545%
17	13.974	1860	1868	1880	rBV	1355605	1919654	39.29%	5.208%
18	14.286	1914	1921	1932	rBV	1001278	1500718	30.71%	4.071%
19	14.492	1948	1956	1983	rBV	492409	822615	16.84%	2.232%
20	15.280	2083	2090	2102	rBV	1809212	2510549	51.38%	6.811%
21	15.404	2105	2111	2121	rBV	444756	612155	12.53%	1.661%
22	15.516	2127	2130	2136	rVB4	7095	10937	0.22%	0.030%
23	16.063	2219	2223	2228	rVB5	5082	6576	0.13%	0.018%
24	17.033	2382	2388	2395	rBV	1390064	1952900	39.97%	5.298%
25	17.133	2398	2405	2416	rBV	2144422	2888812	59.12%	7.837%
26	17.933	2538	2541	2546	rBV6	4341	5527	0.11%	0.015%
27	18.998	2718	2722	2727	rVB2	25528	32079	0.66%	0.087%
28	19.068	2729	2734	2740	rBV	21849	33118	0.68%	0.090%
29	19.433	2790	2796	2804	rBV	2823330	3735836	76.46%	10.135%
30	21.268	3102	3108	3118	rBV2	1804602	2557310	52.34%	6.938%
31	23.974	3559	3568	3583	rBV2	2079906	4886130	100.00%	13.255%
32	24.168	3593	3601	3618	rVB	1385260	3182667	65.14%	8.634%




Sum of corrected areas: 36861771

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030997.D
Acq On : 18 Apr 2024 05:19
Operator : MA/JU
Sample : PB160279BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK279

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

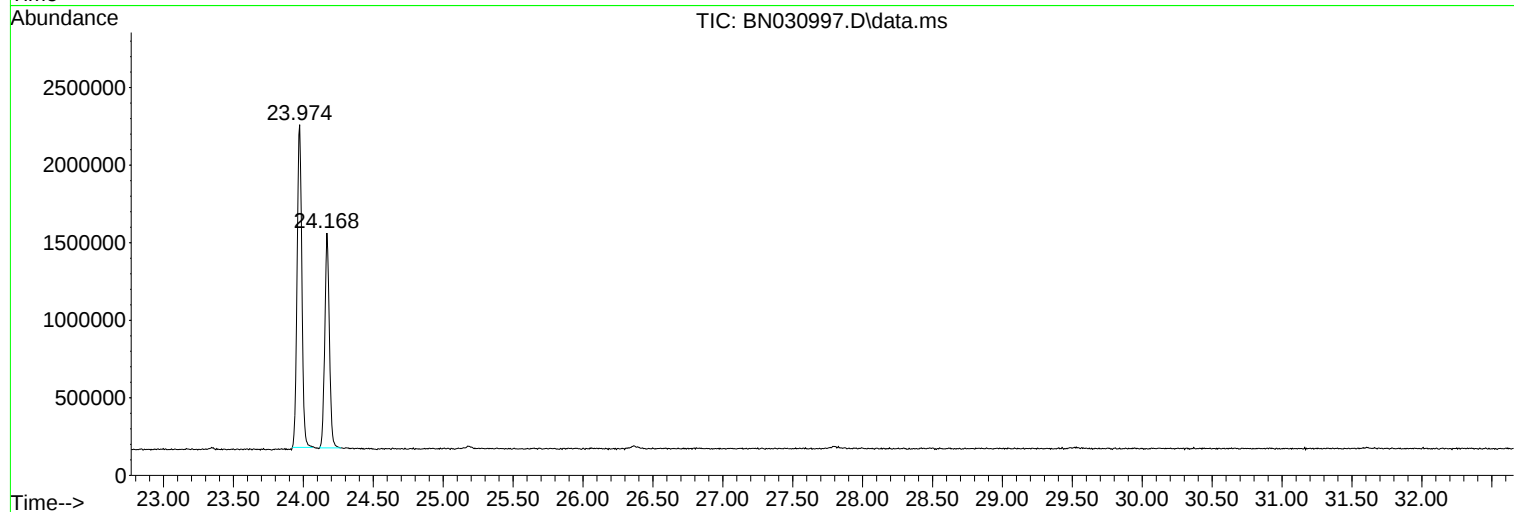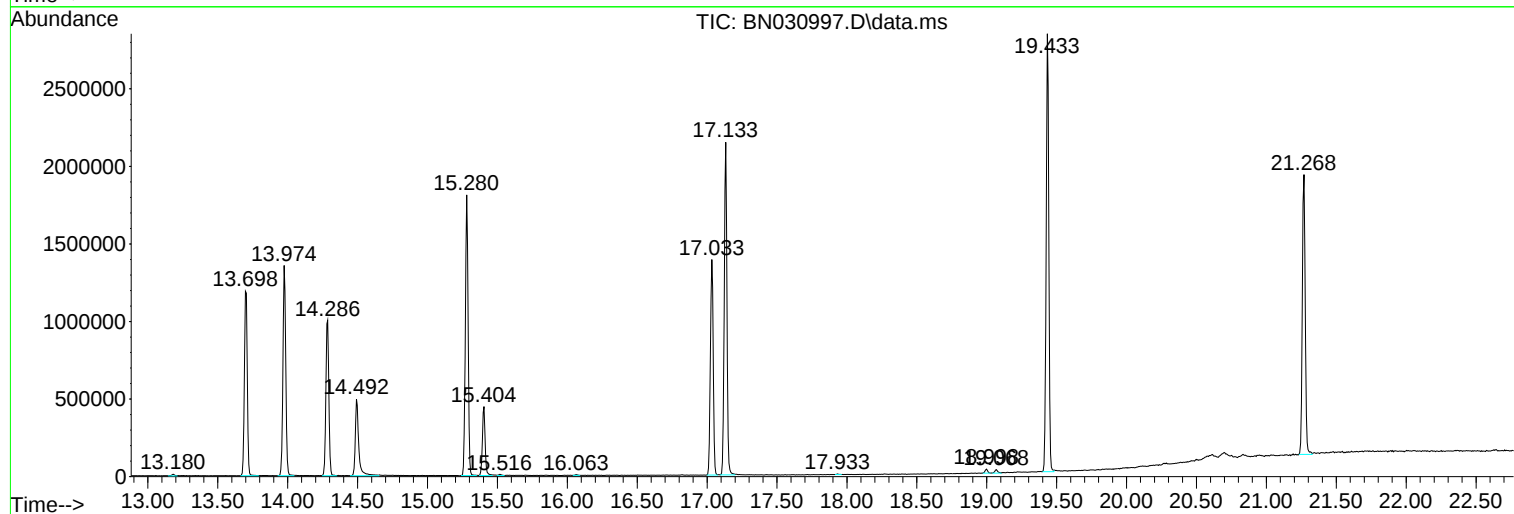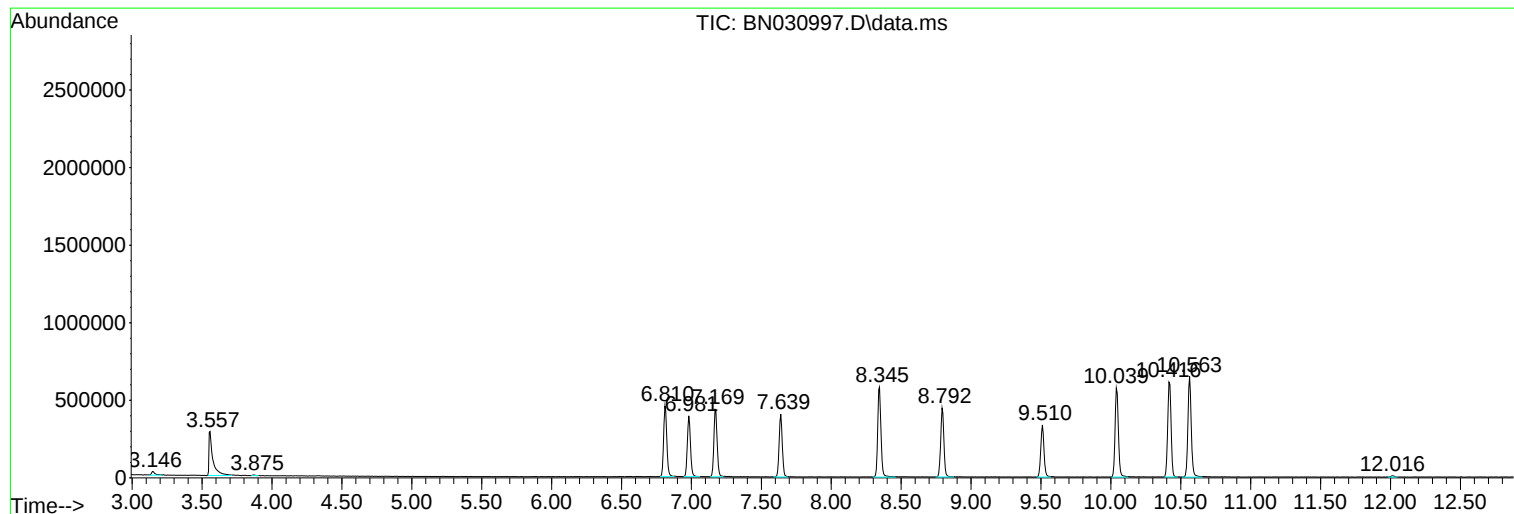

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030997.D
Acq On : 18 Apr 2024 05:19
Operator : MA/JU
Sample : PB160279BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK279

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN030997.D
Acq On : 18 Apr 2024 05:19
Operator : MA/JU
Sample : PB160279BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK279

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc