

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031000.D
 Acq On : 18 Apr 2024 07:57
 Operator : MA/JU
 Sample : PB160277BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK277

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031000.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	37	rVB	25029	40483	0.76%	0.098%
2	3.552	93	96	119	rBV	305761	605569	11.33%	1.461%
3	3.870	147	150	154	rVB3	5482	7124	0.13%	0.017%
4	6.811	642	650	662	rBV	476826	752336	14.08%	1.815%
5	6.981	673	679	688	rBV	417437	641641	12.01%	1.548%
6	7.169	703	711	721	rBV	474229	746620	13.97%	1.802%
7	7.640	784	791	800	rBV	488758	766088	14.34%	1.849%
8	8.340	903	910	922	rBV	613199	981732	18.37%	2.369%
9	8.793	979	987	999	rBV	492596	768009	14.37%	1.853%
10	9.511	1102	1109	1120	rBV	352307	570790	10.68%	1.377%
11	10.040	1193	1199	1208	rBV	607570	983617	18.41%	2.374%
12	10.416	1256	1263	1273	rVB	754434	1239704	23.20%	2.991%
13	10.563	1281	1288	1302	rBV	680073	1145571	21.44%	2.764%
14	12.010	1529	1534	1541	rBV2	10119	17000	0.32%	0.041%
15	13.181	1727	1733	1738	rBV3	10135	15645	0.29%	0.038%
16	13.699	1815	1821	1832	rBV	1413870	1851846	34.65%	4.469%
17	13.975	1861	1868	1878	rBV	1495041	2069347	38.72%	4.993%
18	14.281	1914	1920	1928	rBV	1262630	1844116	34.51%	4.450%
19	14.493	1950	1956	1976	rBV	573977	907375	16.98%	2.190%
20	15.281	2083	2090	2100	rBV	1933013	2720969	50.92%	6.566%
21	15.404	2105	2111	2121	rBV	468044	666104	12.46%	1.607%
22	15.522	2127	2131	2136	rVB2	7777	9974	0.19%	0.024%
23	16.063	2219	2223	2227	rBV4	5387	8010	0.15%	0.019%
24	16.816	2349	2351	2359	rVB4	3789	5665	0.11%	0.014%
25	17.034	2381	2388	2398	rBV	1728438	2419813	45.28%	5.839%
26	17.134	2398	2405	2417	rBV2	2193452	3191262	59.72%	7.701%
27	17.934	2537	2541	2548	rVB8	4681	6292	0.12%	0.015%
28	18.998	2717	2722	2727	rBV3	26396	39399	0.74%	0.095%
29	19.069	2730	2734	2740	rVV	24919	33931	0.63%	0.082%
30	19.434	2790	2796	2806	rBV	3108149	4107560	76.86%	9.912%
31	21.269	3102	3108	3115	rBV2	2156865	3082080	57.67%	7.437%
32	23.969	3559	3567	3590	rVB2	2238736	5344059	100.00%	12.896%
33	24.169	3593	3601	3616	rVB2	1587435	3851394	72.07%	9.294%




Sum of corrected areas: 41441125

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031000.D
Acq On : 18 Apr 2024 07:57
Operator : MA/JU
Sample : PB160277BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK277

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

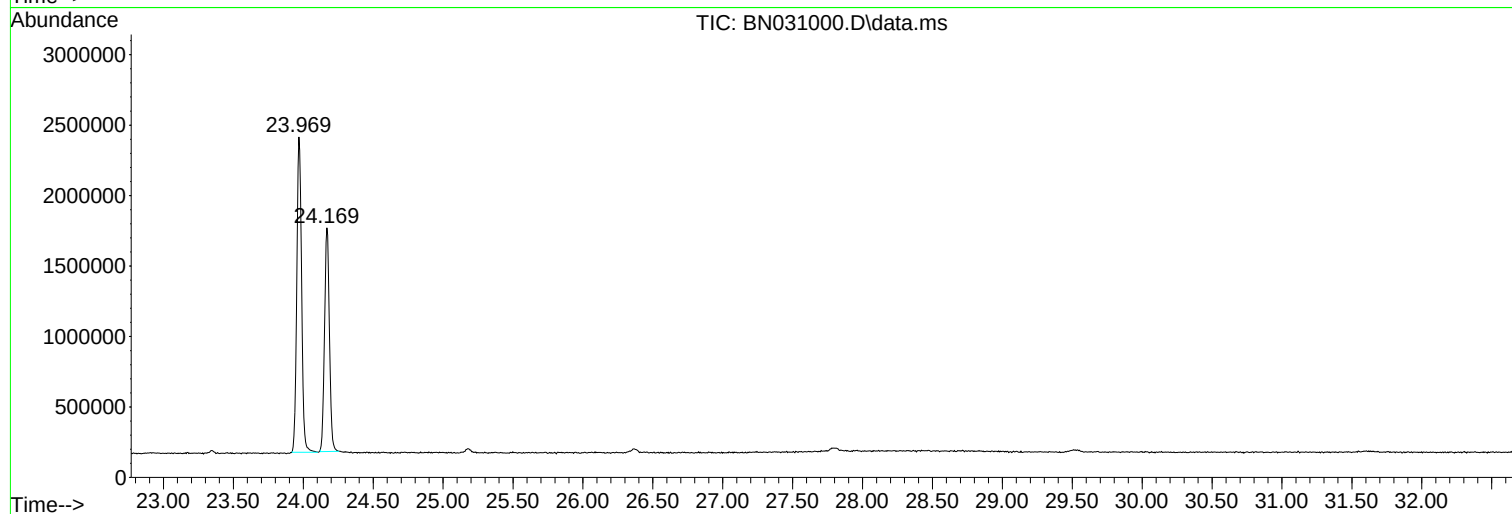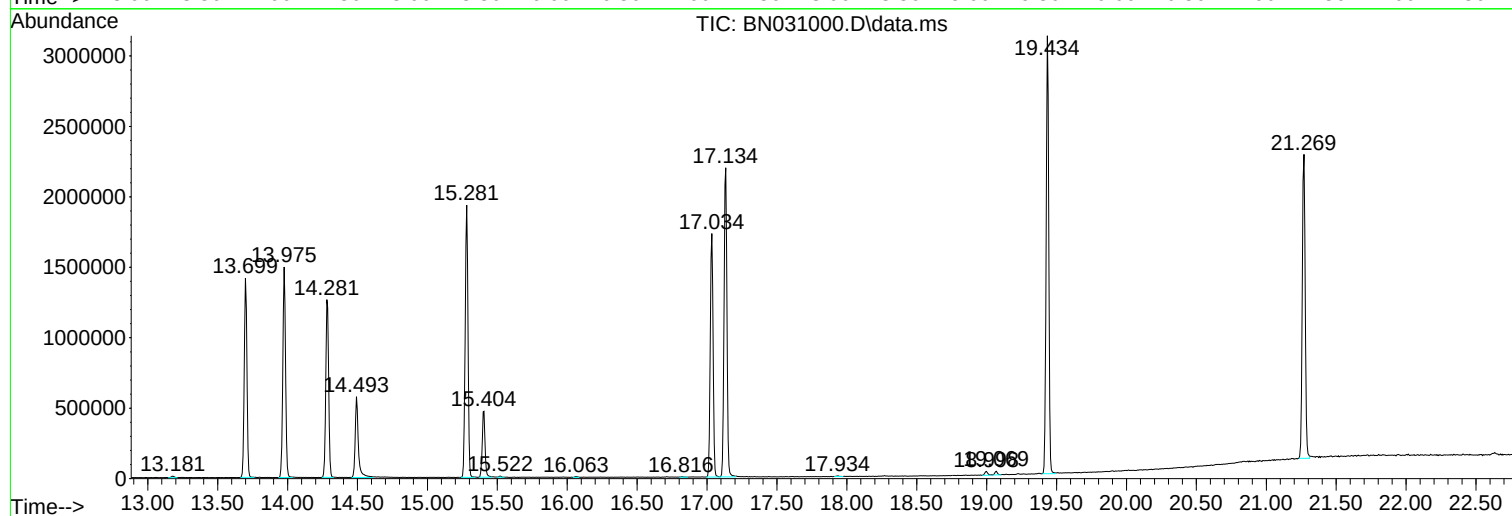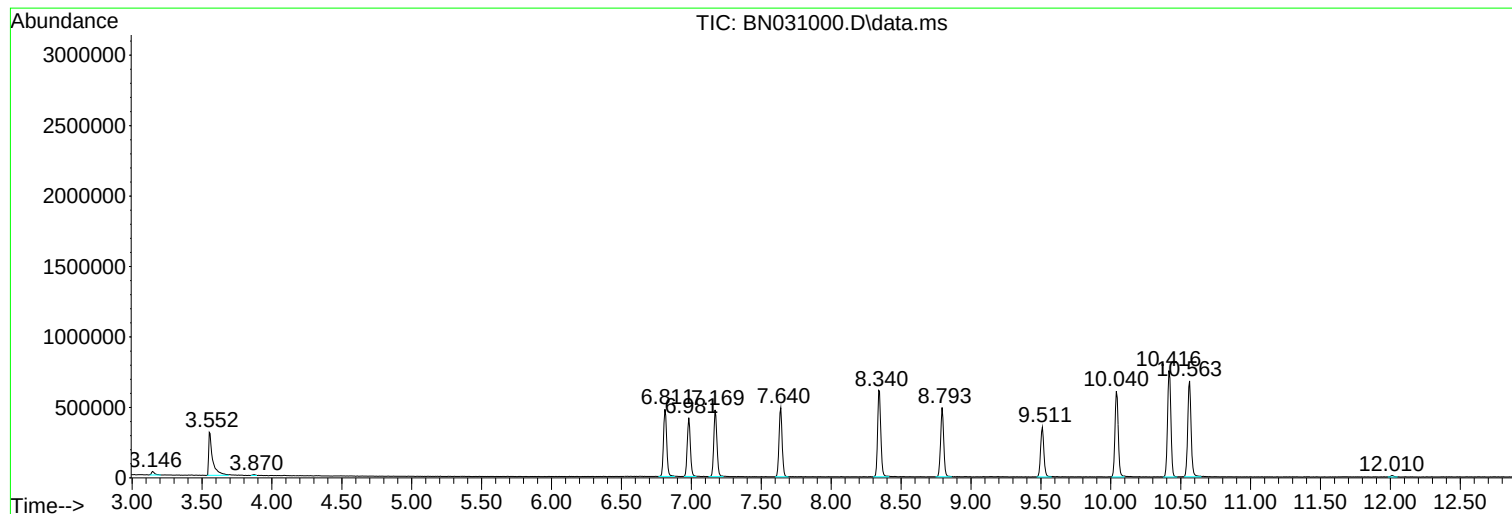

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031000.D
Acq On : 18 Apr 2024 07:57
Operator : MA/JU
Sample : PB160277BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK277

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031000.D
Acq On : 18 Apr 2024 07:57
Operator : MA/JU
Sample : PB160277BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK277

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc