

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031001.D
 Acq On : 18 Apr 2024 08:36
 Operator : MA/JU
 Sample : P2099-11
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0RA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031001.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	35	rVB2	18159	26574	0.42%	0.067%
2	3.569	96	99	117	rBV	51555	116345	1.84%	0.295%
3	4.952	331	334	339	rVB4	6264	9567	0.15%	0.024%
4	6.810	644	650	660	rVB	90446	148536	2.35%	0.377%
5	6.981	673	679	693	rBV	466200	713734	11.31%	1.812%
6	7.169	705	711	722	rBV	384604	612858	9.71%	1.556%
7	7.640	784	791	801	rBV	377312	589634	9.34%	1.497%
8	8.346	904	911	923	rBV	302660	488513	7.74%	1.240%
9	8.793	980	987	997	rBV	532512	862925	13.67%	2.191%
10	9.510	1101	1109	1127	rBV	380247	617104	9.78%	1.567%
11	10.040	1192	1199	1219	rBV	596919	996775	15.79%	2.531%
12	10.416	1256	1263	1271	rBV	575955	949427	15.04%	2.411%
13	10.563	1280	1288	1299	rBV	457016	777197	12.31%	1.973%
14	12.016	1529	1535	1542	rVB	11836	21627	0.34%	0.055%
15	13.175	1728	1732	1738	rVB5	8856	14338	0.23%	0.036%
16	13.698	1815	1821	1838	rVV	1428545	2007768	31.81%	5.098%
17	13.975	1862	1868	1877	rBV	1637866	2324833	36.83%	5.903%
18	14.286	1914	1921	1929	rBV	955476	1420866	22.51%	3.608%
19	14.498	1952	1957	1972	rBV	80533	158502	2.51%	0.402%
20	15.281	2083	2090	2101	rBV	2223385	3079611	48.79%	7.820%
21	15.404	2105	2111	2123	rVV	557292	774150	12.26%	1.966%
22	15.516	2127	2130	2134	rVB2	8695	11688	0.19%	0.030%
23	16.063	2219	2223	2228	rBV3	6905	10036	0.16%	0.025%
24	17.033	2382	2388	2398	rBV	1396796	1882055	29.82%	4.779%
25	17.133	2398	2405	2422	rVV	2803836	3820215	60.52%	9.700%
26	17.710	2498	2503	2507	rBV6	5536	8223	0.13%	0.021%
27	17.933	2536	2541	2549	rBV2	45290	64670	1.02%	0.164%
28	18.998	2718	2722	2728	rBV3	32831	45554	0.72%	0.116%
29	19.069	2729	2734	2738	rBV	32113	47245	0.75%	0.120%
30	19.221	2756	2760	2769	rBV3	41052	58907	0.93%	0.150%
31	19.433	2790	2796	2804	rBV	3534619	4842192	76.71%	12.295%
32	21.268	3102	3108	3121	rBV2	1720405	2463852	39.03%	6.256%
33	23.974	3559	3568	3578	rBV2	2750050	6312340	100.00%	16.028%
34	24.168	3593	3601	3614	rVB3	1249267	3104448	49.18%	7.883%

Sum of corrected areas: 39382309




Instrument :
BNA_N
ClientSampleId :
C0RA9

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031001.D
Acq On : 18 Apr 2024 08:36
Operator : MA/JU
Sample : P2099-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

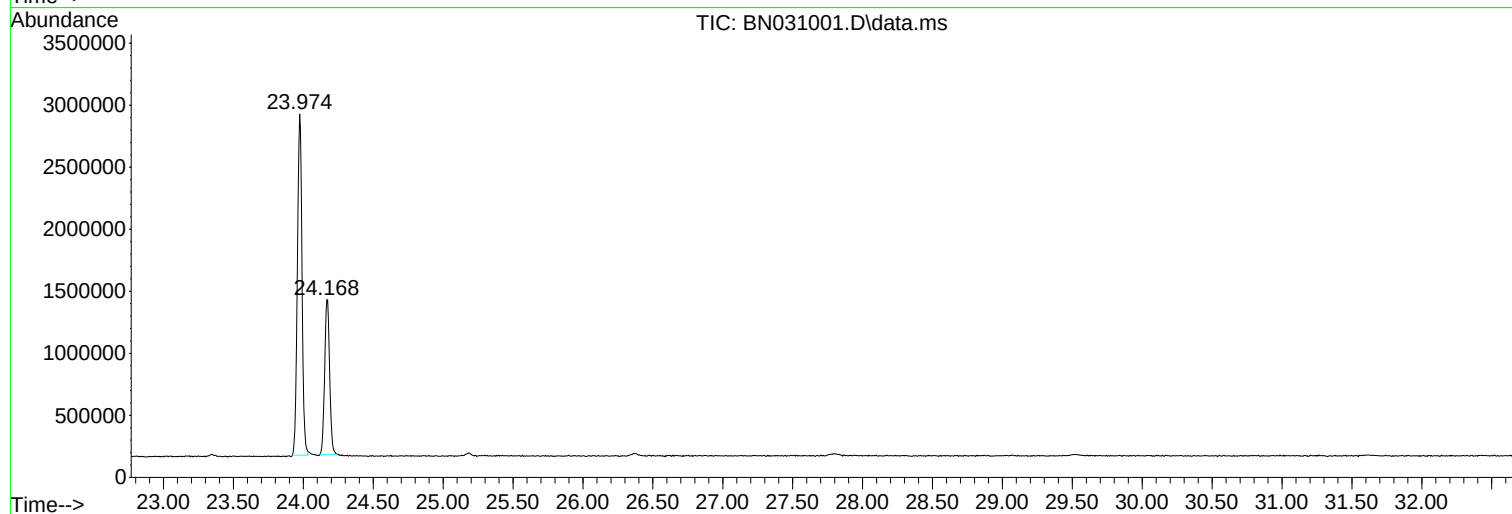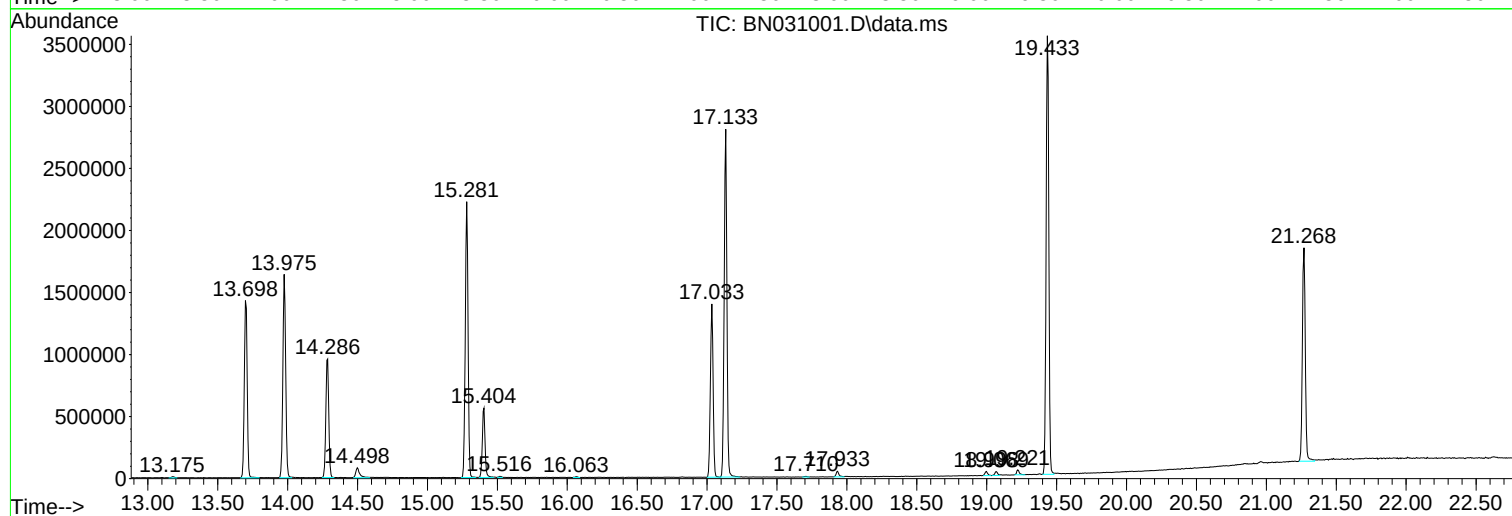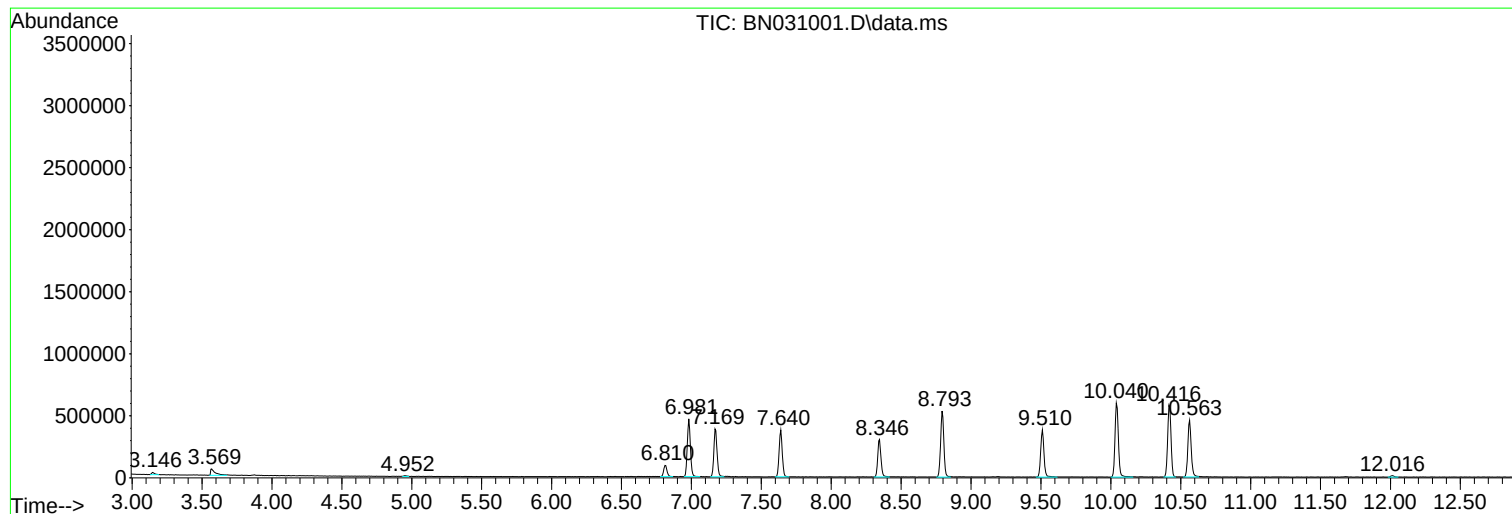

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031001.D
Acq On : 18 Apr 2024 08:36
Operator : MA/JU
Sample : P2099-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031001.D
Acq On : 18 Apr 2024 08:36
Operator : MA/JU
Sample : P2099-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc