

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031003.D
 Acq On : 18 Apr 2024 09:55
 Operator : MA/JU
 Sample : P2077-02
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031003.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	25	27	38	rVB3	12497	19854	0.40%	0.060%
2	3.569	96	99	111	rBV	40428	80274	1.63%	0.244%
3	3.869	147	150	156	rBV4	4762	7582	0.15%	0.023%
4	6.816	645	651	659	rVB	56864	96454	1.96%	0.294%
5	6.981	673	679	689	rBV	312102	487676	9.90%	1.485%
6	7.169	704	711	722	rBV	260985	416875	8.46%	1.269%
7	7.640	784	791	800	rBV	396982	638695	12.97%	1.945%
8	7.722	800	805	813	rVB4	7717	13111	0.27%	0.040%
9	8.346	904	911	922	rBV	187470	306574	6.22%	0.933%
10	8.793	980	987	999	rBV	356895	573021	11.63%	1.745%
11	9.193	1050	1055	1060	rVB3	6980	9293	0.19%	0.028%
12	9.363	1079	1084	1089	rBV7	5272	9227	0.19%	0.028%
13	9.510	1102	1109	1117	rBV	244159	389789	7.91%	1.187%
14	9.646	1128	1132	1135	rBV3	5582	9034	0.18%	0.028%
15	9.916	1174	1178	1186	rVB6	3520	6907	0.14%	0.021%
16	10.040	1193	1199	1211	rBV	419245	678165	13.77%	2.065%
17	10.416	1256	1263	1271	rBV	609561	1028395	20.88%	3.131%
18	10.563	1281	1288	1304	rBV	340069	592628	12.03%	1.804%
19	10.957	1351	1355	1360	rVB5	4088	7570	0.15%	0.023%
20	11.175	1385	1392	1394	rBV7	3782	6580	0.13%	0.020%
21	12.010	1529	1534	1540	rVB2	7325	12402	0.25%	0.038%
22	13.181	1729	1733	1738	rBV3	7904	11279	0.23%	0.034%
23	13.457	1776	1780	1784	rBV3	5771	8948	0.18%	0.027%
24	13.510	1784	1789	1793	rBV3	7115	10536	0.21%	0.032%
25	13.563	1793	1798	1802	rVV4	3269	5240	0.11%	0.016%
26	13.698	1815	1821	1833	rBV	1076647	1423995	28.91%	4.336%
27	13.975	1860	1868	1881	rBV	1111942	1604389	32.57%	4.885%
28	14.281	1914	1920	1927	rBV	1051556	1522522	30.91%	4.636%
29	14.498	1952	1957	1971	rBV2	60238	122976	2.50%	0.374%
30	14.651	1978	1983	1986	rBV3	4242	7547	0.15%	0.023%
31	14.704	1989	1992	1997	rVB5	6133	9954	0.20%	0.030%
32	15.092	2051	2058	2060	rBV6	3634	6731	0.14%	0.020%
33	15.281	2083	2090	2097	rBV	1569753	2220535	45.08%	6.761%
34	15.398	2105	2110	2123	rBV	381492	532766	10.82%	1.622%
35	15.516	2127	2130	2136	rVB3	6347	9229	0.19%	0.028%
36	16.010	2209	2214	2219	rBV8	3768	7475	0.15%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031003.D
Acq On : 18 Apr 2024 09:55
Operator : MA/JU
Sample : P2077-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	16.069	2219	2224	2227	rBV4	7990	12305	0.25%	0.037%
38	16.175	2237	2242	2248	rVB8	3890	6801	0.14%	0.021%
39	16.439	2285	2287	2291	rVB5	5587	6232	0.13%	0.019%
40	16.963	2372	2376	2380	rBV3	12127	16542	0.34%	0.050%
41	17.033	2382	2388	2395	rVV	1466003	2011485	40.84%	6.124%
42	17.133	2398	2405	2415	rBV	1904017	2677416	54.36%	8.152%
43	17.428	2452	2455	2459	rVB6	3044	5227	0.11%	0.016%
44	17.804	2516	2519	2523	rBV6	5171	6374	0.13%	0.019%
45	17.933	2535	2541	2547	rBV	78942	115340	2.34%	0.351%
46	18.263	2593	2597	2603	rVV5	17434	29803	0.61%	0.091%
47	18.369	2612	2615	2618	rVB4	6214	6755	0.14%	0.021%
48	18.416	2621	2623	2628	rVB6	7942	8984	0.18%	0.027%
49	18.804	2687	2689	2695	rVB7	7479	9672	0.20%	0.029%
50	18.998	2718	2722	2726	rBV	26781	36287	0.74%	0.110%
51	19.069	2730	2734	2738	rBV2	31726	45227	0.92%	0.138%
52	19.222	2756	2760	2764	rBV2	55670	69410	1.41%	0.211%
53	19.433	2790	2796	2803	rBV	2853960	3718804	75.50%	11.323%
54	21.269	3102	3108	3118	rBV	1918472	2715945	55.14%	8.269%
55	23.974	3559	3568	3583	rBV2	2214290	4925580	100.00%	14.997%
56	24.168	3593	3601	3617	rVB	1487769	3524863	71.56%	10.732%




Sum of corrected areas: 32843280

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031003.D
Acq On : 18 Apr 2024 09:55
Operator : MA/JU
Sample : P2077-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

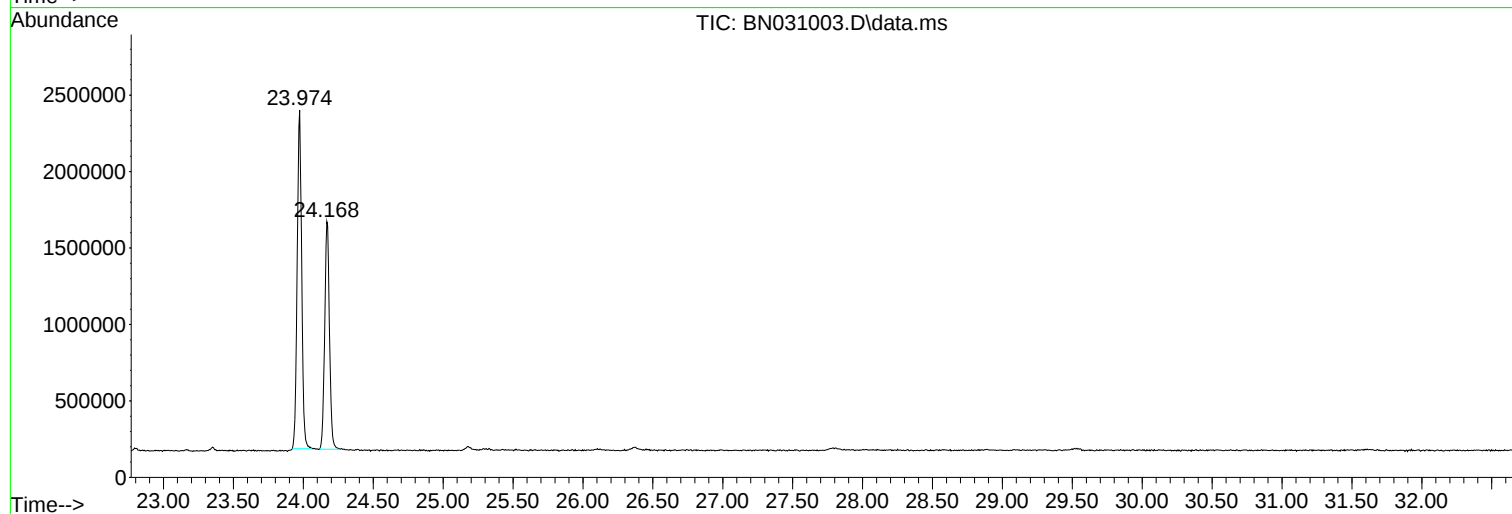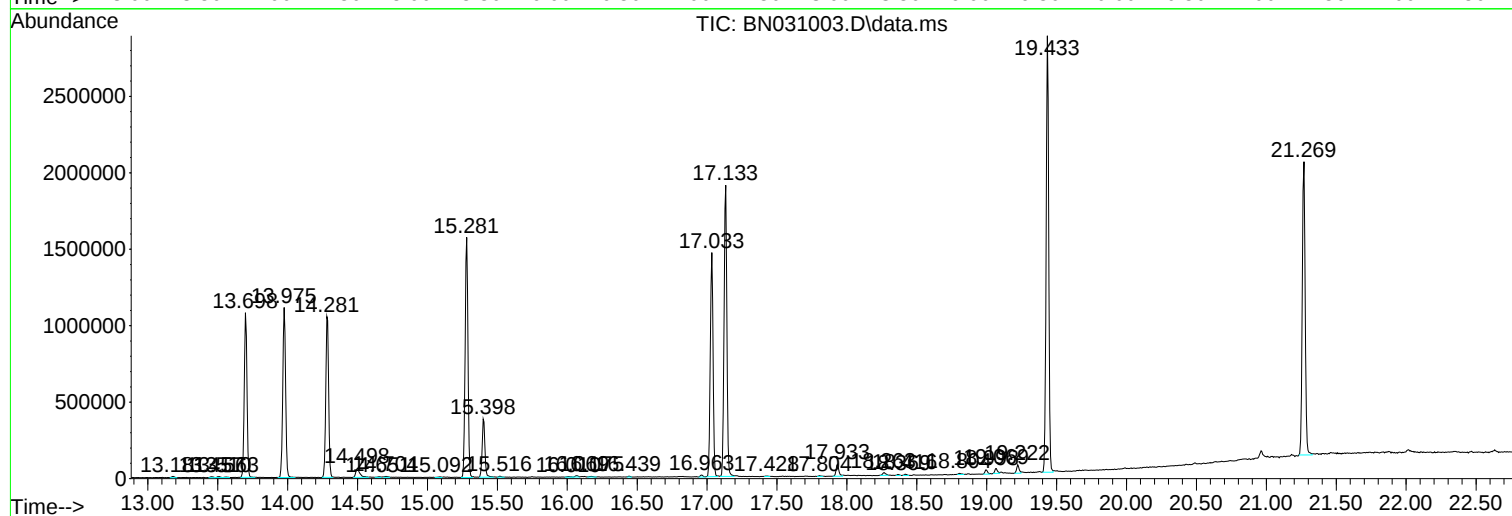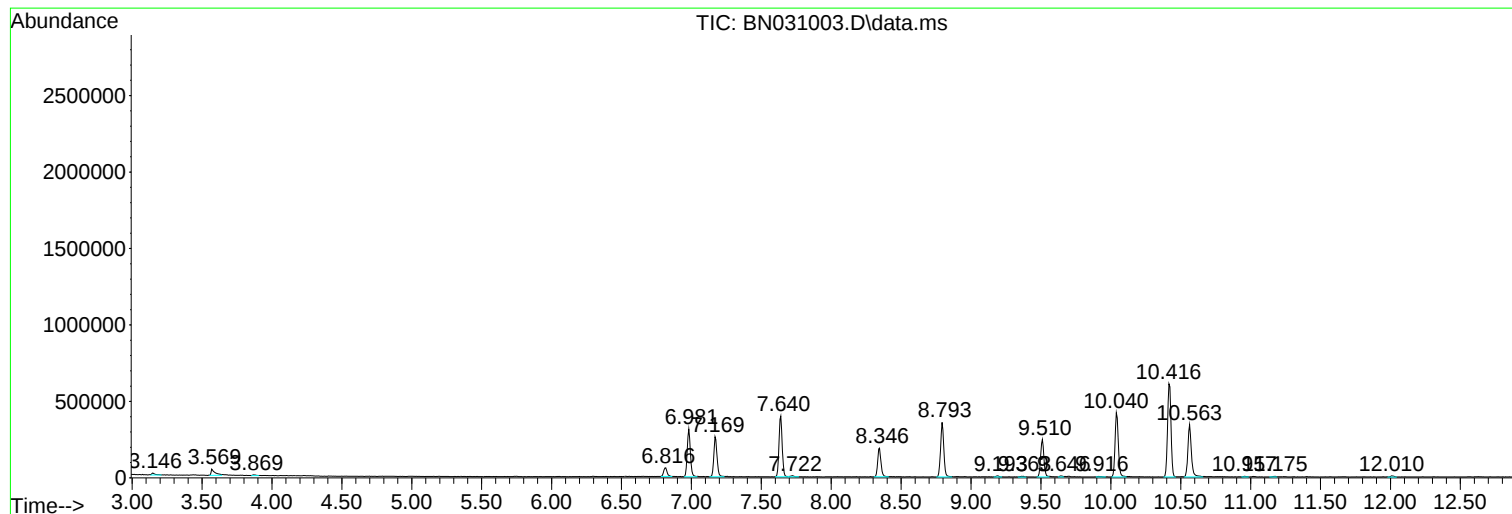

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031003.D
Acq On : 18 Apr 2024 09:55
Operator : MA/JU
Sample : P2077-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031003.D
Acq On : 18 Apr 2024 09:55
Operator : MA/JU
Sample : P2077-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc