

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031004.D
 Acq On : 18 Apr 2024 10:35
 Operator : MA/JU
 Sample : P2077-03
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031004.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	24	28	37	rVB	18405	31562	0.52%	0.072%
2	3.564	96	98	114	rBV	72278	143972	2.37%	0.330%
3	3.875	147	151	155	rBV4	5145	8573	0.14%	0.020%
4	6.810	645	650	661	rVB	78383	133963	2.21%	0.307%
5	6.981	672	679	689	rBV	426165	661397	10.90%	1.518%
6	7.169	704	711	721	rBV	361256	569947	9.39%	1.308%
7	7.640	780	791	800	rBV	543787	875118	14.42%	2.008%
8	7.722	800	805	814	rVB2	9197	19870	0.33%	0.046%
9	8.346	904	911	929	rBV	241577	399965	6.59%	0.918%
10	8.793	980	987	998	rBV	488606	798282	13.16%	1.832%
11	8.899	1003	1005	1009	rVV5	3763	6413	0.11%	0.015%
12	9.187	1050	1054	1060	rVB5	7888	12321	0.20%	0.028%
13	9.363	1081	1084	1092	rVB5	4429	6960	0.11%	0.016%
14	9.510	1098	1109	1121	rBV	353932	572053	9.43%	1.313%
15	9.646	1127	1132	1136	rBV2	8426	14800	0.24%	0.034%
16	9.699	1138	1141	1149	rVB4	4954	8209	0.14%	0.019%
17	9.916	1172	1178	1182	rBV7	5240	10592	0.17%	0.024%
18	10.040	1192	1199	1211	rBV	589034	963617	15.88%	2.211%
19	10.416	1256	1263	1273	rVB	863202	1396882	23.03%	3.205%
20	10.563	1281	1288	1303	rBV	518052	891945	14.70%	2.047%
21	10.963	1351	1356	1360	rBV4	4672	8303	0.14%	0.019%
22	11.175	1385	1392	1394	rBV8	3401	6417	0.11%	0.015%
23	12.016	1530	1535	1540	rBV2	10128	16105	0.27%	0.037%
24	13.181	1728	1733	1739	rBV3	10820	16275	0.27%	0.037%
25	13.457	1774	1780	1784	rBV3	8272	13017	0.21%	0.030%
26	13.510	1784	1789	1794	rVV2	10630	16818	0.28%	0.039%
27	13.557	1794	1797	1802	rVB4	4945	8203	0.14%	0.019%
28	13.698	1813	1821	1831	rBV	1476297	2002395	33.01%	4.595%
29	13.975	1861	1868	1883	rBV	1557010	2241440	36.95%	5.143%
30	14.287	1914	1921	1928	rBV	1381485	2052809	33.84%	4.711%
31	14.498	1951	1957	1968	rBV2	72032	139973	2.31%	0.321%
32	14.657	1979	1984	1987	rBV7	5518	9486	0.16%	0.022%
33	14.704	1987	1992	1997	rVB8	6245	10992	0.18%	0.025%
34	15.139	2064	2066	2072	rVB4	6869	8497	0.14%	0.019%
35	15.281	2083	2090	2099	rBV	2235644	3070947	50.62%	7.047%
36	15.404	2104	2111	2123	rVV	546421	750569	12.37%	1.722%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031004.D
 Acq On : 18 Apr 2024 10:35
 Operator : MA/JU
 Sample : P2077-03
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	15.522	2127	2131	2136	rBV4	10281	14635	0.24%	0.034%
38	16.010	2210	2214	2219	rBV6	10821	18309	0.30%	0.042%
39	16.069	2219	2224	2228	rVV4	12372	19546	0.32%	0.045%
40	16.104	2228	2230	2236	rVV5	4680	8987	0.15%	0.021%
41	16.169	2236	2241	2246	rVB5	8046	11194	0.18%	0.026%
42	16.580	2308	2311	2317	rVB5	4600	6458	0.11%	0.015%
43	16.804	2344	2349	2354	rBV5	12272	19063	0.31%	0.044%
44	16.963	2371	2376	2380	rBV4	13766	17119	0.28%	0.039%
45	17.033	2381	2388	2396	rBV	1890884	2701348	44.53%	6.199%
46	17.133	2398	2405	2416	rVV	2495574	3519221	58.01%	8.075%
47	17.539	2470	2474	2477	rBV	11427	14606	0.24%	0.034%
48	17.810	2516	2520	2527	rBV10	5829	10851	0.18%	0.025%
49	17.933	2536	2541	2549	rBV	71567	107276	1.77%	0.246%
50	18.227	2588	2591	2594	rBV3	10561	13696	0.23%	0.031%
51	18.263	2594	2597	2607	rVB2	20666	41331	0.68%	0.095%
52	18.363	2612	2614	2619	rVB5	8435	9912	0.16%	0.023%
53	18.422	2620	2624	2629	rVB5	8692	13874	0.23%	0.032%
54	18.804	2686	2689	2697	rVB6	9264	15627	0.26%	0.036%
55	18.869	2697	2700	2705	rBV3	8153	12178	0.20%	0.028%
56	18.998	2718	2722	2729	rVB3	35713	47505	0.78%	0.109%
57	19.063	2729	2733	2738	rBV	40458	62549	1.03%	0.144%
58	19.222	2756	2760	2768	rBV3	32392	43834	0.72%	0.101%
59	19.433	2790	2796	2804	rBV	3502797	4674865	77.06%	10.727%
60	20.963	3053	3056	3064	rBV3	55034	75381	1.24%	0.173%
61	21.268	3102	3108	3121	rBV2	2535806	3618142	59.64%	8.302%
62	23.974	3559	3568	3583	rBV	2613563	6066766	100.00%	13.921%
63	24.174	3593	3602	3616	rVB	1882215	4516412	74.45%	10.364%




Sum of corrected areas: 43579372

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031004.D
Acq On : 18 Apr 2024 10:35
Operator : MA/JU
Sample : P2077-03
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

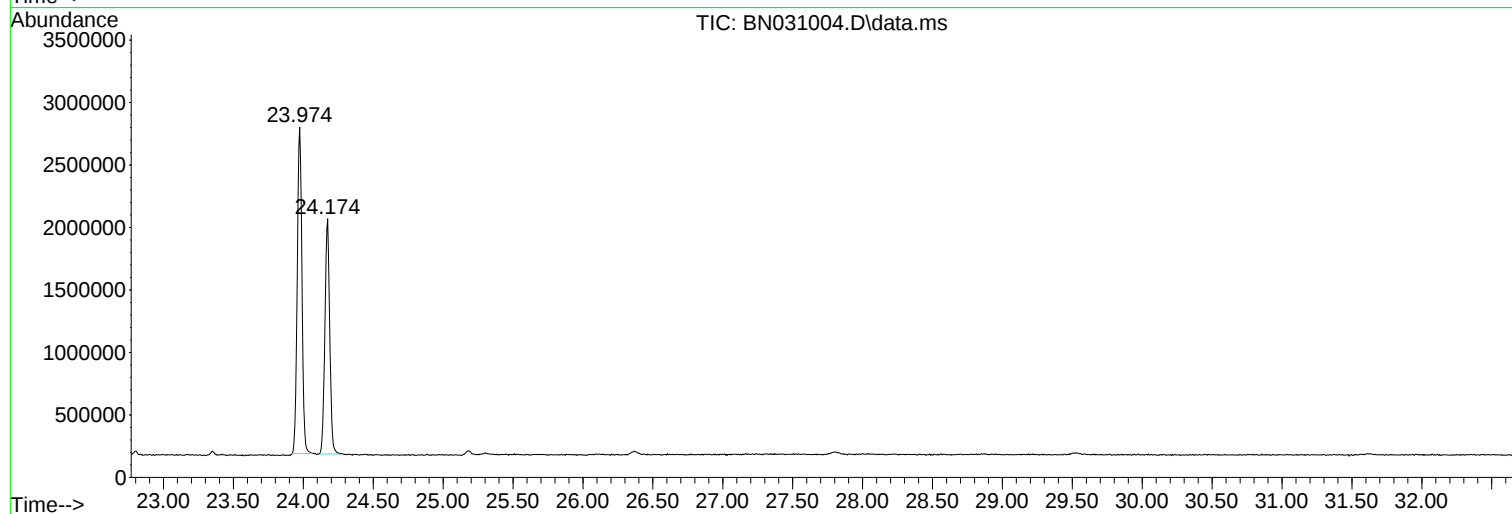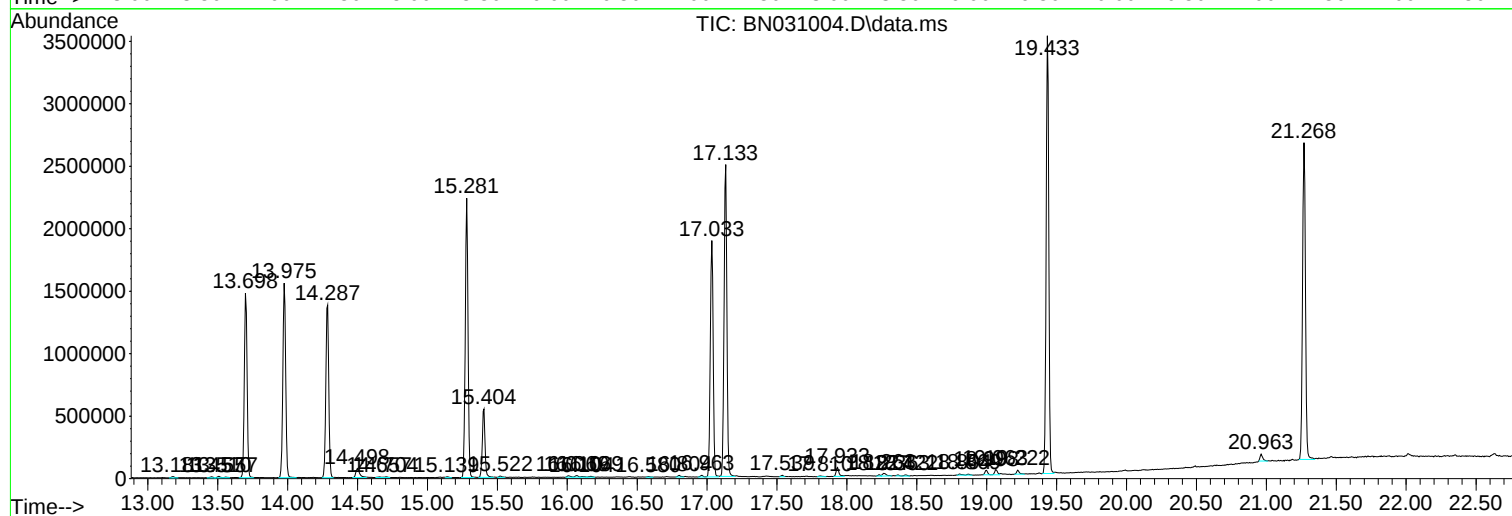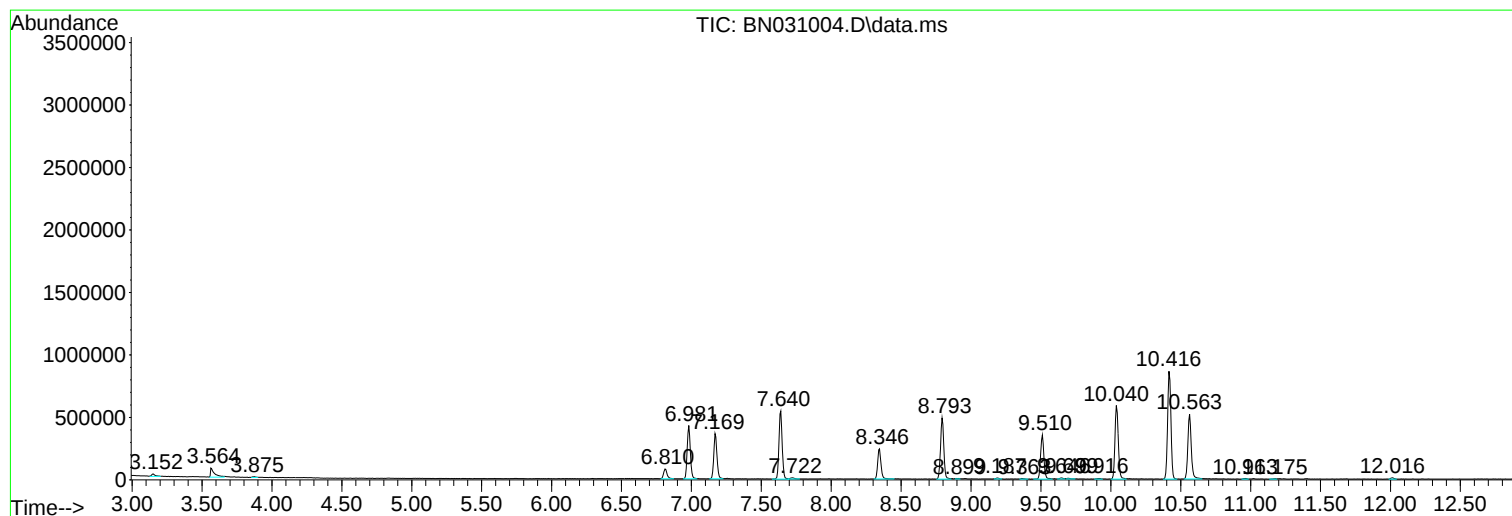

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031004.D
Acq On : 18 Apr 2024 10:35
Operator : MA/JU
Sample : P2077-03
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031004.D
Acq On : 18 Apr 2024 10:35
Operator : MA/JU
Sample : P2077-03
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc