

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031005.D
 Acq On : 18 Apr 2024 11:14
 Operator : MA/JU
 Sample : P2077-04
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031005.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	24	28	33	rBV	18913	26271	0.38%	0.057%
2	3.570	98	99	113	rBV	32981	70141	1.02%	0.151%
3	3.864	147	149	154	rVB3	6018	8860	0.13%	0.019%
4	6.811	645	650	658	rVV	95091	159312	2.31%	0.343%
5	6.981	671	679	692	rBV	474527	732901	10.63%	1.578%
6	7.169	702	711	724	rBV	399129	650564	9.44%	1.401%
7	7.640	784	791	800	rBV	552174	897490	13.02%	1.933%
8	7.722	800	805	813	rVB2	12890	22220	0.32%	0.048%
9	8.340	904	910	922	rBV	308544	503810	7.31%	1.085%
10	8.793	979	987	1001	rBV	545869	885902	12.85%	1.908%
11	8.893	1001	1004	1009	rVV5	5027	8632	0.13%	0.019%
12	8.963	1011	1016	1021	rVB6	4775	9379	0.14%	0.020%
13	9.187	1048	1054	1063	rVB4	16561	30323	0.44%	0.065%
14	9.369	1080	1085	1089	rBV4	4798	7688	0.11%	0.017%
15	9.511	1102	1109	1120	rBV	396205	638223	9.26%	1.374%
16	9.646	1126	1132	1137	rBV	10052	17036	0.25%	0.037%
17	9.699	1137	1141	1144	rVB4	4896	7411	0.11%	0.016%
18	9.905	1172	1176	1182	rBV5	5132	9504	0.14%	0.020%
19	10.040	1192	1199	1214	rBV	650998	1070833	15.53%	2.306%
20	10.416	1256	1263	1274	rBV	841988	1410686	20.46%	3.038%
21	10.563	1280	1288	1304	rBV	480757	843470	12.24%	1.816%
22	10.958	1350	1355	1361	rBV3	5778	9456	0.14%	0.020%
23	11.405	1423	1431	1436	rBV5	3570	7592	0.11%	0.016%
24	11.681	1470	1478	1482	rVB3	9315	14888	0.22%	0.032%
25	12.010	1526	1534	1540	rBV2	11560	18874	0.27%	0.041%
26	13.175	1726	1732	1737	rBV3	6534	10753	0.16%	0.023%
27	13.451	1775	1779	1784	rBV2	8886	13274	0.19%	0.029%
28	13.504	1784	1788	1792	rVV	12547	16594	0.24%	0.036%
29	13.557	1792	1797	1802	rVV5	4844	8286	0.12%	0.018%
30	13.699	1812	1821	1828	rBV	1514884	2101914	30.49%	4.527%
31	13.975	1860	1868	1876	rBV	1654478	2380047	34.53%	5.125%
32	14.281	1914	1920	1929	rBV	1430547	2097224	30.42%	4.516%
33	14.498	1951	1957	1978	rBV	93907	179695	2.61%	0.387%
34	14.704	1988	1992	1996	rVB5	5435	9125	0.13%	0.020%
35	15.281	2083	2090	2098	rBV	2321186	3221266	46.73%	6.937%
36	15.398	2104	2110	2122	rBV	643869	854725	12.40%	1.841%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031005.D
 Acq On : 18 Apr 2024 11:14
 Operator : MA/JU
 Sample : P2077-04
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	15.522	2127	2131	2135	rVB4	10046	13988	0.20%	0.030%
38	16.010	2211	2214	2218	rVB6	4559	7277	0.11%	0.016%
39	16.069	2218	2224	2228	rBV4	14290	22562	0.33%	0.049%
40	16.169	2237	2241	2247	rVV8	7439	13272	0.19%	0.029%
41	16.916	2364	2368	2371	rBV2	7785	9147	0.13%	0.020%
42	16.963	2372	2376	2380	rVB2	14852	18074	0.26%	0.039%
43	17.034	2382	2388	2394	rBV	1957130	2748875	39.88%	5.920%
44	17.134	2398	2405	2416	rBV2	2622909	3800925	55.14%	8.185%
45	17.422	2447	2454	2459	rBV8	5985	15381	0.22%	0.033%
46	17.710	2499	2503	2510	rVB	27971	38096	0.55%	0.082%
47	17.804	2515	2519	2523	rBV5	7092	11401	0.17%	0.025%
48	17.934	2536	2541	2548	rBV	62654	97669	1.42%	0.210%
49	18.269	2593	2598	2607	rVV3	27785	56016	0.81%	0.121%
50	18.369	2612	2615	2618	rVV5	9741	12739	0.18%	0.027%
51	18.416	2620	2623	2629	rVB7	8815	13747	0.20%	0.030%
52	18.804	2686	2689	2697	rBV8	12610	23991	0.35%	0.052%
53	18.998	2717	2722	2725	rBV3	39006	55497	0.81%	0.120%
54	19.063	2729	2733	2737	rBV	43006	57507	0.83%	0.124%
55	19.222	2756	2760	2766	rBV3	29663	38087	0.55%	0.082%
56	19.434	2790	2796	2804	rVV	3858183	5143033	74.61%	11.076%
57	20.963	3053	3056	3064	rBV4	46295	72051	1.05%	0.155%
58	21.269	3102	3108	3119	rBV	2633218	3687980	53.50%	7.942%
59	23.974	3558	3568	3586	rBV	2908348	6893649	100.00%	14.846%
60	24.169	3592	3601	3618	rVB	1866748	4630386	67.17%	9.972%




Sum of corrected areas: 46435719

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031005.D
Acq On : 18 Apr 2024 11:14
Operator : MA/JU
Sample : P2077-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

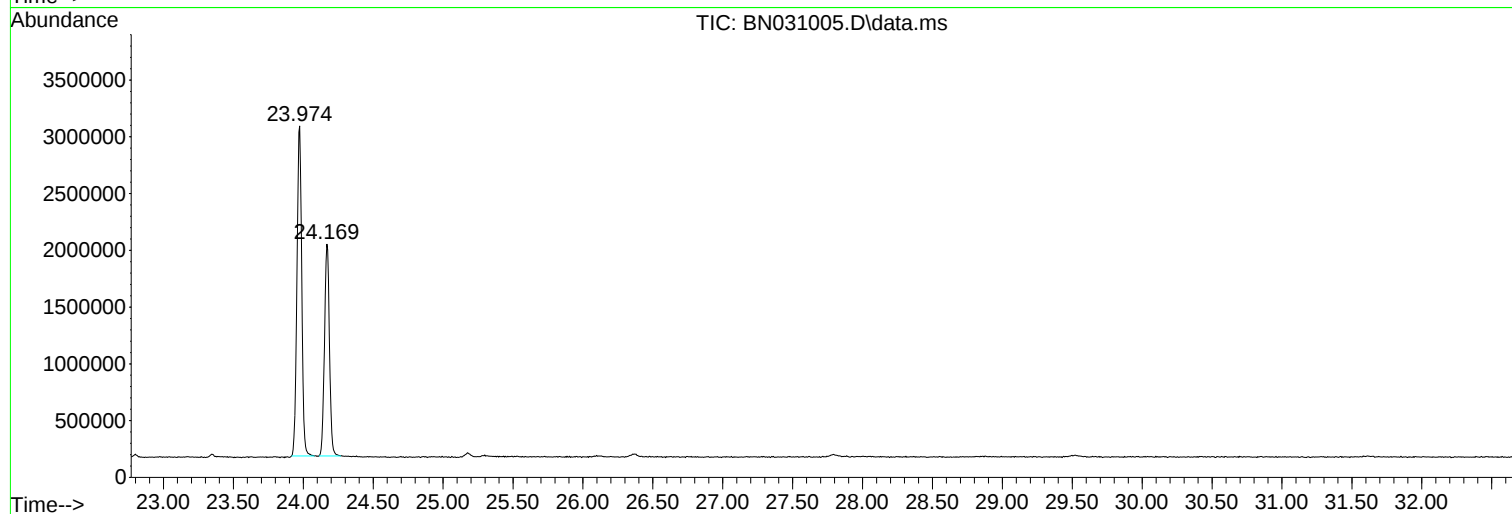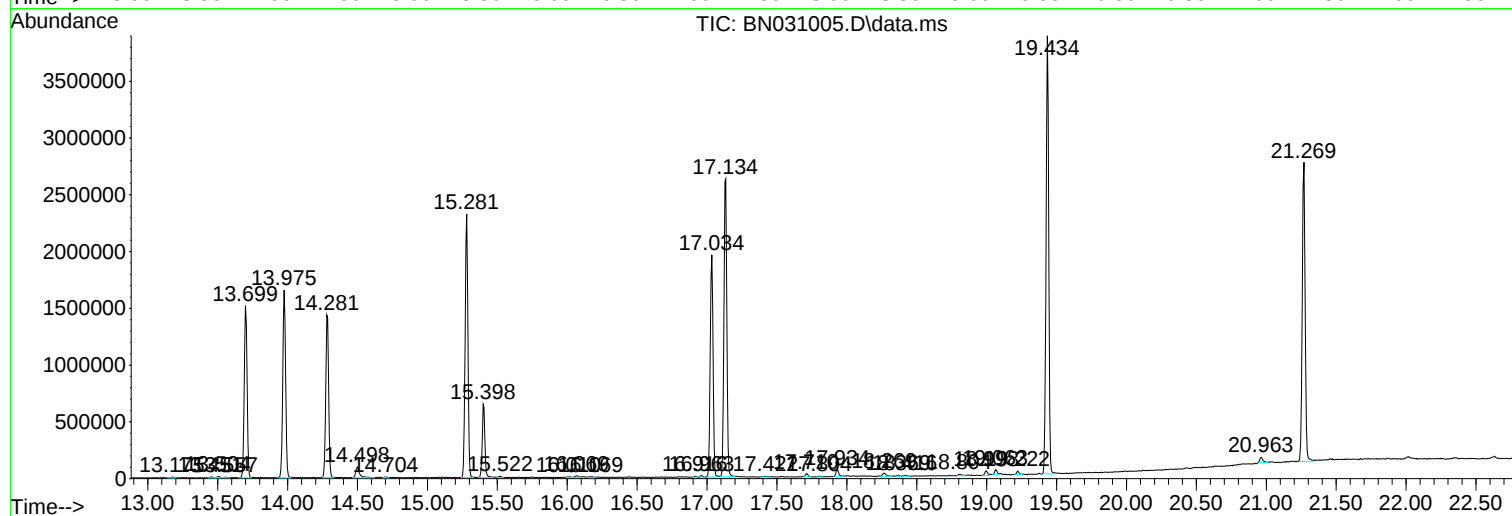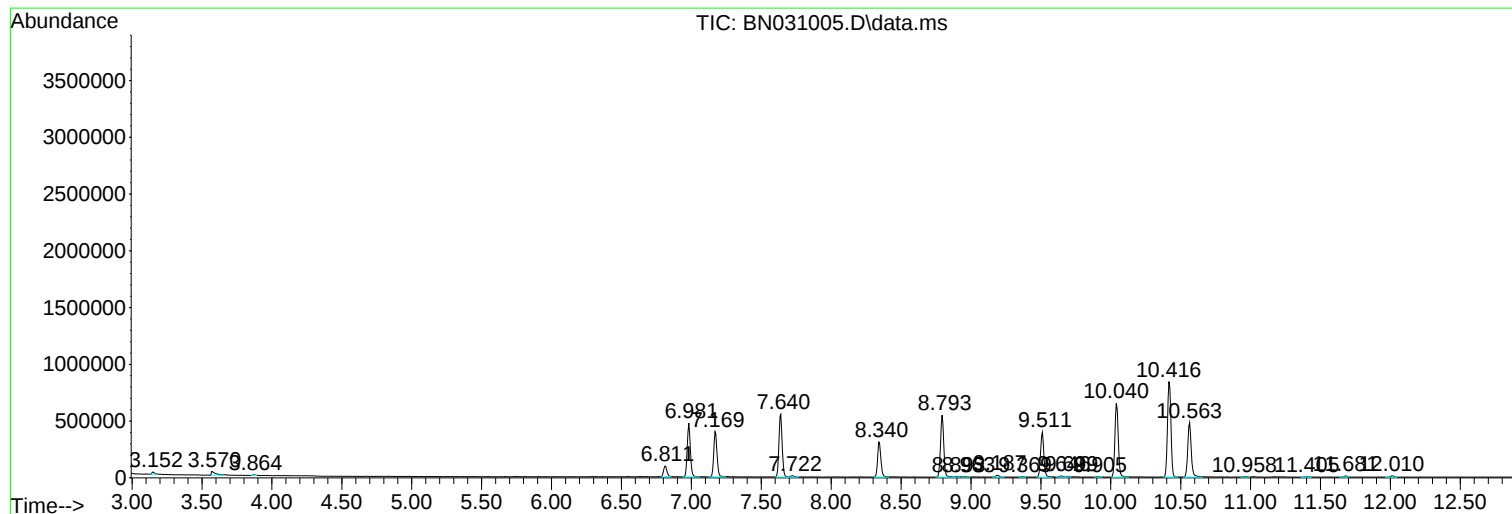

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031005.D
Acq On : 18 Apr 2024 11:14
Operator : MA/JU
Sample : P2077-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031005.D
Acq On : 18 Apr 2024 11:14
Operator : MA/JU
Sample : P2077-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc