

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031006.D
 Acq On : 18 Apr 2024 11:54
 Operator : MA/JU
 Sample : P2077-05
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	24	28	35	rVB	21804	32722	0.40%	0.058%
2	3.569	96	99	112	rBV	54838	108309	1.34%	0.193%
3	3.875	147	151	155	rVB4	8276	11150	0.14%	0.020%
4	6.810	645	650	661	rVB	133060	215314	2.66%	0.384%
5	6.981	673	679	694	rVB	561544	882437	10.89%	1.573%
6	7.169	704	711	723	rBV	512954	809839	9.99%	1.444%
7	7.640	784	791	799	rBV	675542	1091821	13.47%	1.946%
8	7.722	801	805	812	rVB2	9212	17004	0.21%	0.030%
9	8.340	904	910	924	rBV	412242	667523	8.24%	1.190%
10	8.793	980	987	1000	rBV	673183	1072855	13.24%	1.912%
11	9.193	1047	1055	1060	rBV2	27738	44255	0.55%	0.079%
12	9.510	1101	1109	1121	rBV	486623	789723	9.74%	1.408%
13	9.646	1127	1132	1136	rBV2	10820	17094	0.21%	0.030%
14	9.698	1136	1141	1147	rVB5	7521	12211	0.15%	0.022%
15	9.904	1168	1176	1185	rBV9	3641	8803	0.11%	0.016%
16	10.040	1192	1199	1211	rBV	809406	1319524	16.28%	2.352%
17	10.416	1256	1263	1272	rBV	1058439	1724681	21.28%	3.074%
18	10.563	1280	1288	1301	rBV	599276	1050725	12.96%	1.873%
19	10.963	1349	1356	1361	rBV3	6811	11636	0.14%	0.021%
20	11.016	1361	1365	1374	rVB5	5166	8799	0.11%	0.016%
21	11.404	1425	1431	1437	rVB4	5034	8836	0.11%	0.016%
22	11.681	1472	1478	1483	rVB2	11562	16365	0.20%	0.029%
23	12.016	1529	1535	1543	rVB2	15079	25568	0.32%	0.046%
24	13.181	1728	1733	1739	rVB2	13517	19797	0.24%	0.035%
25	13.457	1774	1780	1784	rBV2	8705	13762	0.17%	0.025%
26	13.504	1784	1788	1794	rVV	13399	19670	0.24%	0.035%
27	13.698	1813	1821	1830	rBV	1874714	2536615	31.30%	4.522%
28	13.975	1861	1868	1880	rBV2	1998465	2909027	35.89%	5.186%
29	14.286	1914	1921	1929	rBV	1716930	2503718	30.89%	4.463%
30	14.498	1947	1957	1972	rBV	159996	309828	3.82%	0.552%
31	14.704	1990	1992	1997	rVB5	7960	10034	0.12%	0.018%
32	15.281	2083	2090	2098	rBV	2728569	3854985	47.56%	6.872%
33	15.404	2104	2111	2123	rBV	806901	1125362	13.89%	2.006%
34	15.522	2127	2131	2136	rVB2	11724	16816	0.21%	0.030%
35	16.016	2210	2215	2218	rBV6	6030	9843	0.12%	0.018%
36	16.069	2218	2224	2227	rVV3	16361	26453	0.33%	0.047%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031006.D
 Acq On : 18 Apr 2024 11:54
 Operator : MA/JU
 Sample : P2077-05
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	16.110	2227	2231	2233	rVV4	5895	9600	0.12%	0.017%
38	16.169	2237	2241	2246	rVB7	9297	14485	0.18%	0.026%
39	16.439	2284	2287	2291	rBV3	7840	9726	0.12%	0.017%
40	16.963	2373	2376	2380	rVB6	9151	10564	0.13%	0.019%
41	17.033	2381	2388	2394	rVV	2291832	3236903	39.94%	5.770%
42	17.133	2398	2405	2415	rVV	3409700	4738966	58.47%	8.447%
43	17.210	2416	2418	2423	rVB3	10211	13160	0.16%	0.023%
44	17.933	2536	2541	2552	rBV	191048	289747	3.57%	0.516%
45	18.269	2593	2598	2609	rVB	34596	64220	0.79%	0.114%
46	18.416	2620	2623	2630	rVB6	10130	15152	0.19%	0.027%
47	18.998	2718	2722	2728	rBV2	49513	66798	0.82%	0.119%
48	19.069	2729	2734	2738	rBV	59950	94908	1.17%	0.169%
49	19.222	2756	2760	2768	rBV	100668	140103	1.73%	0.250%
50	19.433	2790	2796	2809	rBV	4486334	6285568	77.55%	11.204%
51	20.963	3052	3056	3065	rBV2	105410	192229	2.37%	0.343%
52	21.268	3102	3108	3117	rBV	3073667	4279487	52.80%	7.628%
53	23.974	3558	3568	3584	rBV	3351236	8104814	100.00%	14.447%
54	24.174	3593	3602	3615	rVB	2182687	5229611	64.52%	9.322%




Sum of corrected areas: 56099145

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031006.D
Acq On : 18 Apr 2024 11:54
Operator : MA/JU
Sample : P2077-05
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

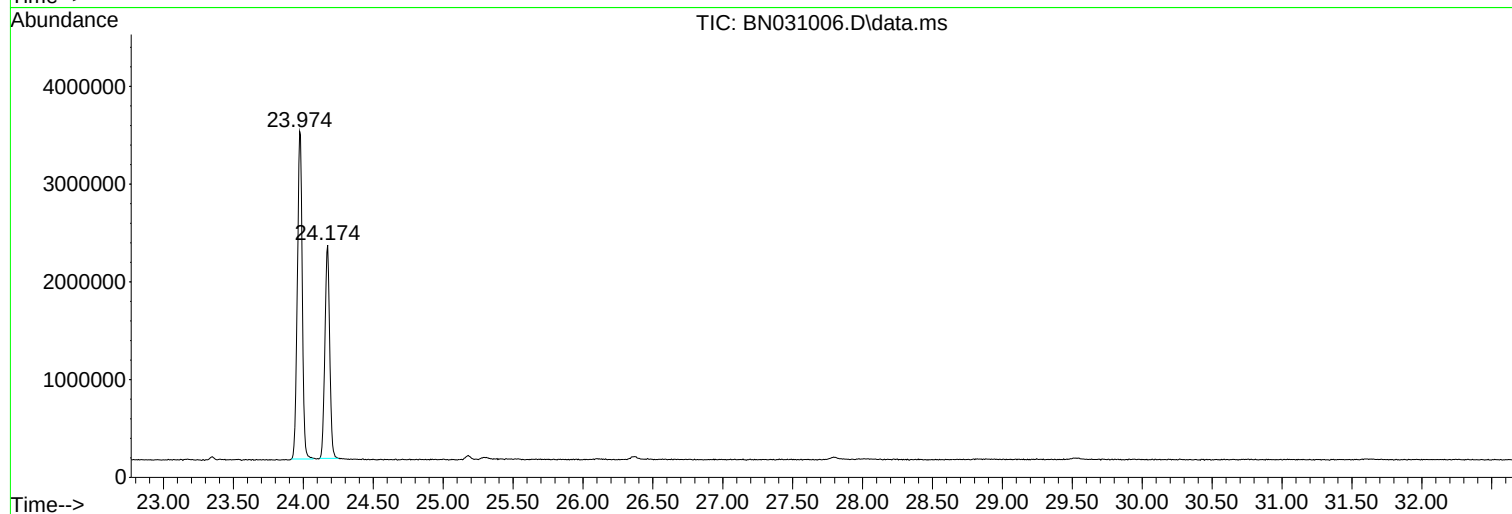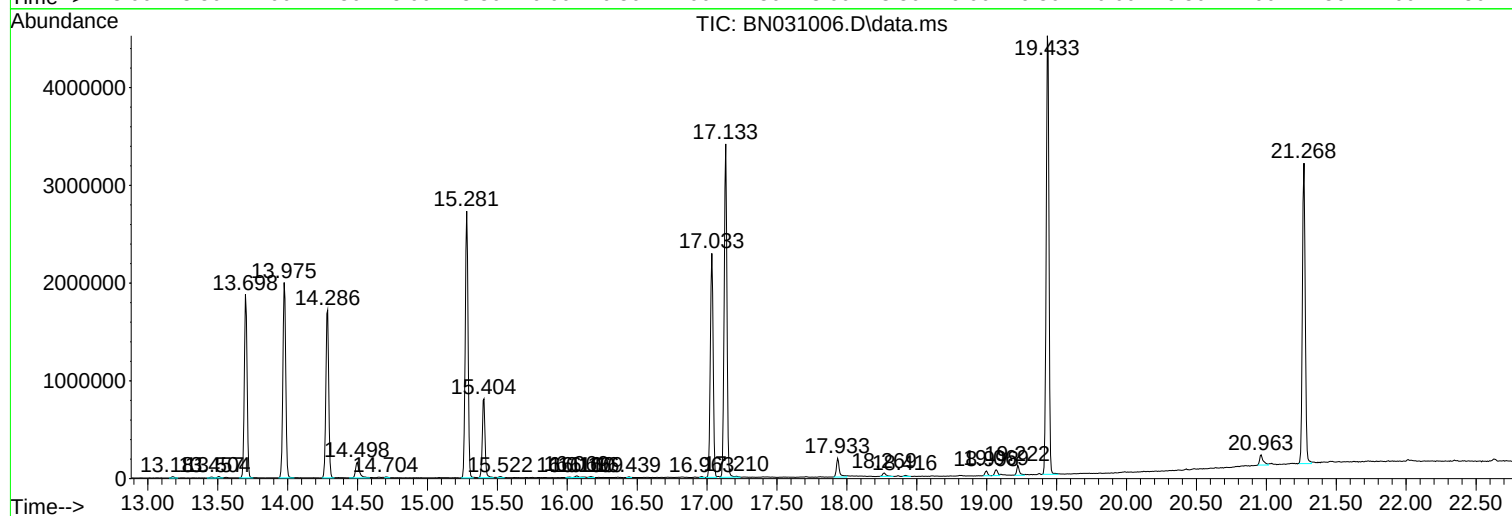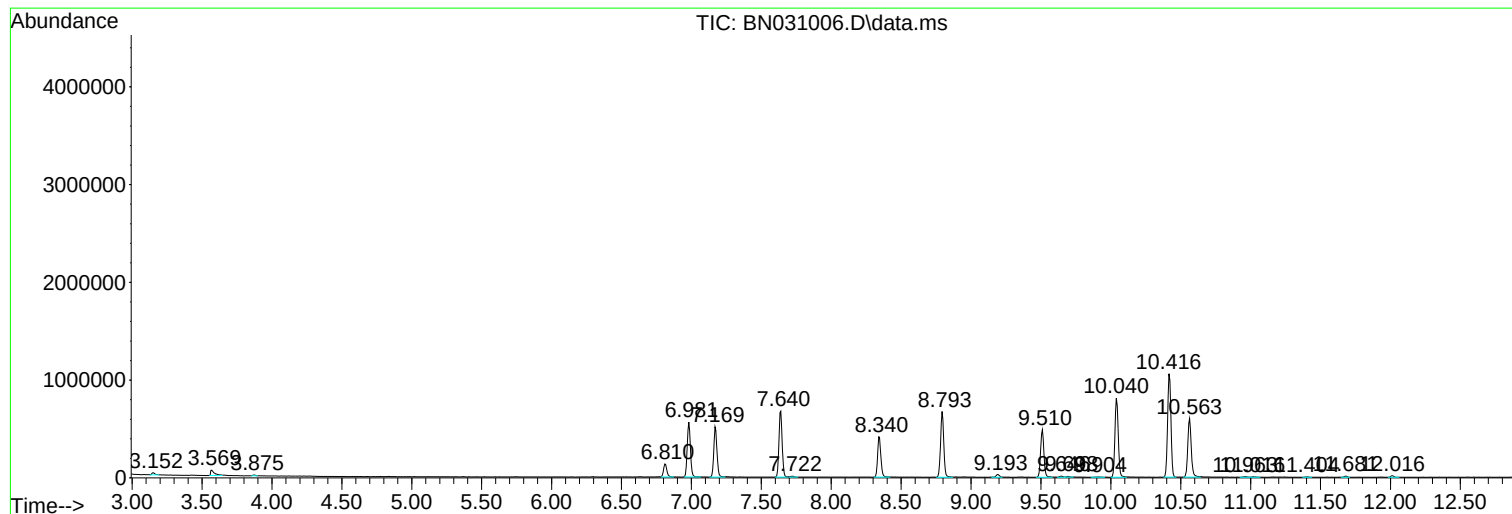

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031006.D
Acq On : 18 Apr 2024 11:54
Operator : MA/JU
Sample : P2077-05
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031006.D
Acq On : 18 Apr 2024 11:54
Operator : MA/JU
Sample : P2077-05
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc