

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031008.D
 Acq On : 18 Apr 2024 13:52
 Operator : MA/JU
 Sample : P2060-04
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1D01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031008.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	33	rBV	13357	18138	0.33%	0.055%
2	3.569	97	99	109	rBV	44421	87253	1.60%	0.264%
3	6.810	645	650	662	rVB	93105	151970	2.79%	0.461%
4	6.981	673	679	689	rVB	366761	576269	10.58%	1.747%
5	7.169	705	711	722	rBV	319995	525165	9.64%	1.592%
6	7.640	783	791	797	rBV	306625	492699	9.04%	1.493%
7	7.698	797	801	807	rVB	59576	91548	1.68%	0.277%
8	8.345	904	911	920	rBV	282256	463813	8.51%	1.406%
9	8.463	927	931	935	rVB4	7336	10198	0.19%	0.031%
10	8.792	981	987	1002	rBV	429179	685570	12.59%	2.078%
11	9.510	1102	1109	1120	rBV	292963	479638	8.81%	1.454%
12	9.922	1174	1179	1183	rVB3	5095	8457	0.16%	0.026%
13	10.039	1193	1199	1211	rBV	493636	819629	15.05%	2.484%
14	10.204	1222	1227	1233	rVB8	4554	8192	0.15%	0.025%
15	10.416	1256	1263	1270	rBV	469333	791907	14.54%	2.400%
16	10.563	1281	1288	1301	rBV	195032	338568	6.22%	1.026%
17	12.010	1530	1534	1541	rVB	8723	13718	0.25%	0.042%
18	12.886	1679	1683	1688	rBV3	4106	6247	0.11%	0.019%
19	13.122	1715	1723	1728	rBV	8357	13734	0.25%	0.042%
20	13.181	1728	1733	1738	rVB2	6693	9716	0.18%	0.029%
21	13.698	1814	1821	1834	rBV	1222205	1663155	30.53%	5.041%
22	13.975	1861	1868	1877	rBV	1334644	1912543	35.11%	5.797%
23	14.280	1914	1920	1930	rBV	814308	1195419	21.95%	3.623%
24	14.498	1952	1957	1970	rBV2	73092	151828	2.79%	0.460%
25	14.963	2031	2036	2041	rBV2	8626	13733	0.25%	0.042%
26	15.092	2054	2058	2067	rVB5	10400	18731	0.34%	0.057%
27	15.280	2083	2090	2099	rBV	1867774	2600721	47.74%	7.883%
28	15.398	2105	2110	2119	rBV	422807	596123	10.94%	1.807%
29	15.516	2127	2130	2134	rVB4	7577	10205	0.19%	0.031%
30	16.063	2220	2223	2228	rBV4	5042	6908	0.13%	0.021%
31	17.033	2382	2388	2397	rVB	1118742	1540912	28.29%	4.671%
32	17.133	2398	2405	2418	rBV	2274212	3186143	58.49%	9.657%
33	17.327	2434	2438	2441	rVB2	6802	9048	0.17%	0.027%
34	17.421	2450	2454	2458	rBV5	3206	5704	0.10%	0.017%
35	17.704	2498	2502	2507	rBV	106880	137078	2.52%	0.415%
36	17.933	2536	2541	2547	rBV2	23680	34233	0.63%	0.104%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031008.D
Acq On : 18 Apr 2024 13:52
Operator : MA/JU
Sample : P2060-04
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1D01

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	18.010	2551	2554	2562	rVB2	7845	14567	0.27%	0.044%
38	18.368	2612	2615	2618	rBV4	8801	9461	0.17%	0.029%
39	18.804	2685	2689	2691	rBV3	3943	5823	0.11%	0.018%
40	18.992	2718	2721	2728	rVB2	23087	31897	0.59%	0.097%
41	19.068	2730	2734	2739	rVV	21779	29963	0.55%	0.091%
42	19.221	2756	2760	2767	rBV4	24172	33669	0.62%	0.102%
43	19.433	2790	2796	2804	rBV	3104498	4042183	74.21%	12.252%
44	21.268	3102	3108	3116	rBV2	1494060	2067192	37.95%	6.266%
45	23.974	3559	3568	3585	rBV2	2388665	5447217	100.00%	16.511%
46	24.168	3593	3601	3616	rVB2	1107464	2634675	48.37%	7.986%




Sum of corrected areas: 32991560

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031008.D
Acq On : 18 Apr 2024 13:52
Operator : MA/JU
Sample : P2060-04
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1D01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

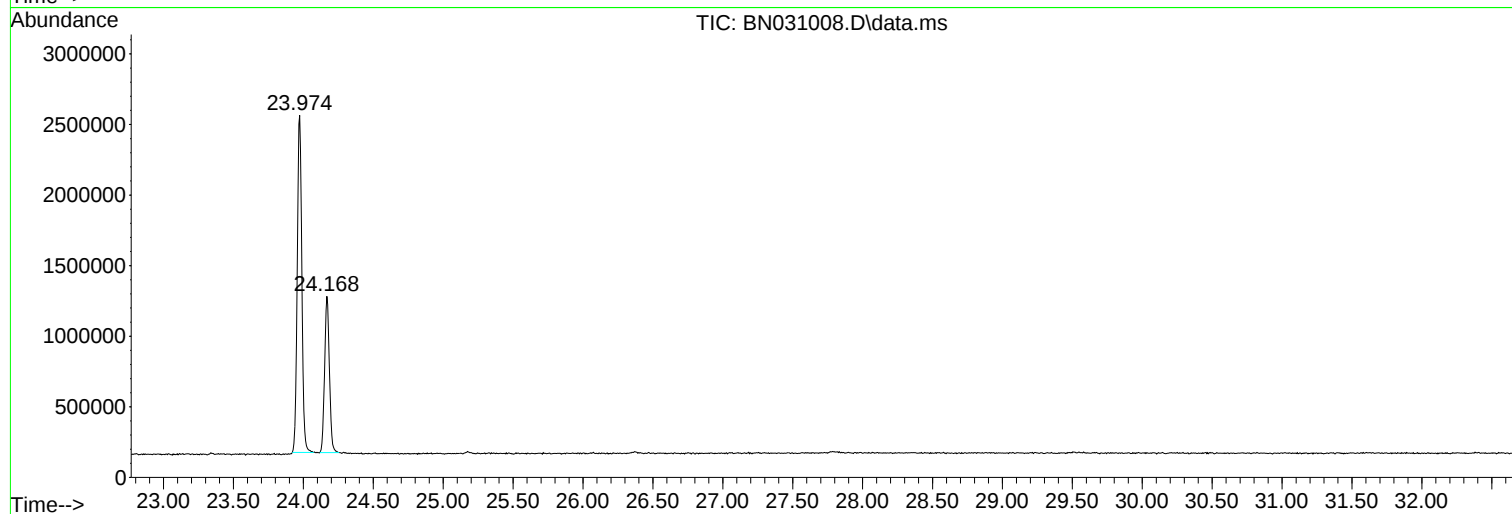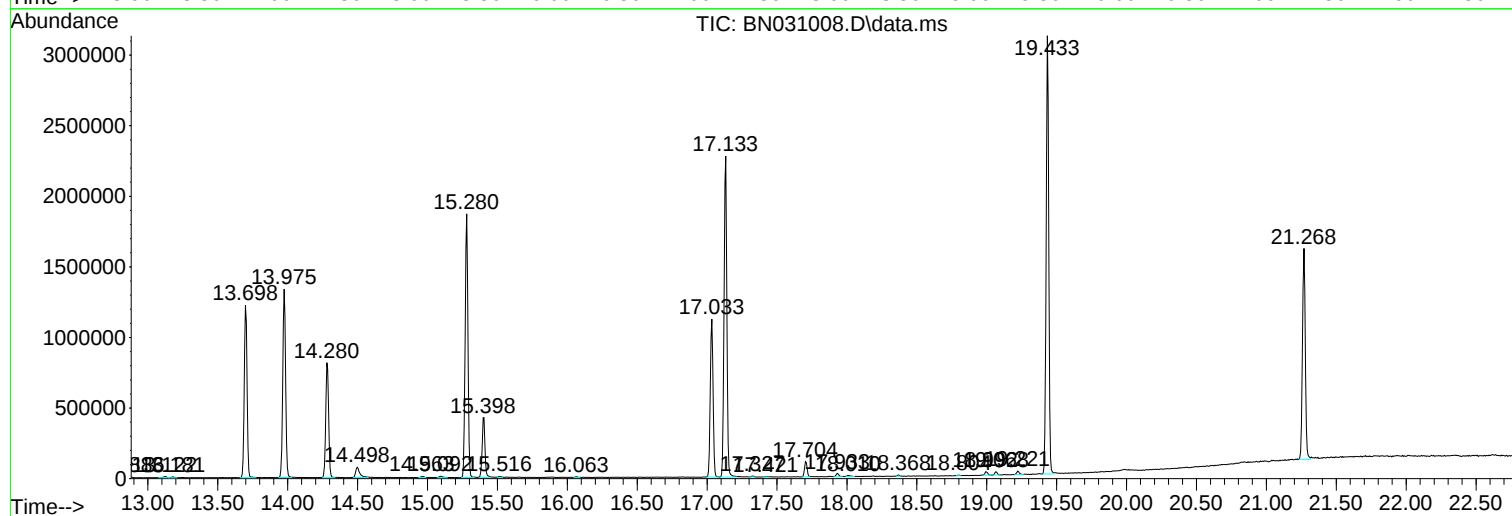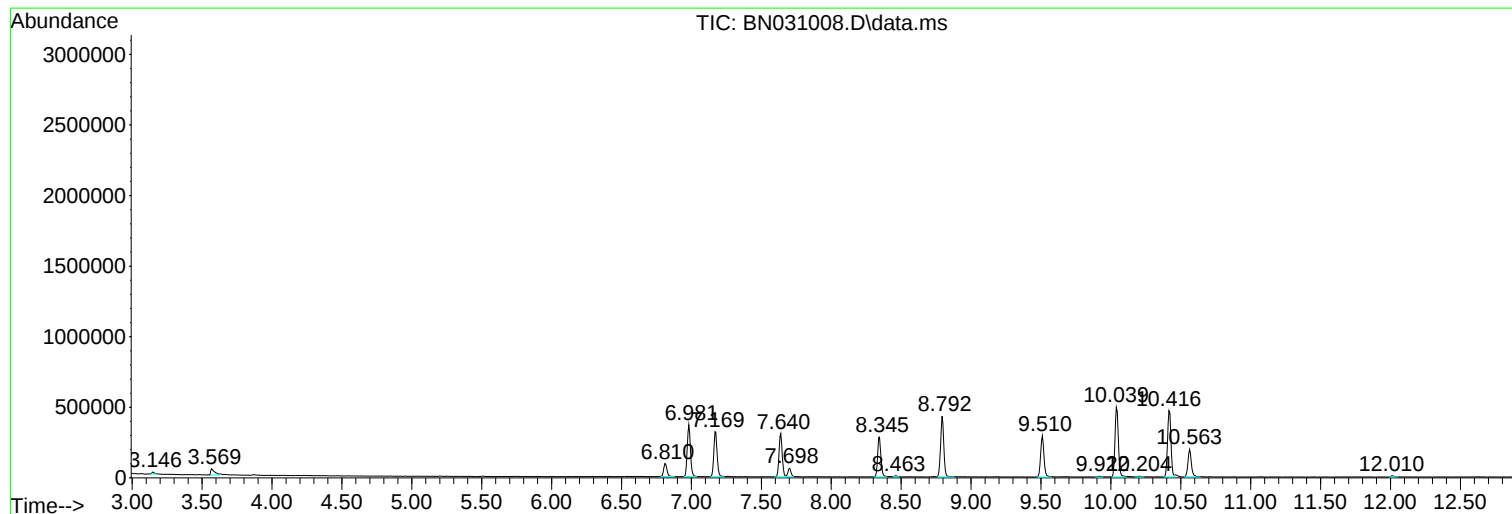

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031008.D
Acq On : 18 Apr 2024 13:52
Operator : MA/JU
Sample : P2060-04
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1D01










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Hexanol, 2-ethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.698	3.72 ng/ul	91548	1,4-Dichlorobenzene-d4	7.640

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	83
2	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	83
3	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	80
4	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	72
5	Heptane, 1,1'-oxybis-			214	C14H30O	000629-64-1	53

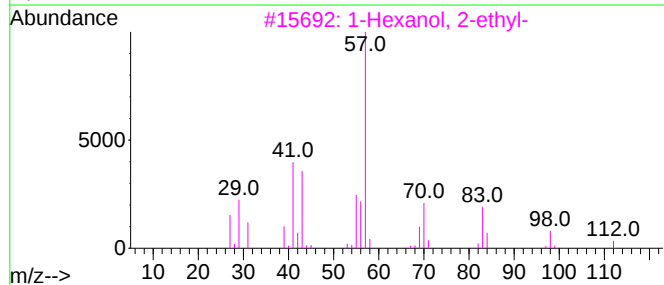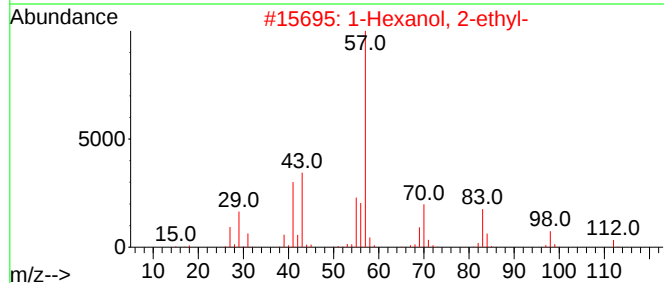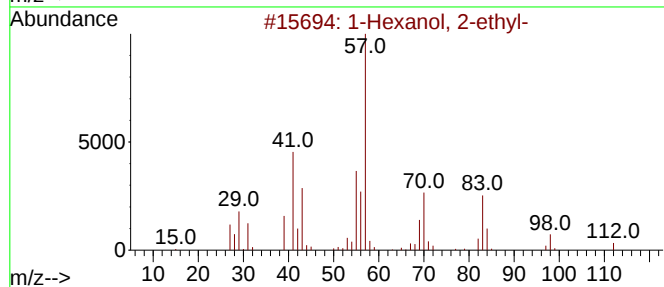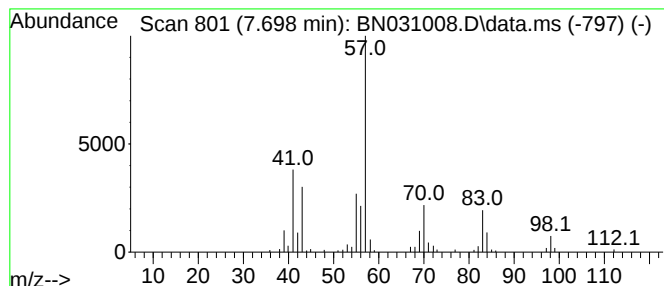

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031008.D
Acq On : 18 Apr 2024 13:52
Operator : MA/JU
Sample : P2060-04
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1D01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexanol, 2-et...	7.698	3.7	ng/ul	91548	1	7.640	492699	20.0