

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031013.D
 Acq On : 18 Apr 2024 17:55
 Operator : MA/JU
 Sample : PB160322BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK322

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031013.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	23	27	33	rBV	26868	37783	0.73%	0.094%
2	3.552	94	96	123	rBV	339353	646655	12.54%	1.605%
3	3.875	147	151	156	rVB4	5126	8687	0.17%	0.022%
4	6.810	644	650	665	rVB	516624	801490	15.54%	1.989%
5	6.981	673	679	691	rVB	449826	692830	13.43%	1.719%
6	7.169	704	711	725	rVB	506391	802411	15.56%	1.991%
7	7.634	784	790	798	rBV	401949	648364	12.57%	1.609%
8	8.340	904	910	923	rBV	661545	1050385	20.36%	2.607%
9	8.793	980	987	999	rBV	518912	816904	15.84%	2.027%
10	9.510	1102	1109	1121	rBV	384042	612171	11.87%	1.519%
11	10.040	1192	1199	1213	rBV	663384	1073088	20.81%	2.663%
12	10.416	1254	1263	1271	rBV	659462	1067447	20.70%	2.649%
13	10.563	1279	1288	1298	rBV	724742	1220965	23.67%	3.030%
14	12.016	1529	1535	1540	rBV2	11707	18526	0.36%	0.046%
15	13.175	1727	1732	1740	rBV	10647	17716	0.34%	0.044%
16	13.698	1814	1821	1834	rBV	1459303	1944782	37.71%	4.826%
17	13.975	1861	1868	1881	rBV	1603330	2216473	42.97%	5.501%
18	14.281	1914	1920	1933	rBV	1066162	1577147	30.58%	3.914%
19	14.492	1949	1956	1976	rBV	586266	949650	18.41%	2.357%
20	15.281	2083	2090	2101	rBV	2070924	2878354	55.81%	7.143%
21	15.404	2104	2111	2124	rVV	500464	714666	13.86%	1.774%
22	15.516	2128	2130	2135	rVB3	8186	10440	0.20%	0.026%
23	16.069	2219	2224	2227	rBV7	4965	8155	0.16%	0.020%
24	17.033	2382	2388	2398	rBV	1495938	2040567	39.56%	5.064%
25	17.133	2398	2405	2418	rBV	2316498	3289289	63.77%	8.163%
26	18.998	2718	2722	2727	rBV	25750	33397	0.65%	0.083%
27	19.069	2730	2734	2740	rVV2	21257	30712	0.60%	0.076%
28	19.433	2790	2796	2806	rBV	3254151	4167132	80.79%	10.342%
29	21.269	3102	3108	3122	rBV	1800873	2599703	50.40%	6.452%
30	23.968	3559	3567	3583	rVB2	2324486	5157819	100.00%	12.800%
31	24.168	3593	3601	3617	rVB	1329386	3160360	61.27%	7.843%




Sum of corrected areas: 40294068

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031013.D
Acq On : 18 Apr 2024 17:55
Operator : MA/JU
Sample : PB160322BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK322

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

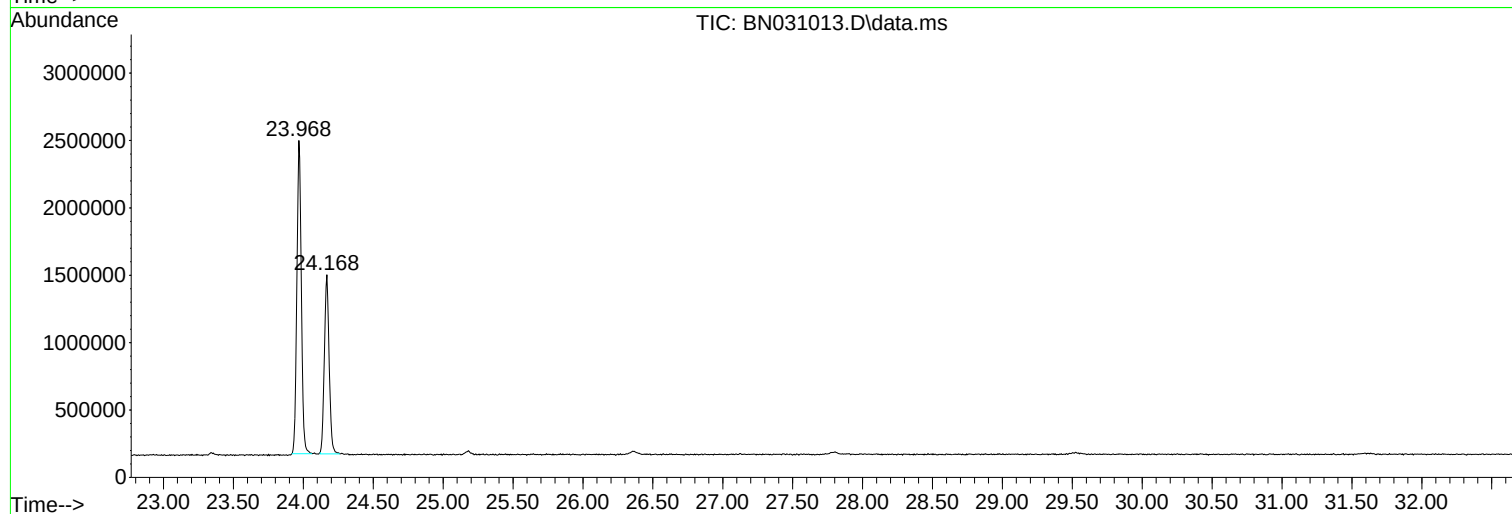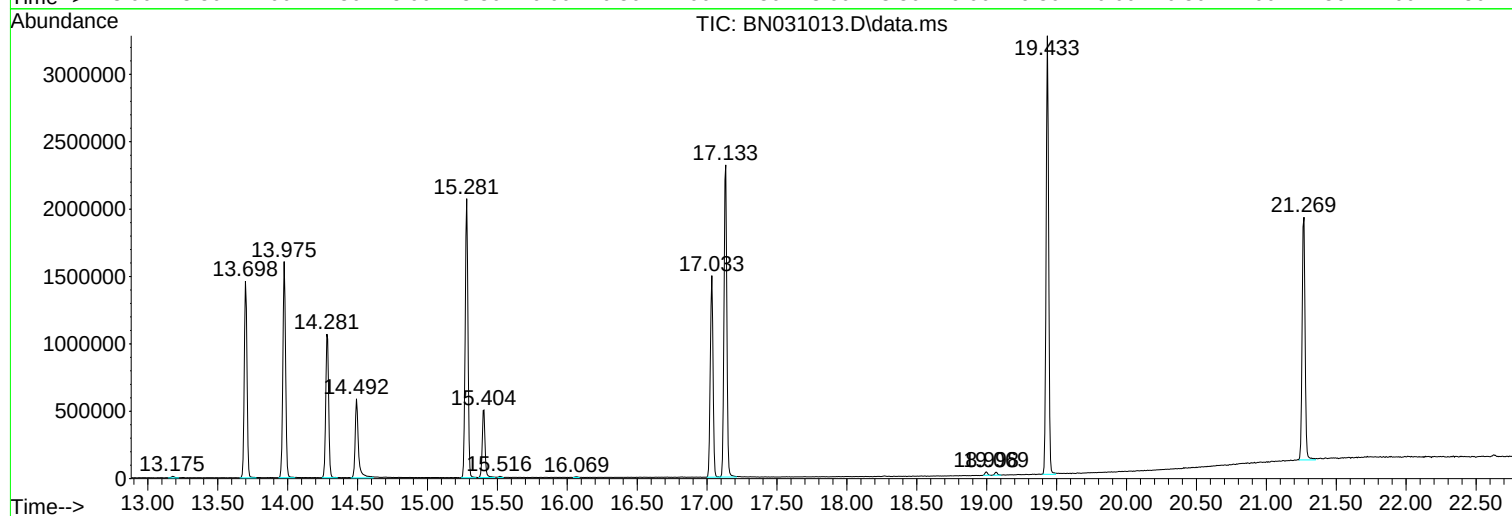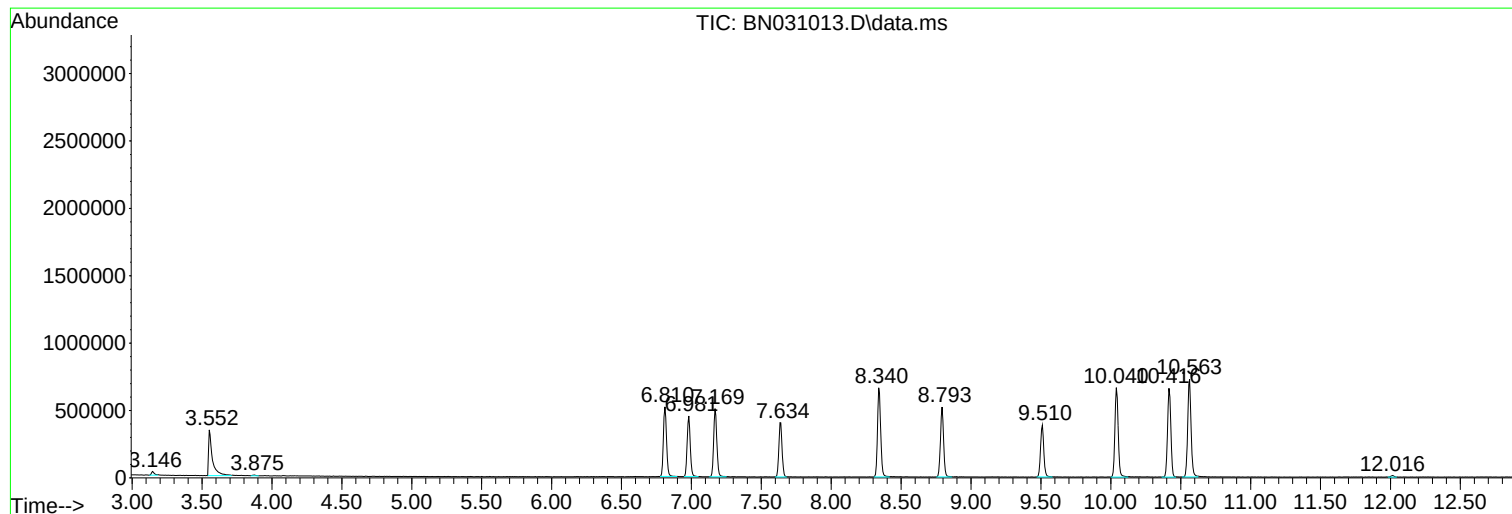

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031013.D
Acq On : 18 Apr 2024 17:55
Operator : MA/JU
Sample : PB160322BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK322

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031013.D
Acq On : 18 Apr 2024 17:55
Operator : MA/JU
Sample : PB160322BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK322

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------