

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031014.D
 Acq On : 18 Apr 2024 18:35
 Operator : MA/JU
 Sample : PB160260TB 10X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLEB260

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	23	27	35	rBV	29931	44062	0.89%	0.106%
2	3.552	94	96	120	rBV	372165	677165	13.61%	1.632%
3	3.869	146	150	155	rBV4	5288	9228	0.19%	0.022%
4	6.810	644	650	668	rVB	547594	851361	17.11%	2.051%
5	6.981	673	679	689	rVB	475143	734424	14.76%	1.770%
6	7.169	703	711	723	rBV	543174	847786	17.04%	2.043%
7	7.640	783	791	800	rBV	427802	697981	14.03%	1.682%
8	8.340	904	910	922	rBV	695127	1107239	22.25%	2.668%
9	8.793	980	987	997	rBV	543343	874078	17.57%	2.106%
10	9.510	1102	1109	1122	rBV	402111	651821	13.10%	1.571%
11	10.040	1192	1199	1214	rBV	693128	1130103	22.71%	2.723%
12	10.416	1256	1263	1274	rBV	677628	1113241	22.38%	2.682%
13	10.563	1279	1288	1308	rBV	757690	1297485	26.08%	3.126%
14	12.016	1528	1535	1543	rBV2	11872	21381	0.43%	0.052%
15	13.175	1729	1732	1739	rBV5	6801	10984	0.22%	0.026%
16	13.698	1814	1821	1828	rBV	1541006	2057905	41.36%	4.959%
17	13.975	1861	1868	1878	rBV	1612651	2336116	46.95%	5.629%
18	14.281	1914	1920	1932	rBV	1131187	1654571	33.26%	3.987%
19	14.492	1950	1956	1983	rBV	625998	993765	19.97%	2.394%
20	15.281	2083	2090	2104	rBV	2200273	3033418	60.97%	7.309%
21	15.404	2104	2111	2124	rVV	551308	753822	15.15%	1.816%
22	15.522	2126	2131	2137	rVB5	9464	15768	0.32%	0.038%
23	16.063	2217	2223	2227	rBV6	5585	8672	0.17%	0.021%
24	17.033	2381	2388	2398	rBV	1507726	2139619	43.01%	5.155%
25	17.133	2398	2405	2420	rVV	2421759	3399099	68.32%	8.190%
26	18.998	2718	2722	2728	rBV2	27374	36863	0.74%	0.089%
27	19.069	2730	2734	2738	rVV	23366	29908	0.60%	0.072%
28	19.433	2790	2796	2808	rBV	3304626	4325643	86.94%	10.423%
29	21.268	3102	3108	3121	rBV2	1827519	2627970	52.82%	6.332%
30	23.974	3559	3568	3580	rBV	2225927	4975251	100.00%	11.988%
31	24.162	3592	3600	3613	rBV	1268478	3045409	61.21%	7.338%




Sum of corrected areas: 41502138

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031014.D
Acq On : 18 Apr 2024 18:35
Operator : MA/JU
Sample : PB160260TB 10X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

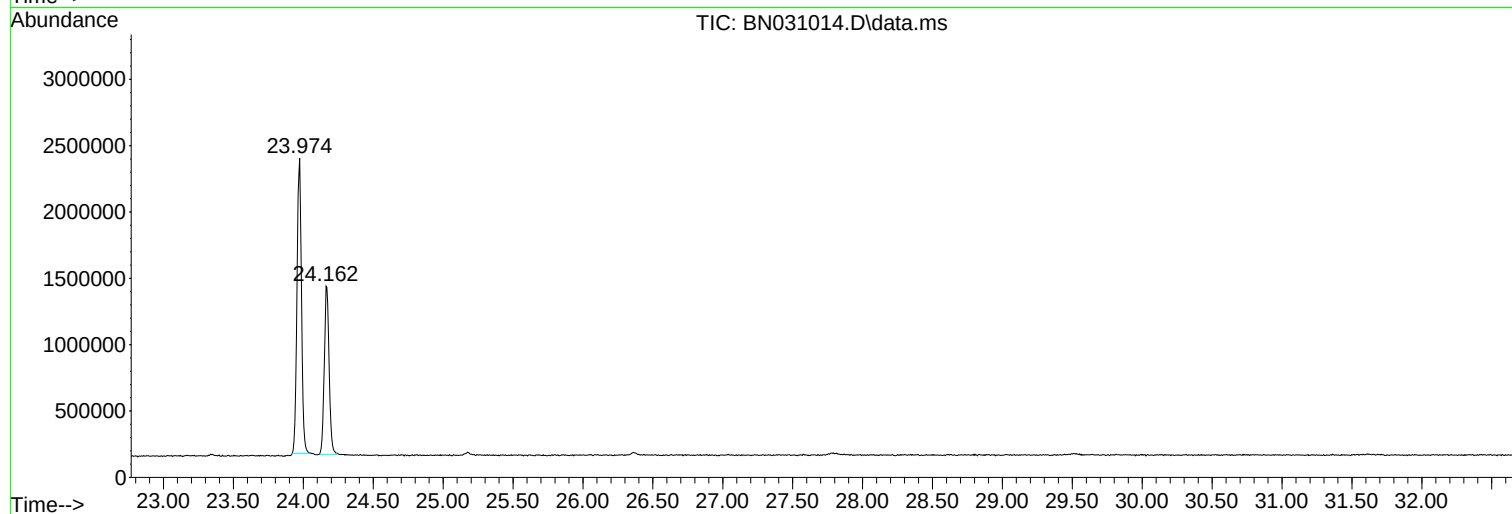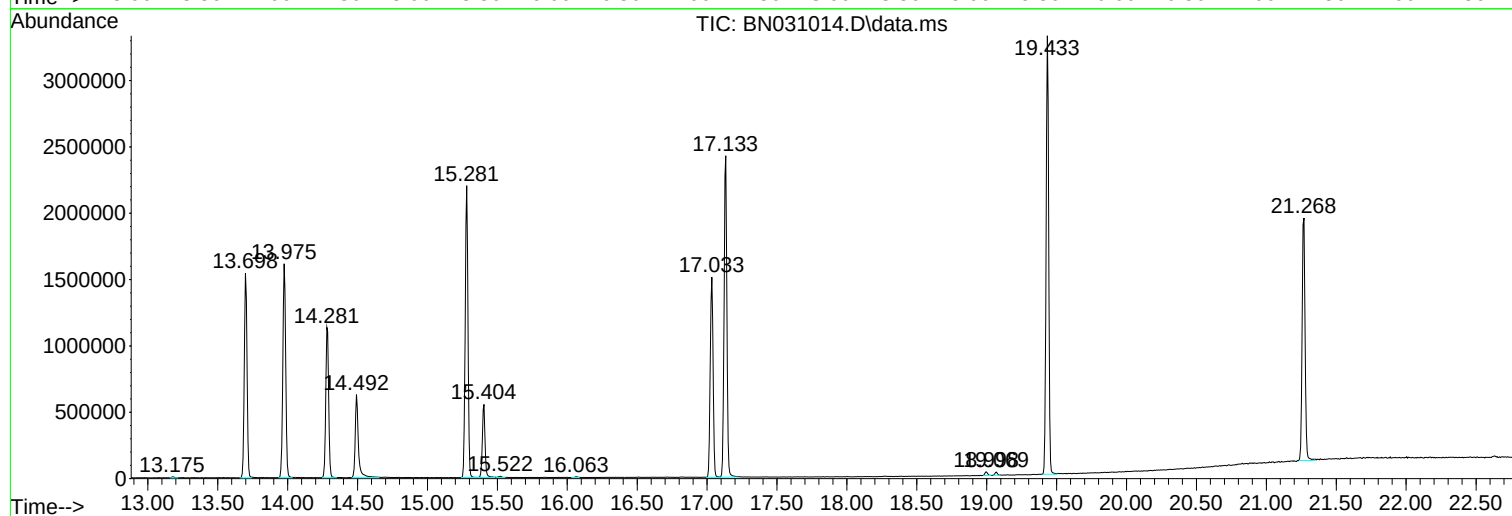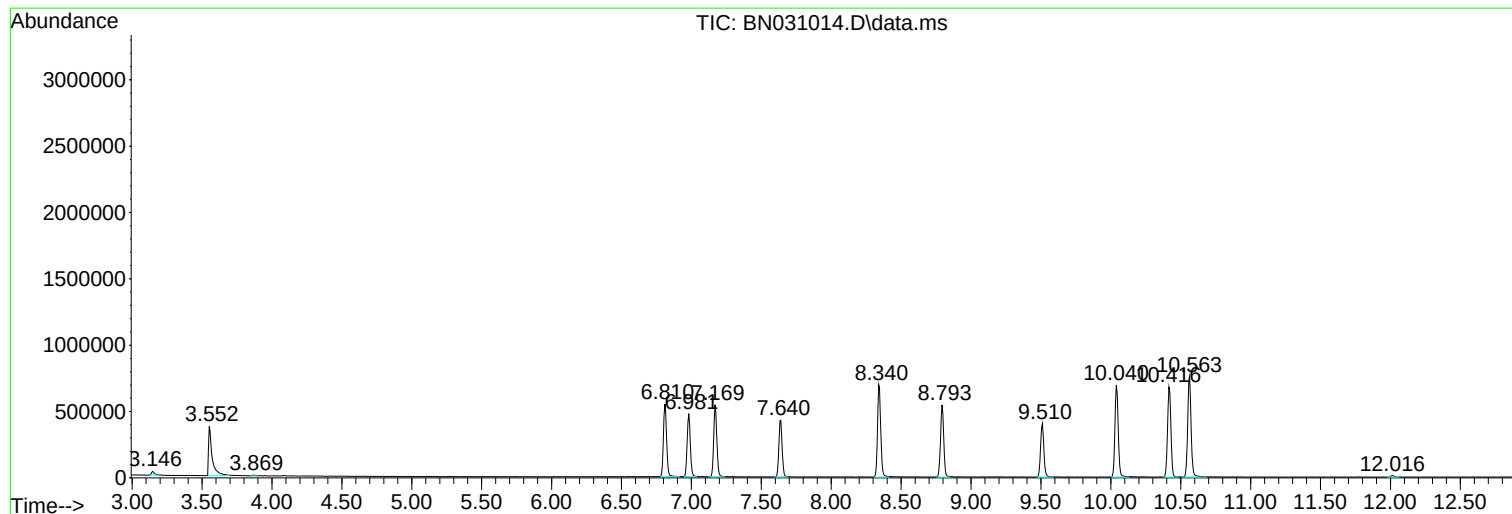

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031014.D
Acq On : 18 Apr 2024 18:35
Operator : MA/JU
Sample : PB160260TB 10X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031014.D
Acq On : 18 Apr 2024 18:35
Operator : MA/JU
Sample : PB160260TB 10X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB260

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc