

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031025.D
 Acq On : 19 Apr 2024 01:49
 Operator : MA/JU
 Sample : P2037-21
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1CY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031025.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	34	rVB2	15477	21811	0.54%	0.067%
2	3.428	72	75	82	rVB4	6767	12402	0.31%	0.038%
3	3.558	95	97	112	rBV	171497	316419	7.85%	0.975%
4	3.875	147	151	154	rBV5	4350	5945	0.15%	0.018%
5	6.810	643	650	663	rBV	320233	513953	12.75%	1.584%
6	6.981	672	679	692	rBV	278605	433673	10.76%	1.336%
7	7.169	705	711	723	rBV	304142	480309	11.92%	1.480%
8	7.634	782	790	800	rBV	384056	631447	15.67%	1.946%
9	8.340	904	910	927	rBV	439423	696961	17.29%	2.148%
10	8.793	980	987	995	rBV	326013	527532	13.09%	1.626%
11	8.951	1010	1014	1019	rBV8	3083	6468	0.16%	0.020%
12	9.193	1050	1055	1060	rVB8	3162	4101	0.10%	0.013%
13	9.363	1078	1084	1092	rVB7	8526	16494	0.41%	0.051%
14	9.510	1102	1109	1117	rBV	175023	299613	7.43%	0.923%
15	10.040	1192	1199	1211	rBV	381123	641956	15.93%	1.978%
16	10.216	1225	1229	1234	rVV6	3111	6417	0.16%	0.020%
17	10.416	1256	1263	1270	rBV	636512	1027427	25.49%	3.166%
18	10.563	1279	1288	1298	rBV	469755	822574	20.41%	2.535%
19	10.628	1298	1299	1306	rVB8	4000	5695	0.14%	0.018%
20	11.163	1385	1390	1398	rBV4	9601	18816	0.47%	0.058%
21	11.845	1502	1506	1510	rVB6	4154	6265	0.16%	0.019%
22	12.010	1527	1534	1542	rVB5	7618	18099	0.45%	0.056%
23	12.316	1582	1586	1591	rVB7	3225	4673	0.12%	0.014%
24	13.104	1716	1720	1725	rBV4	7320	13261	0.33%	0.041%
25	13.181	1727	1733	1738	rVB3	12562	19761	0.49%	0.061%
26	13.698	1814	1821	1836	rBV	1038190	1385894	34.39%	4.271%
27	13.804	1836	1839	1844	rVB7	3224	4468	0.11%	0.014%
28	13.886	1850	1853	1858	rVB4	3960	5718	0.14%	0.018%
29	13.975	1858	1868	1876	rBV	1149932	1647723	40.88%	5.078%
30	14.186	1900	1904	1907	rVB2	9716	11512	0.29%	0.035%
31	14.281	1913	1920	1929	rBV	1073082	1559307	38.69%	4.805%
32	14.504	1951	1958	1974	rBV3	51694	126320	3.13%	0.389%
33	14.633	1977	1980	1986	rVV7	2760	5928	0.15%	0.018%
34	14.681	1986	1988	1996	rVB8	4044	8174	0.20%	0.025%
35	15.139	2062	2066	2072	rVB	16532	20939	0.52%	0.065%
36	15.281	2083	2090	2100	rBV	1543197	2211431	54.87%	6.815%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031025.D
 Acq On : 19 Apr 2024 01:49
 Operator : MA/JU
 Sample : P2037-21
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1CY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	15.398	2105	2110	2115	rVB4	20799	30383	0.75%	0.094%
38	15.528	2126	2132	2134	rBV4	6855	13018	0.32%	0.040%
39	15.633	2147	2150	2155	rVB6	3124	5341	0.13%	0.016%
40	15.692	2158	2160	2166	rBV7	3883	7726	0.19%	0.024%
41	16.004	2209	2213	2221	rBV2	30970	60562	1.50%	0.187%
42	16.063	2221	2223	2230	rVB5	8138	9280	0.23%	0.029%
43	16.345	2267	2271	2274	rBV5	3679	6184	0.15%	0.019%
44	16.580	2307	2311	2314	rBV5	4194	5775	0.14%	0.018%
45	16.692	2325	2330	2338	rBV10	3872	9520	0.24%	0.029%
46	16.798	2344	2348	2353	rBV2	33551	43665	1.08%	0.135%
47	16.845	2353	2356	2362	rVB	16855	22088	0.55%	0.068%
48	17.033	2381	2388	2393	rBV	1467524	2040019	50.62%	6.287%
49	17.127	2398	2404	2415	rVV	1701151	2523194	62.60%	7.776%
50	17.227	2418	2421	2425	rVB6	8799	15114	0.38%	0.047%
51	17.422	2452	2454	2456	rBV3	6899	6485	0.16%	0.020%
52	17.533	2470	2473	2479	rVB	35783	44466	1.10%	0.137%
53	17.639	2484	2491	2496	rBV	8367	20129	0.50%	0.062%
54	17.810	2517	2520	2523	rBV5	6979	10339	0.26%	0.032%
55	17.933	2537	2541	2549	rBV9	27238	48229	1.20%	0.149%
56	18.227	2588	2591	2595	rBV	32326	40663	1.01%	0.125%
57	18.363	2612	2614	2618	rVB4	12941	13927	0.35%	0.043%
58	18.869	2697	2700	2707	rVB	33061	41783	1.04%	0.129%
59	18.992	2718	2721	2726	rVB	25958	29161	0.72%	0.090%
60	19.092	2735	2738	2743	rVB	47104	64402	1.60%	0.198%
61	19.433	2790	2796	2804	rBV	2454432	3374648	83.73%	10.400%
62	19.986	2888	2890	2894	rVB2	41635	42491	1.05%	0.131%
63	20.957	3051	3055	3076	rVB	253553	485804	12.05%	1.497%
64	21.263	3102	3107	3113	rBV2	1888568	2601497	64.55%	8.017%
65	23.968	3558	3567	3577	rBV2	1694681	4030349	100.00%	12.421%
66	24.162	3592	3600	3613	rVB2	1264134	3263189	80.97%	10.056%


Sum of corrected areas: 32448917

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031025.D
Acq On : 19 Apr 2024 01:49
Operator : MA/JU
Sample : P2037-21
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

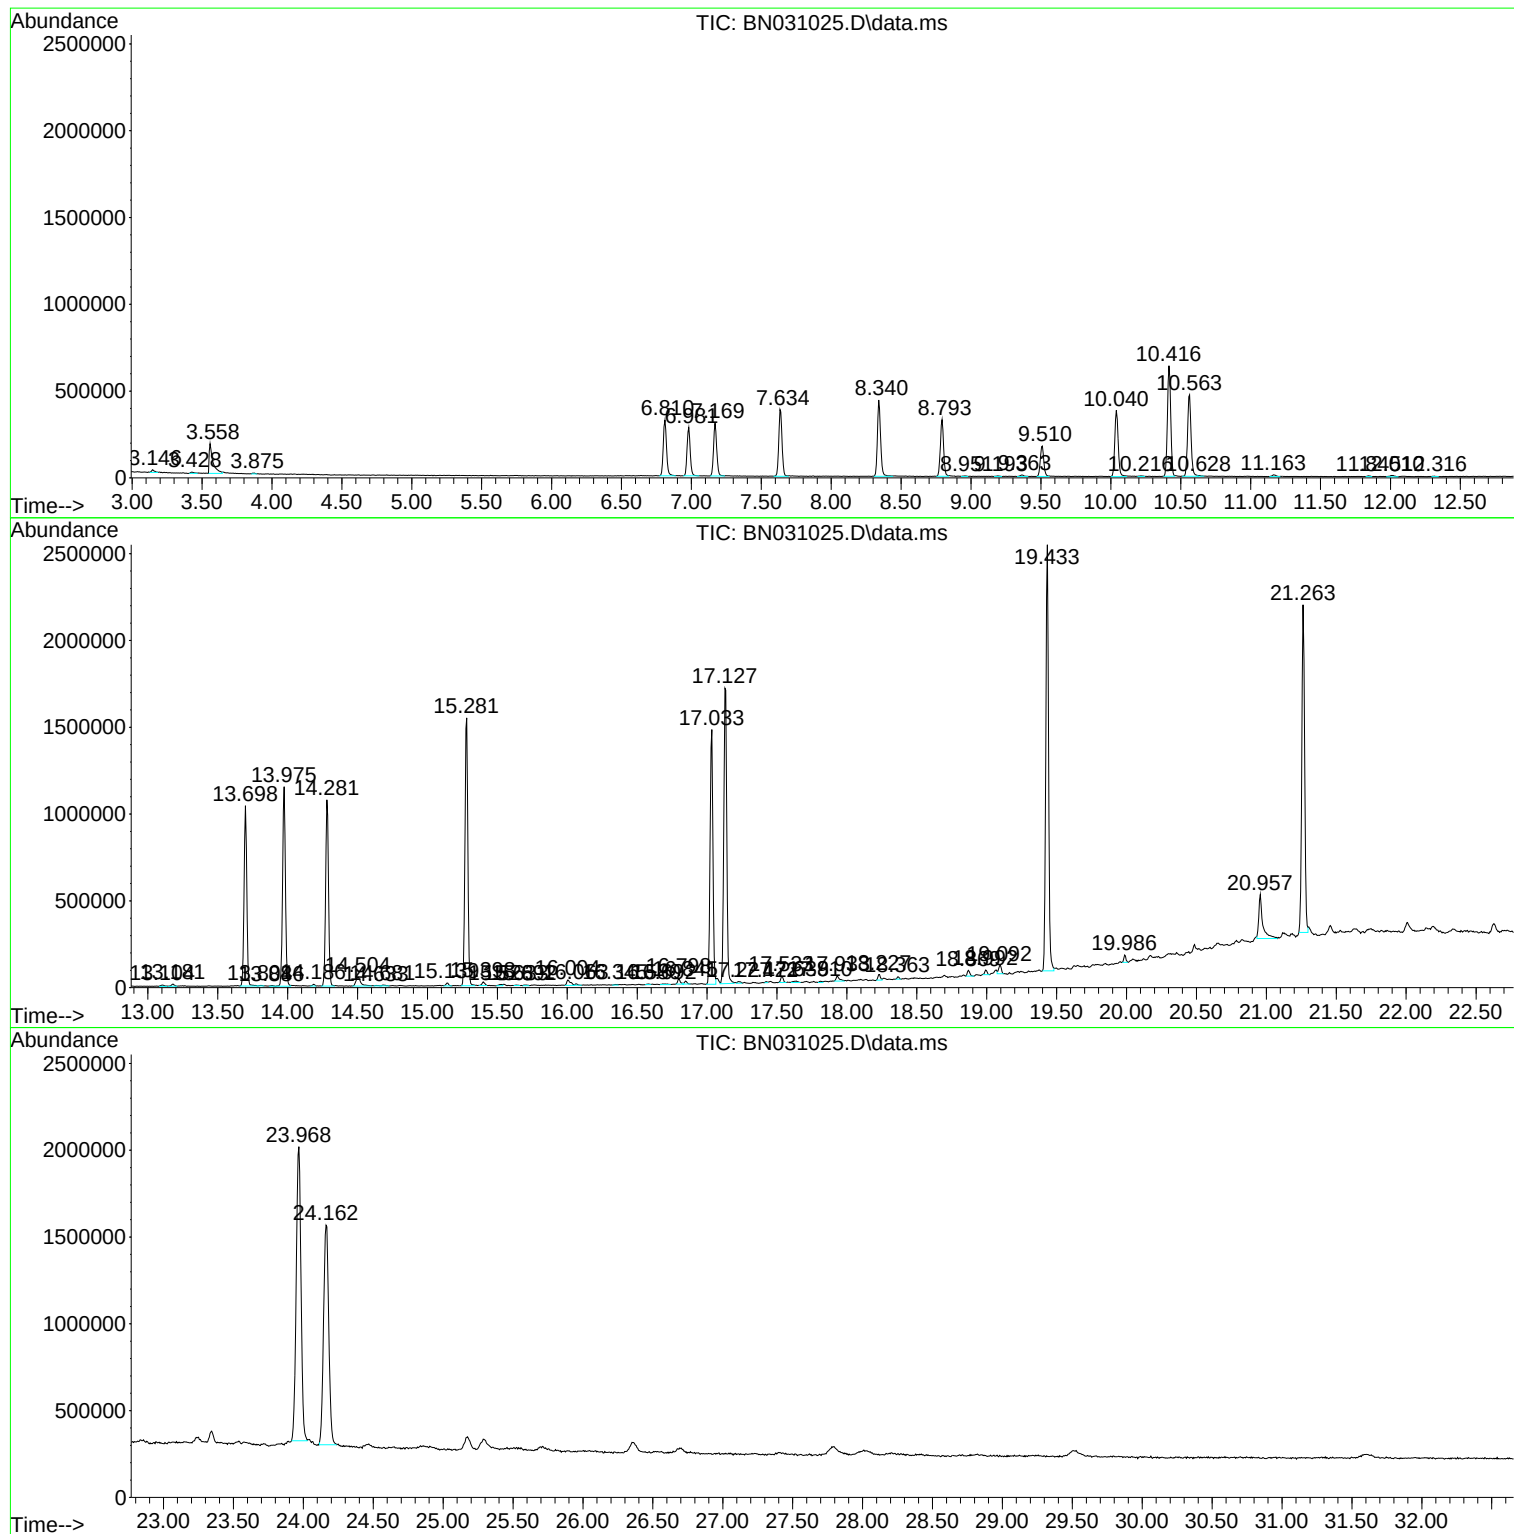

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031025.D
Acq On : 19 Apr 2024 01:49
Operator : MA/JU
Sample : P2037-21
Misc :
ALS Vial : 60 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
E1CY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
20.957	3.73 ng/ul	485804	Chrysene-d12		21.262	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	5-Octadecene, (E)-		252	C18H36	007206-21-5	95
2	Pentadecafluorooctanoic acid, oc...		666	C26H37F15O2	1000406-04-8	94
3	1-Heneicosanol		312	C21H44O	015594-90-8	93
4	Eicosyl pentafluoropropionate		444	C23H41F5O2	1000351-80-8	91
5	Heptafluorobutyric acid, n-octad...		466	C22H37F7O2	000400-57-7	91

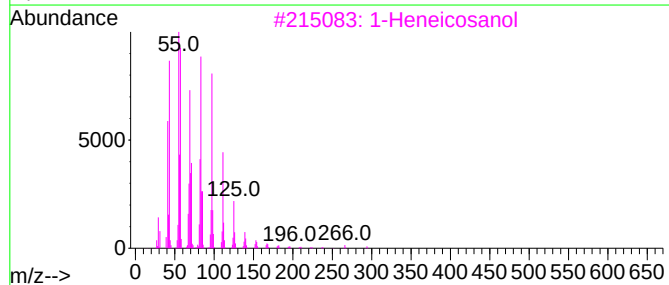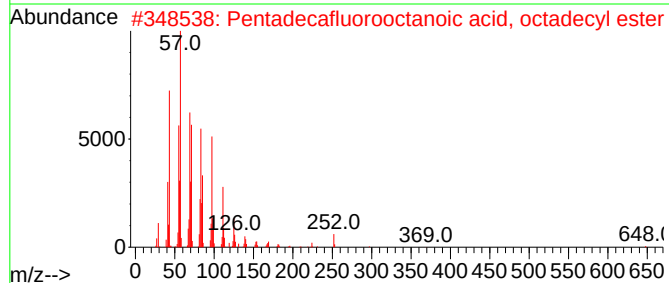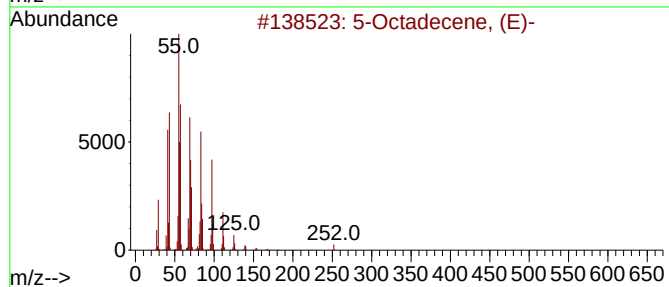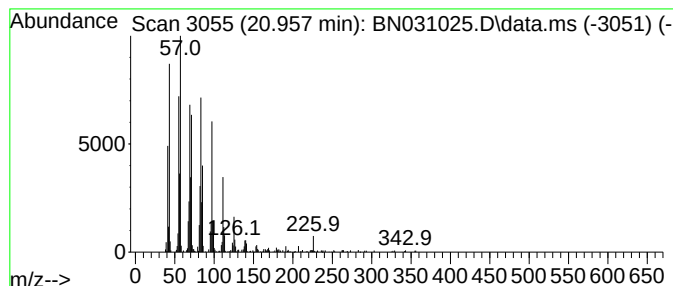

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031025.D
Acq On : 19 Apr 2024 01:49
Operator : MA/JU
Sample : P2037-21
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	20.957	3.7	ng/u1	485804	5	21.262	2601500	20.0