

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031029.D
 Acq On : 19 Apr 2024 05:05
 Operator : MA/JU
 Sample : PB160251BL
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK251

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031029.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	23	27	43	rVB	21271	39290	0.84%	0.114%
2	3.552	93	96	124	rBV	249288	487461	10.37%	1.419%
3	3.870	147	150	154	rBV6	4658	5686	0.12%	0.017%
4	6.811	643	650	659	rBV	395714	608914	12.95%	1.773%
5	6.981	671	679	692	rBV	323963	521572	11.09%	1.518%
6	7.169	704	711	724	rBV	391451	610904	12.99%	1.779%
7	7.634	784	790	803	rBV	369704	586848	12.48%	1.708%
8	8.340	904	910	923	rBV	510618	809245	17.21%	2.356%
9	8.793	980	987	996	rBV	378607	628134	13.36%	1.829%
10	9.505	1102	1108	1121	rBV	289404	482178	10.26%	1.404%
11	10.040	1191	1199	1212	rBV	504062	826507	17.58%	2.406%
12	10.416	1256	1263	1274	rVB	585879	955049	20.31%	2.780%
13	10.557	1280	1287	1298	rBV	554098	943873	20.08%	2.748%
14	12.010	1528	1534	1543	rVB3	8560	17451	0.37%	0.051%
15	13.175	1729	1732	1737	rBV3	7852	11284	0.24%	0.033%
16	13.698	1814	1821	1830	rBV	1081207	1504451	32.00%	4.380%
17	13.975	1861	1868	1877	rBV	1185016	1723105	36.65%	5.016%
18	14.281	1914	1920	1931	rVB	1032332	1452535	30.90%	4.229%
19	14.492	1948	1956	1971	rBV	436780	731973	15.57%	2.131%
20	14.834	2010	2014	2020	rVB6	2360	6002	0.13%	0.017%
21	15.281	2083	2090	2098	rBV	1566368	2268648	48.26%	6.605%
22	15.398	2105	2110	2119	rBV	411712	565404	12.03%	1.646%
23	15.516	2127	2130	2134	rVB3	6319	8734	0.19%	0.025%
24	16.063	2219	2223	2227	rBV4	6127	7744	0.16%	0.023%
25	16.822	2346	2352	2355	rBV5	3844	7633	0.16%	0.022%
26	17.034	2381	2388	2398	rBV	1361624	1924553	40.94%	5.603%
27	17.128	2398	2404	2419	rVV	1897265	2704384	57.52%	7.873%
28	18.992	2717	2721	2727	rBV3	22575	31766	0.68%	0.092%
29	19.063	2729	2733	2739	rVV3	20205	30740	0.65%	0.089%
30	19.433	2790	2796	2805	rBV	2511548	3432341	73.01%	9.992%
31	21.263	3101	3107	3115	rBV2	1794654	2553852	54.32%	7.435%
32	23.963	3558	3566	3588	rVB	1921633	4701260	100.00%	13.687%
33	24.163	3592	3600	3611	rVV2	1288527	3159839	67.21%	9.199%




Sum of corrected areas: 34349360

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031029.D
Acq On : 19 Apr 2024 05:05
Operator : MA/JU
Sample : PB160251BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK251

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

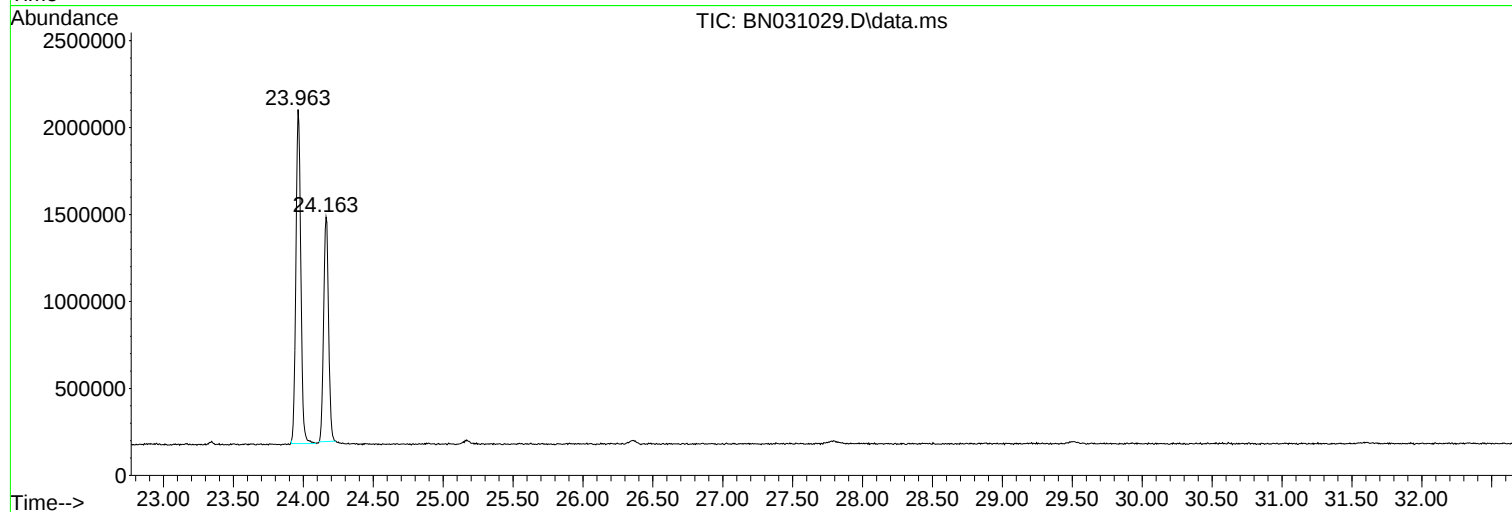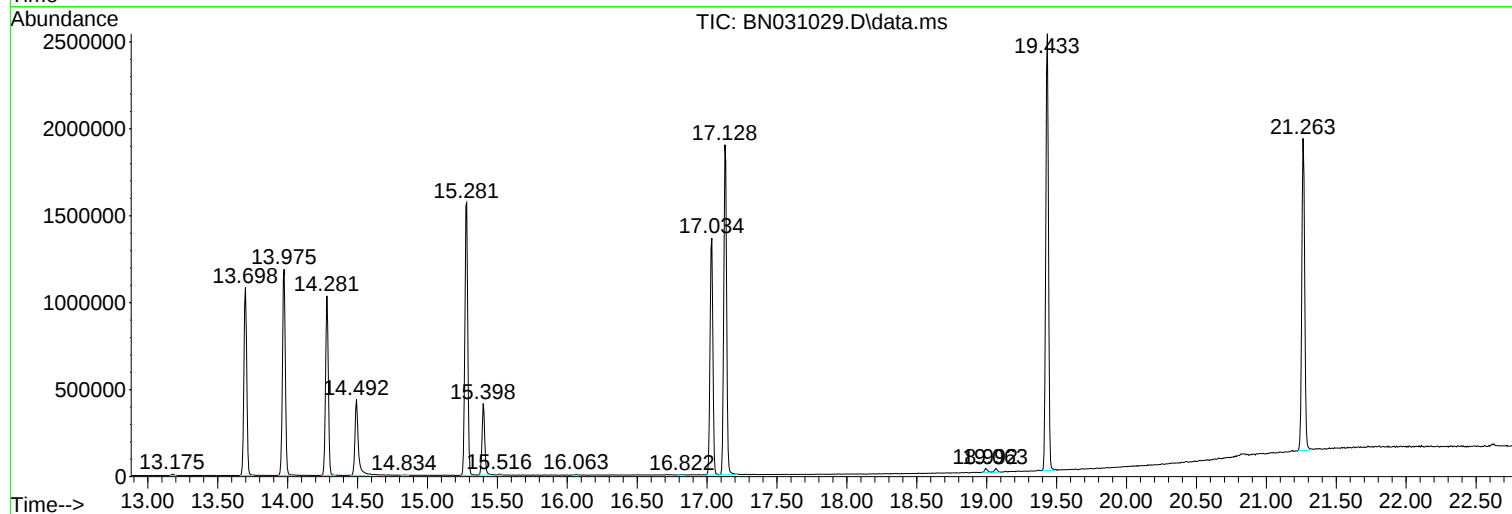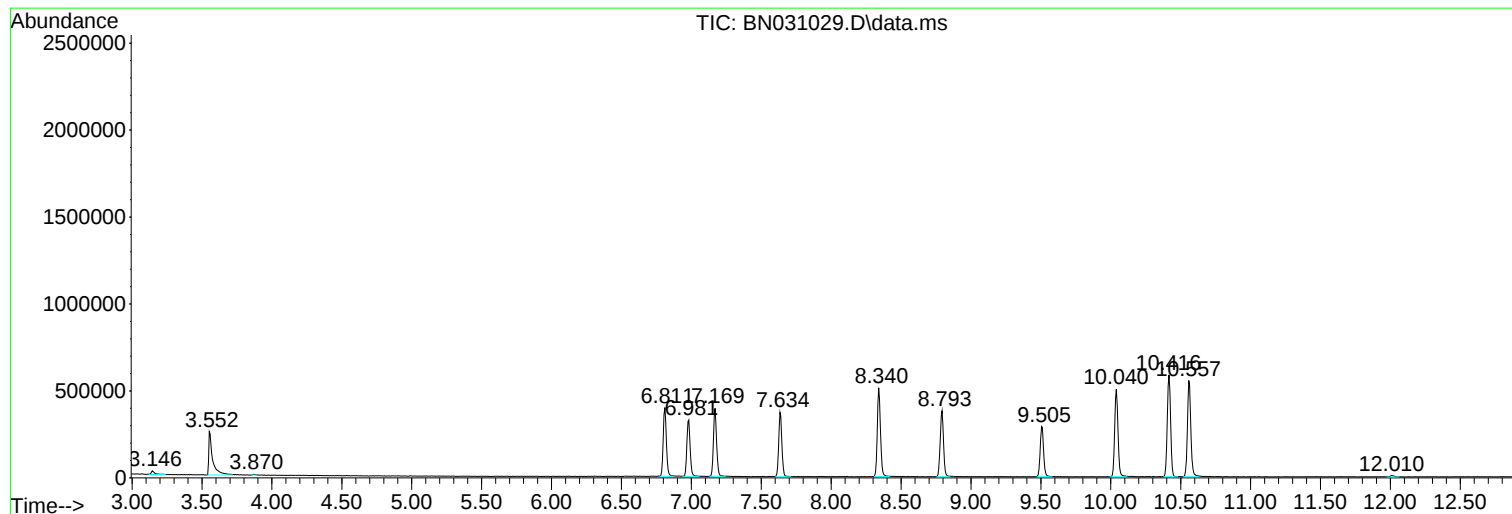

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031029.D
Acq On : 19 Apr 2024 05:05
Operator : MA/JU
Sample : PB160251BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK251

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031029.D
Acq On : 19 Apr 2024 05:05
Operator : MA/JU
Sample : PB160251BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK251

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------