

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031032.D
 Acq On : 19 Apr 2024 07:02
 Operator : MA/JU
 Sample : PB160331BL
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK331

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031032.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	34	rBV	22467	30515	0.55%	0.076%
2	3.552	93	96	119	rBV	303819	562400	10.05%	1.394%
3	6.810	644	650	660	rBV	475943	764420	13.66%	1.895%
4	6.981	673	679	690	rBV	391023	608203	10.87%	1.507%
5	7.169	705	711	722	rBV	481335	779171	13.93%	1.931%
6	7.640	784	791	798	rBV	400954	641868	11.47%	1.591%
7	8.346	903	911	923	rBV	611566	1018800	18.21%	2.525%
8	8.793	979	987	996	rBV	473345	782068	13.98%	1.938%
9	9.510	1102	1109	1120	rBV	382173	637966	11.40%	1.581%
10	10.040	1193	1199	1209	rBV	631783	1055664	18.87%	2.616%
11	10.422	1254	1264	1274	rBV	627024	1054152	18.84%	2.613%
12	10.563	1280	1288	1297	rBV	655997	1129257	20.18%	2.799%
13	12.016	1531	1535	1542	rVB	13188	17999	0.32%	0.045%
14	13.181	1726	1733	1738	rBV2	15162	24455	0.44%	0.061%
15	13.698	1815	1821	1831	rBV	1206993	1665991	29.78%	4.129%
16	13.975	1861	1868	1880	rBV2	1400628	2128791	38.05%	5.276%
17	14.286	1915	1921	1932	rVB	1064689	1551563	27.73%	3.845%
18	14.492	1950	1956	1977	rBV	538877	928517	16.60%	2.301%
19	15.280	2084	2090	2097	rBV	1888793	2683993	47.97%	6.652%
20	15.404	2105	2111	2122	rBV	511598	724361	12.95%	1.795%
21	15.522	2127	2131	2135	rVB6	11158	20919	0.37%	0.052%
22	17.033	2382	2388	2397	rBV	1436689	2032784	36.33%	5.038%
23	17.133	2399	2405	2412	rBV2	2258720	3161077	56.50%	7.834%
24	19.433	2791	2796	2805	rBV	2805224	3976620	71.07%	9.856%
25	21.268	3104	3108	3117	rVB2	2037804	3299087	58.96%	8.176%
26	23.974	3562	3568	3579	rVB2	2318441	5595098	100.00%	13.867%
27	24.174	3596	3602	3610	rVB2	1433357	3473502	62.08%	8.609%




Sum of corrected areas: 40349241

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031032.D
Acq On : 19 Apr 2024 07:02
Operator : MA/JU
Sample : PB160331BL
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK331

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

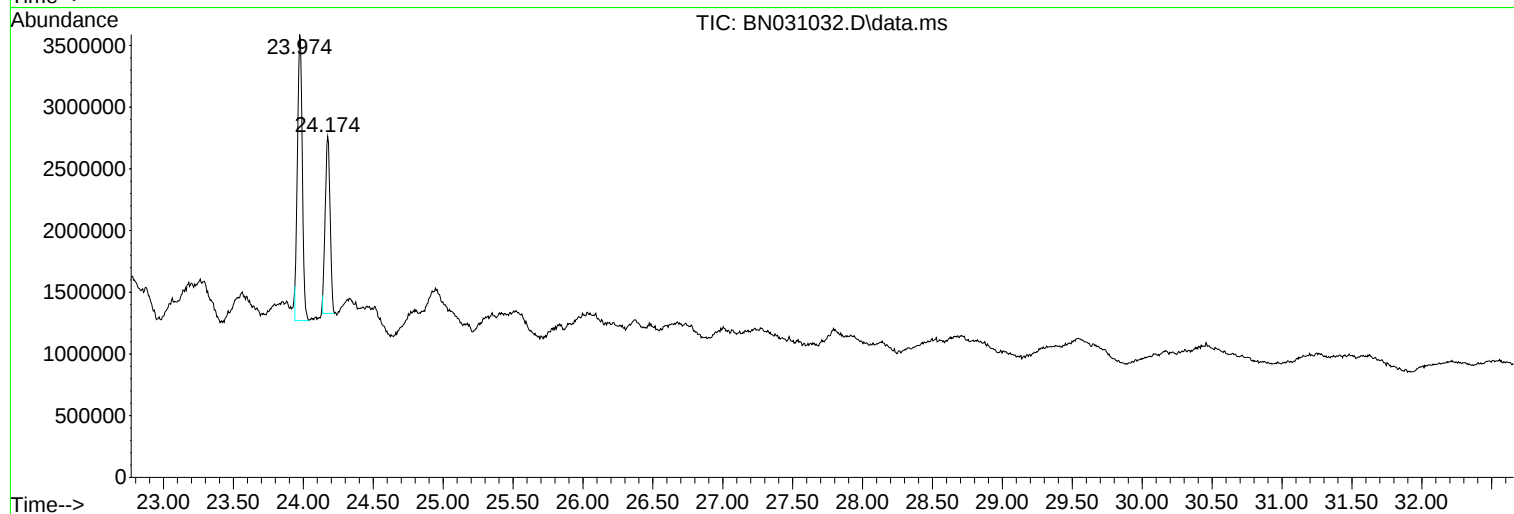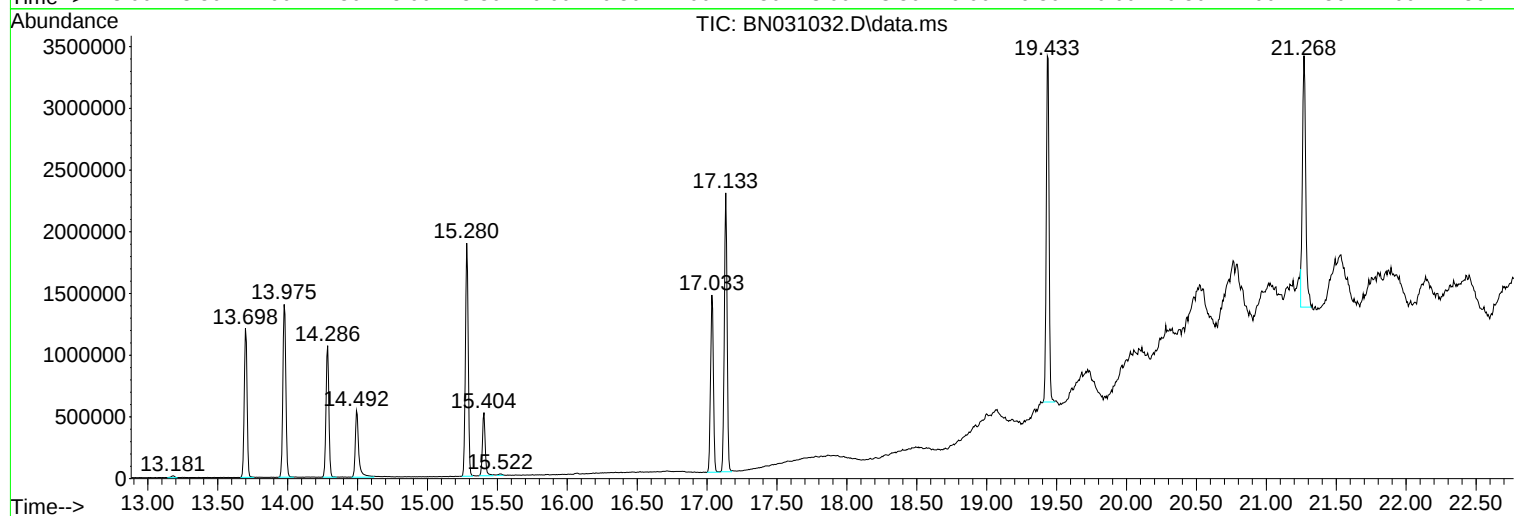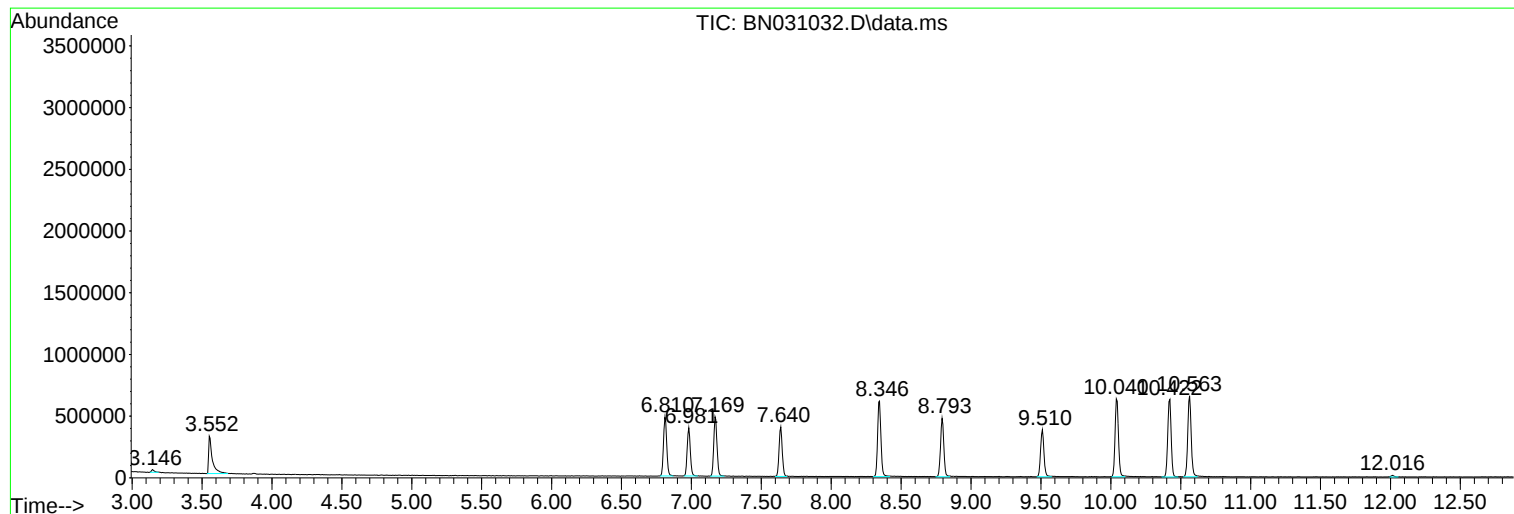

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031032.D
Acq On : 19 Apr 2024 07:02
Operator : MA/JU
Sample : PB160331BL
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK331

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031032.D
Acq On : 19 Apr 2024 07:02
Operator : MA/JU
Sample : PB160331BL
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK331

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------