

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
 Data File : BN031034.D
 Acq On : 19 Apr 2024 08:20
 Operator : MA/JU
 Sample : PB160242TB 10X
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLEB242

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	41	rVB	27979	47495	0.83%	0.122%
2	3.552	94	96	118	rBV	323179	598866	10.41%	1.532%
3	3.870	147	150	156	rVB7	4678	8905	0.15%	0.023%
4	6.811	641	650	659	rBV	490899	786097	13.67%	2.011%
5	6.981	673	679	689	rVB	392580	616497	10.72%	1.577%
6	7.169	704	711	719	rBV	493441	788423	13.71%	2.017%
7	7.640	784	791	799	rBV	345720	558205	9.71%	1.428%
8	8.340	903	910	924	rBV	639431	1033971	17.98%	2.645%
9	8.793	978	987	998	rBV	487552	805449	14.01%	2.061%
10	9.510	1102	1109	1120	rBV	392011	657880	11.44%	1.683%
11	10.040	1191	1199	1214	rBV	638914	1080683	18.79%	2.765%
12	10.416	1256	1263	1273	rBV	553829	907354	15.78%	2.321%
13	10.563	1281	1288	1304	rBV	684687	1192740	20.74%	3.052%
14	12.010	1530	1534	1539	rBV3	10346	17626	0.31%	0.045%
15	13.175	1727	1732	1736	rBV5	8865	12745	0.22%	0.033%
16	13.698	1814	1821	1836	rBV	1241550	1728862	30.06%	4.423%
17	13.975	1861	1868	1880	rBV2	1420933	2135397	37.13%	5.463%
18	14.281	1914	1920	1929	rBV	896856	1327364	23.08%	3.396%
19	14.492	1950	1956	1976	rBV	584109	957165	16.64%	2.449%
20	15.281	2084	2090	2101	rBV	1881541	2700624	46.96%	6.909%
21	15.404	2104	2111	2124	rVV	519347	756292	13.15%	1.935%
22	15.522	2127	2131	2136	rVB3	9624	13643	0.24%	0.035%
23	16.063	2219	2223	2228	rVB6	7247	11374	0.20%	0.029%
24	17.034	2382	2388	2398	rBV	1262485	1737198	30.21%	4.445%
25	17.134	2398	2405	2419	rBV	2305125	3197709	55.61%	8.181%
26	18.998	2718	2722	2726	rBV2	36617	52961	0.92%	0.135%
27	19.069	2731	2734	2739	rVB2	32521	43293	0.75%	0.111%
28	19.433	2790	2796	2803	rBV	3003982	4073681	70.84%	10.422%
29	21.269	3103	3108	3114	rVB2	1688267	2369550	41.21%	6.062%
30	23.974	3560	3568	3578	rVB2	2456409	5750582	100.00%	14.713%
31	24.168	3594	3601	3611	rVB	1298989	3117640	54.21%	7.976%




Sum of corrected areas: 39086271

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031034.D
Acq On : 19 Apr 2024 08:20
Operator : MA/JU
Sample : PB160242TB 10X
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB242

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

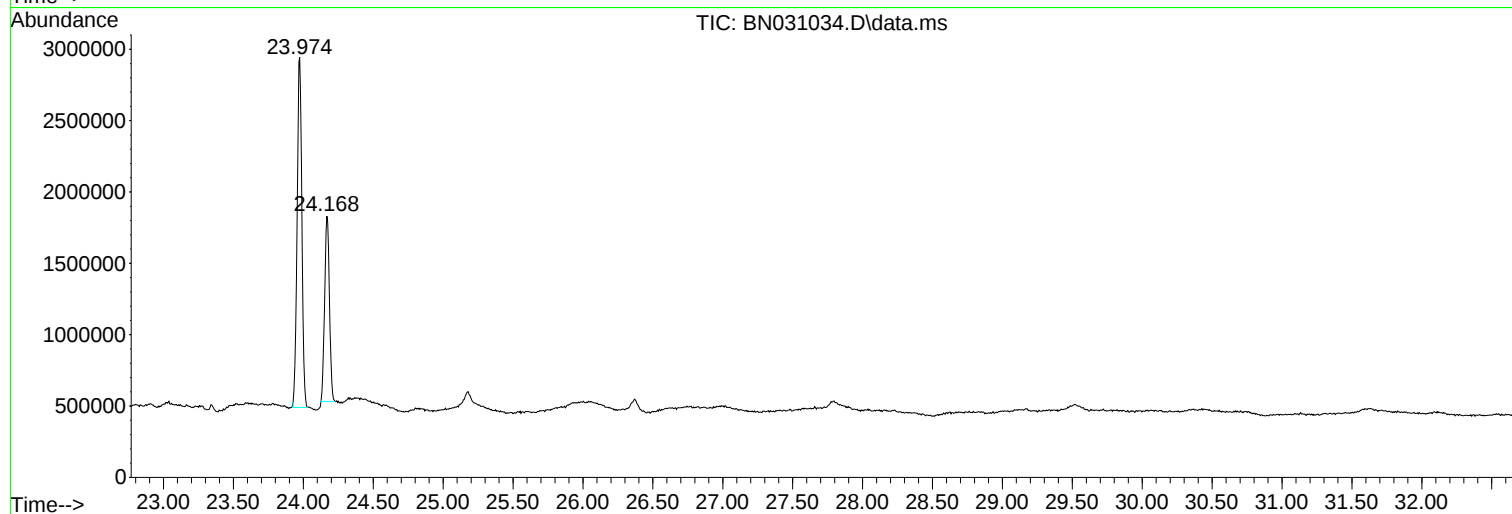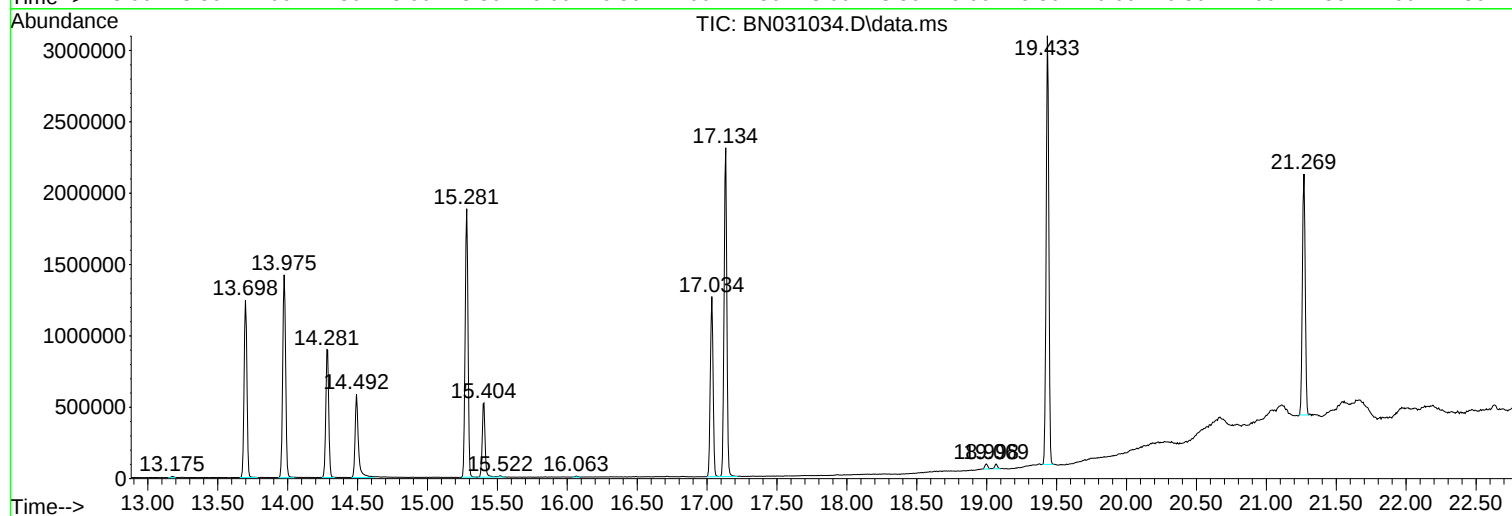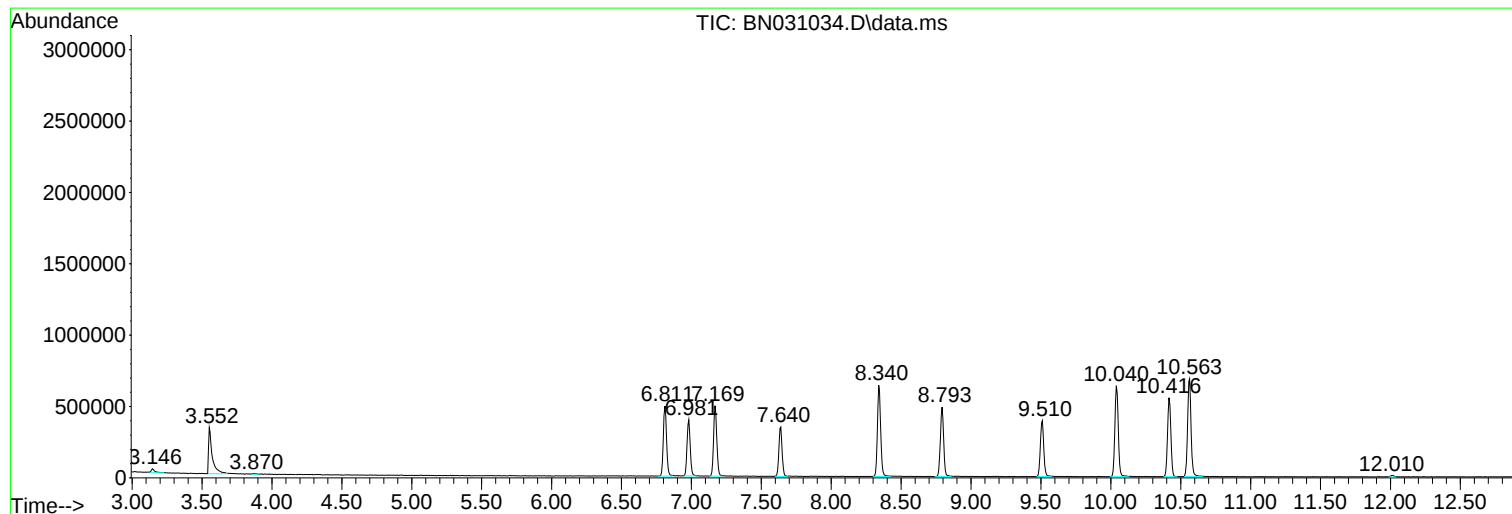

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031034.D
Acq On : 19 Apr 2024 08:20
Operator : MA/JU
Sample : PB160242TB 10X
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB242

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041724\
Data File : BN031034.D
Acq On : 19 Apr 2024 08:20
Operator : MA/JU
Sample : PB160242TB 10X
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB242

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc