
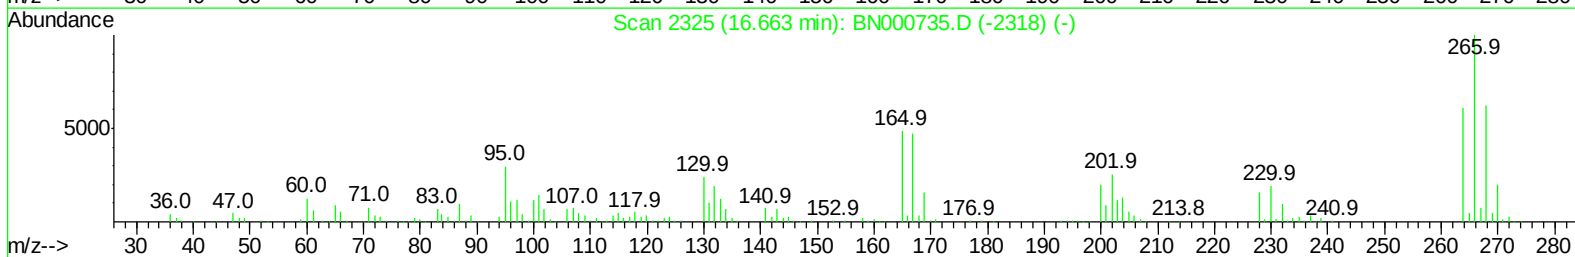
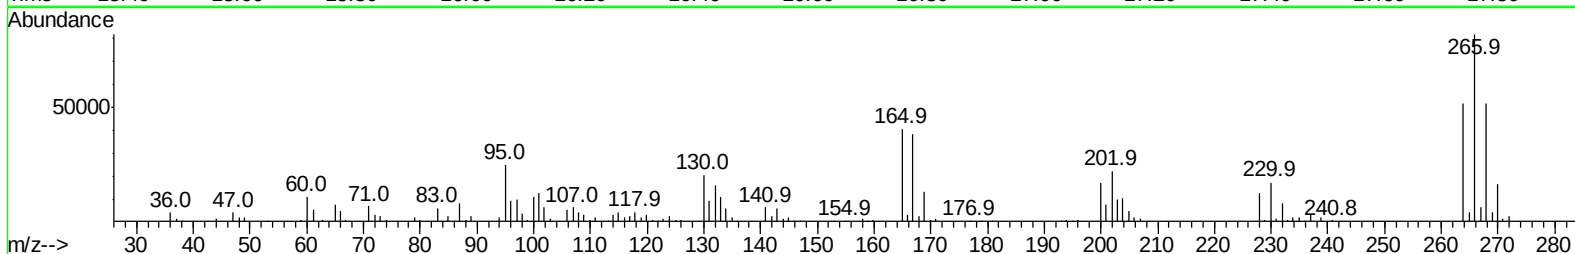


Data Path : Z:\HPCHEM1\BNA N\DATA\BN041818\
Data File : BN000740.D
Acq On : 18 Apr 2018 15:01
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 07:38:29 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN041818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 18 16:58:01 2018
Response via : Initial Calibration

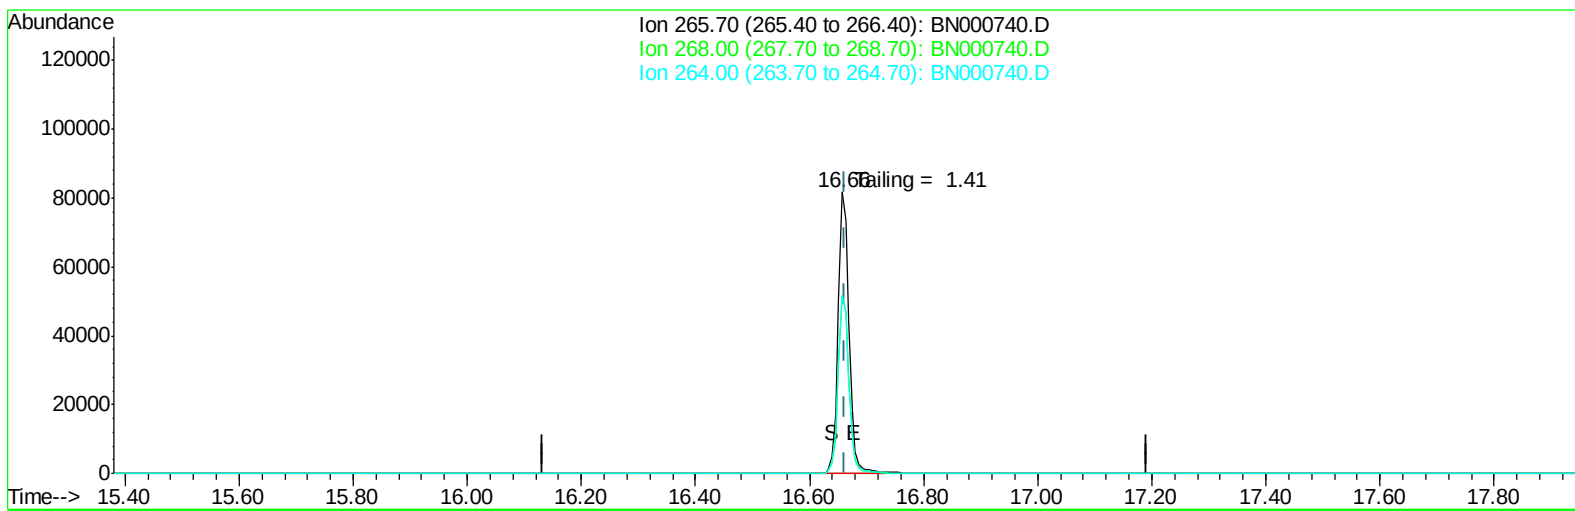

TIC: BN000740.D

(69) Pentachlorophenol (C)




16.657min (-0.006) 37836.66ng

response 108709

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.35
264.00	62.00	62.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA N\DATA\BN041818\
Data File : BN000740.D
Acq On : 18 Apr 2018 15:01
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 07:38:29 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN041818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 18 16:58:01 2018
Response via : Initial Calibration

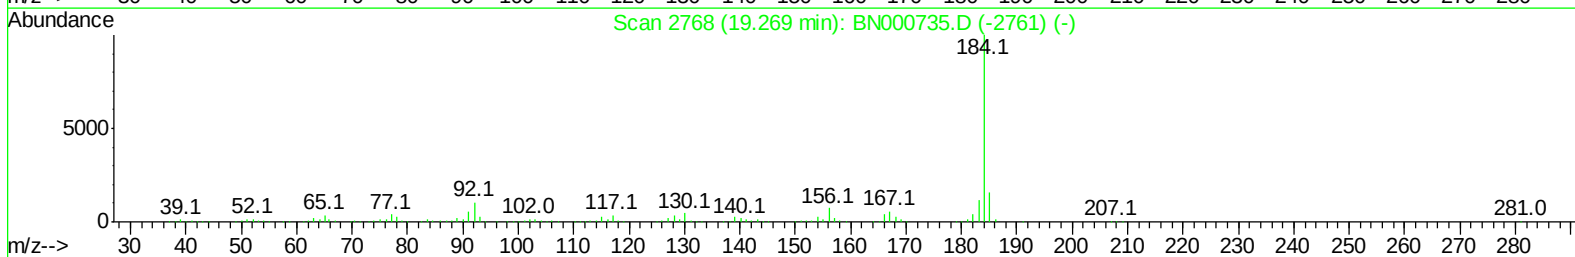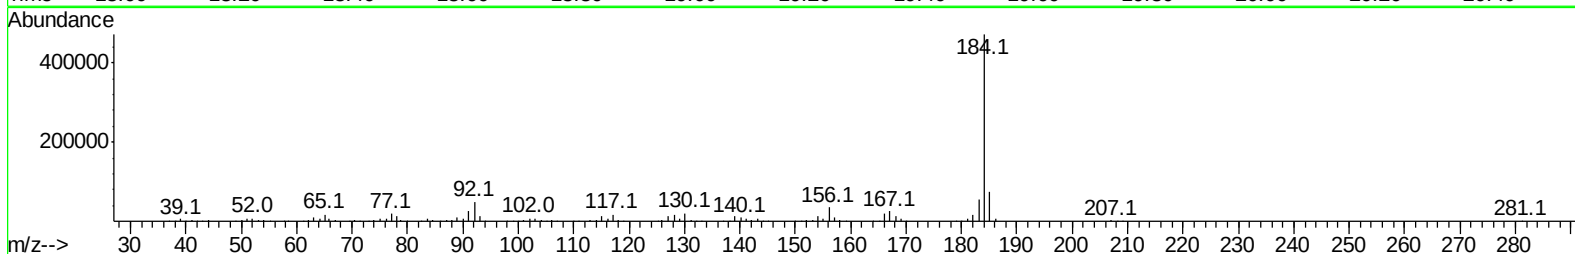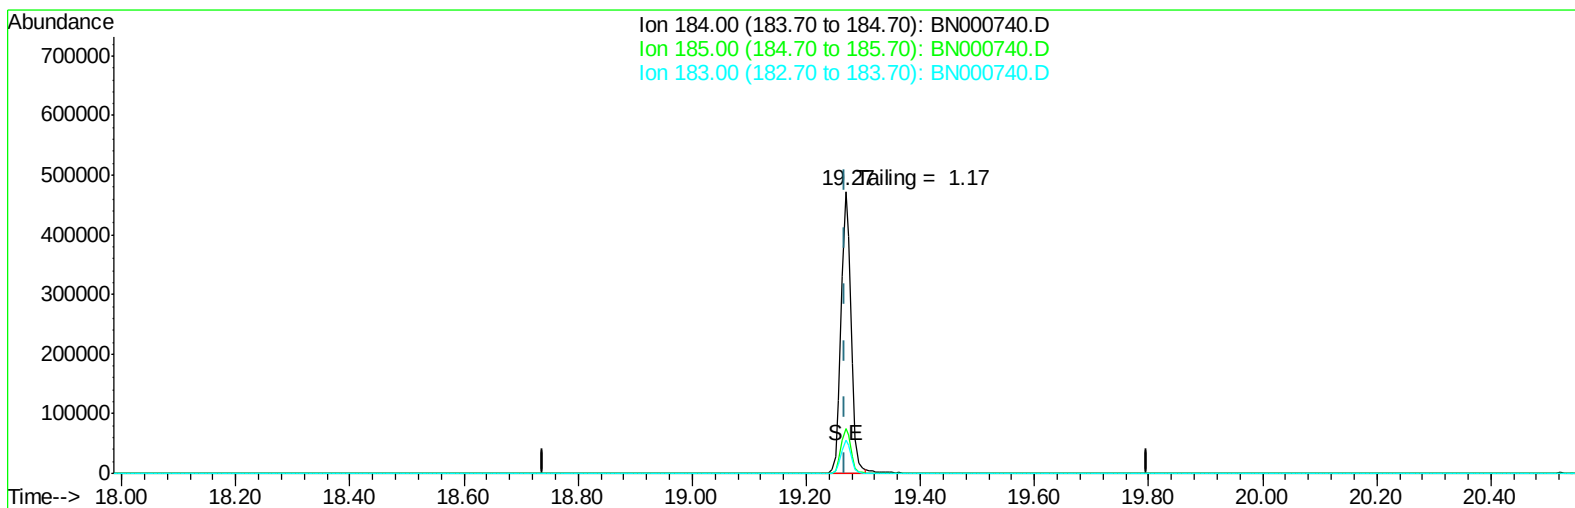

TIC: BN000740.D

(76) Benzidine

19.269min (+0.000) 0.00ng

response 588613

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	16.03
183.00	13.30	11.64
0.00	0.00	0.00