
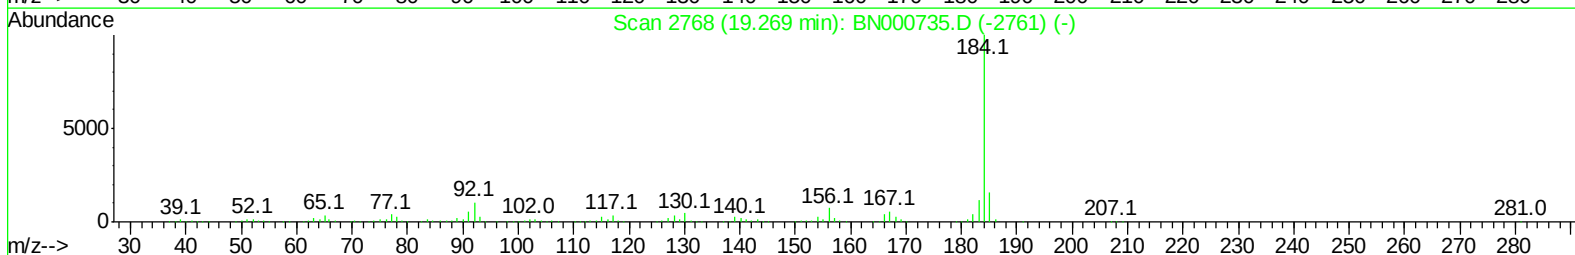
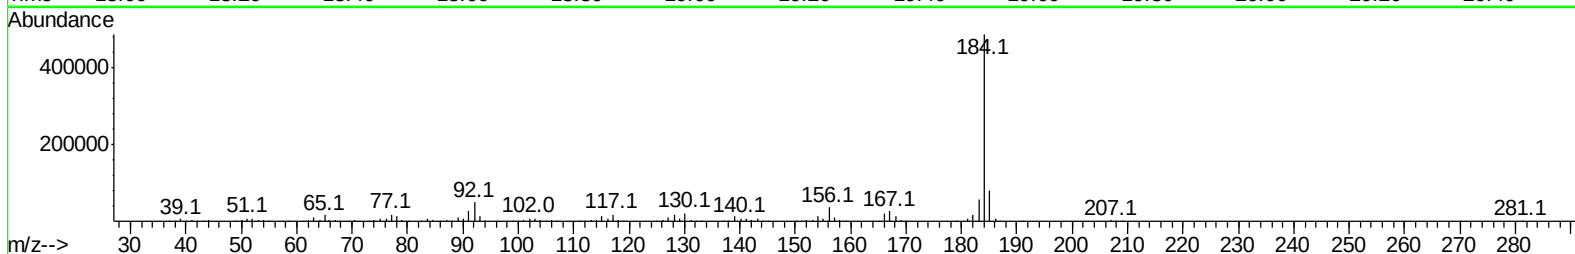


Data Path : Z:\HPCHEM1\BNA N\DATA\BN041818\
Data File : BN000758.D
Acq On : 19 Apr 2018 02:00
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 07:40:10 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN041818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 18 16:58:01 2018
Response via : Initial Calibration

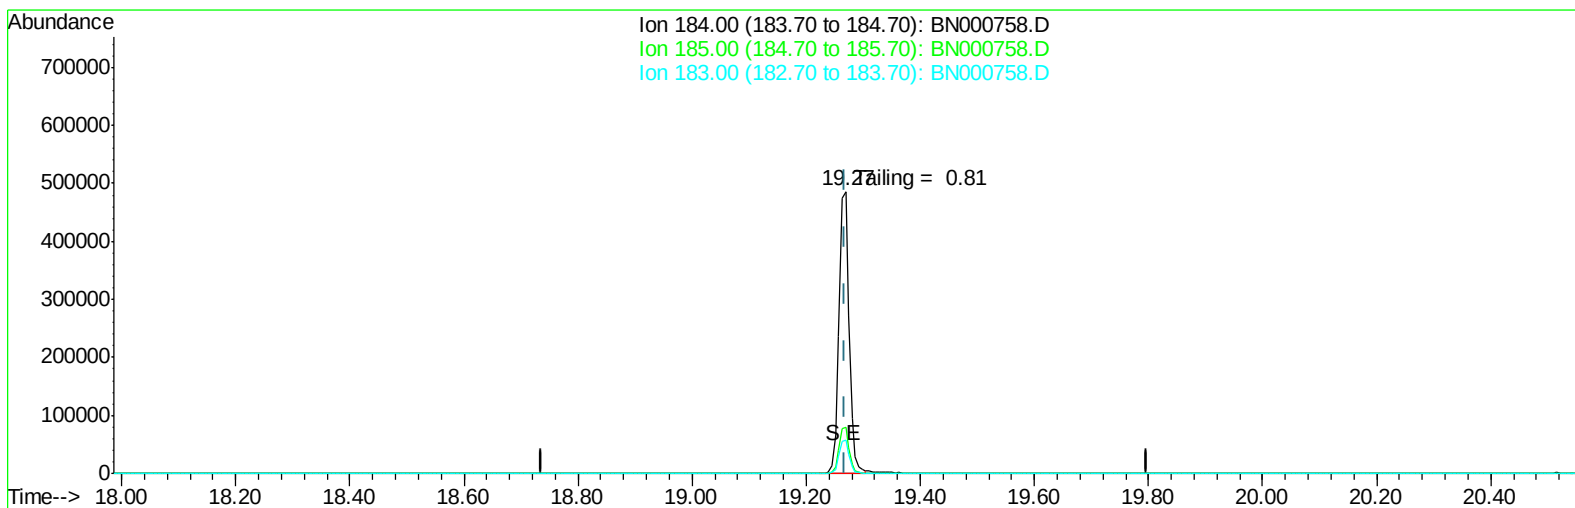

TIC: BN000758.D

(76) Benzidine

19.269min (+0.001) 0.00ng

response 609572

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	16.56
183.00	13.30	11.87
0.00	0.00	0.00