


Data Path : Z:\HPCHEM1\BNA N\DATA\BN041818\
Data File : BN000730.D
Acq On : 18 Apr 2018 08:47
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN041818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 18 16:58:01 2018

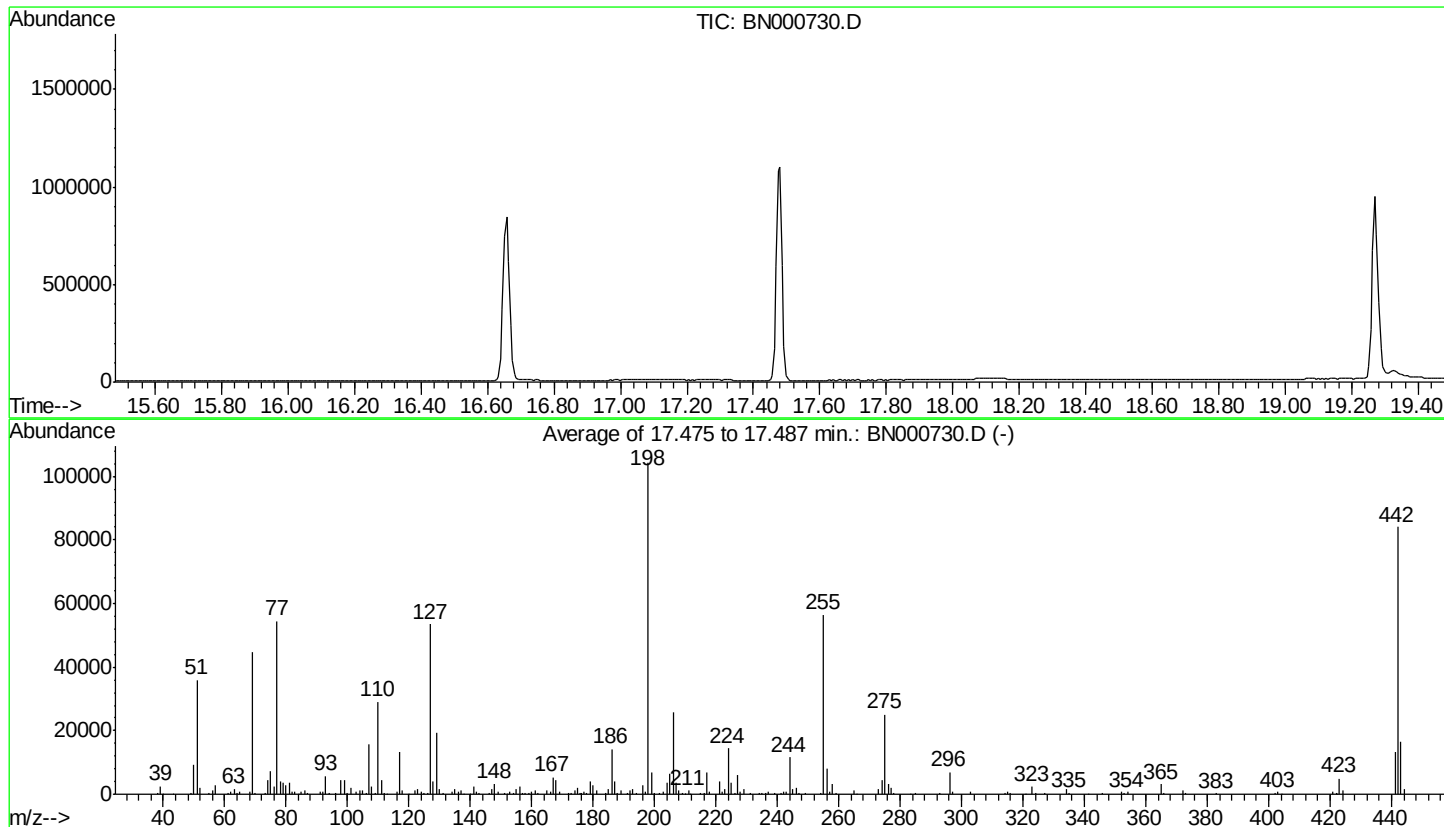

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	35853	PASS
68	69	0.00	2	1.8	803	PASS
69	198	0.00	100	42.8	44642	PASS
70	69	0.00	2	0.5	220	PASS
127	198	10	80	51.3	53509	PASS
197	198	0.00	2	0.8	856	PASS
198	198	100	100	100.0	104330	PASS
199	198	5	9	6.7	6971	PASS
275	198	10	60	23.9	24976	PASS
365	198	1	100	3.0	3164	PASS
441	443	0.01	100	80.1	13115	PASS
442	198	50	100	80.5	84000	PASS
443	442	15	24	19.5	16372	PASS