


Data Path : Z:\HPCHEM1\BNA N\Data\BN041818\
 Data File : BN000740.D
 Acq On : 18 Apr 2018 15:01
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN041818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 18 16:58:01 2018

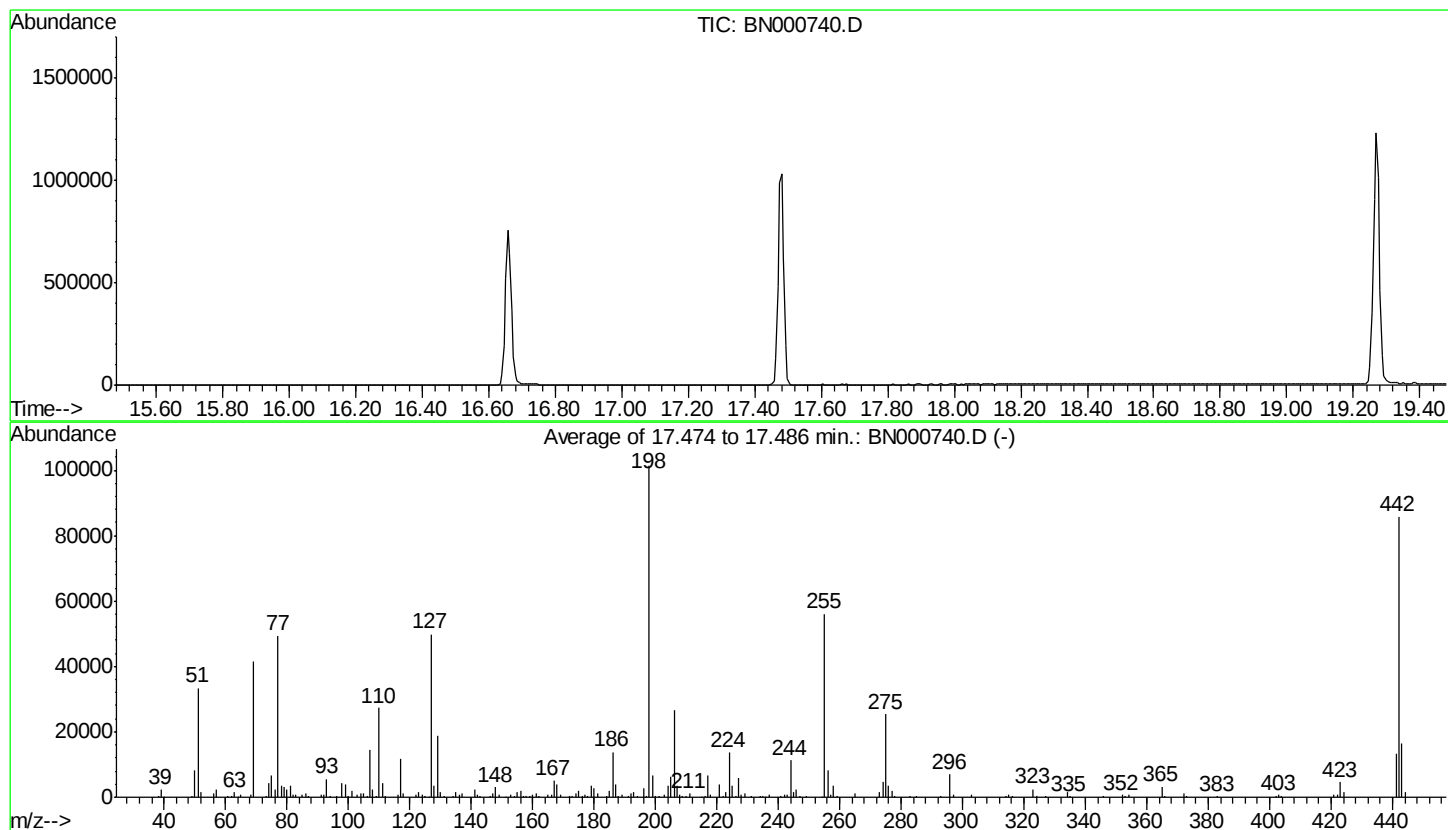

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	33370	PASS
68	69	0.00	2	1.8	761	PASS
69	198	0.00	100	40.9	41466	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.1	49818	PASS
197	198	0.00	2	0.3	254	PASS
198	198	100	100	100.0	101384	PASS
199	198	5	9	6.7	6772	PASS
275	198	10	60	25.0	25389	PASS
365	198	1	100	3.3	3314	PASS
441	443	0.01	100	81.4	13382	PASS
442	198	50	100	84.7	85850	PASS
443	442	15	24	19.2	16445	PASS