


Data Path : Z:\HPCHEM1\BNA N\Data\BN041818\
 Data File : BN000758.D
 Acq On : 19 Apr 2018 02:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN041818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 18 16:58:01 2018

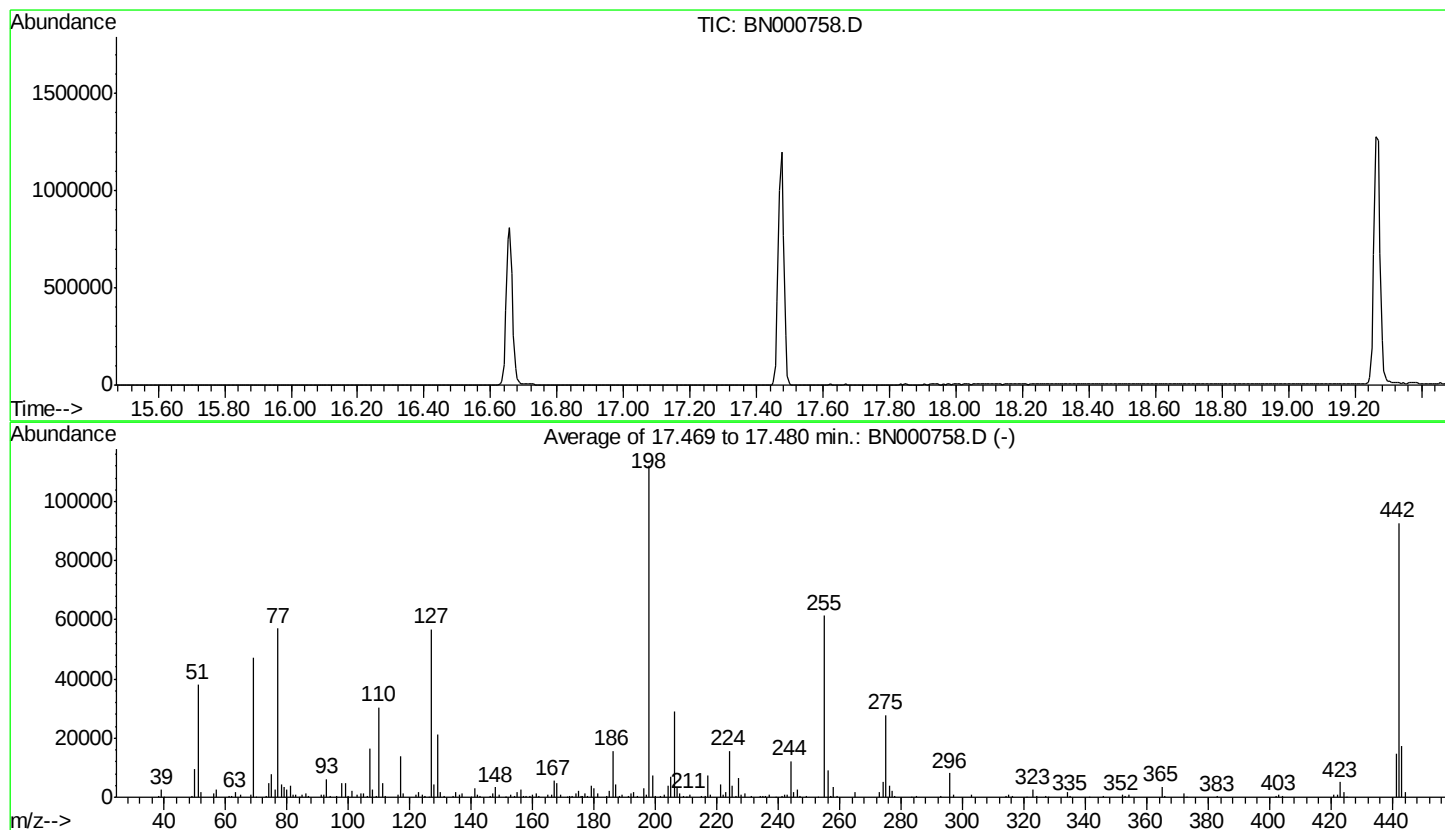

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	38000	PASS
68	69	0.00	2	1.8	836	PASS
69	198	0.00	100	42.0	47176	PASS
70	69	0.00	2	0.2	111	PASS
127	198	10	80	50.7	56906	PASS
197	198	0.00	2	0.7	806	PASS
198	198	100	100	100.0	112197	PASS
199	198	5	9	6.8	7587	PASS
275	198	10	60	24.8	27808	PASS
365	198	1	100	3.2	3611	PASS
441	443	0.01	100	84.4	14604	PASS
442	198	50	100	82.8	92864	PASS
443	442	15	24	18.6	17307	PASS