
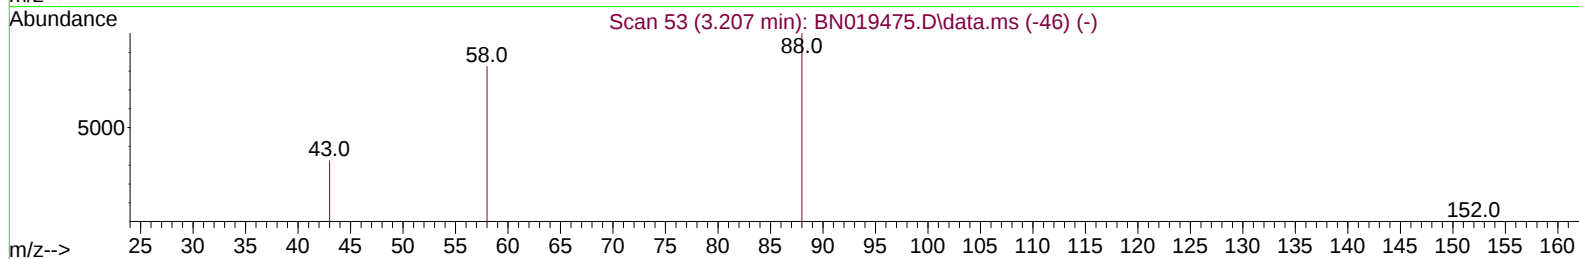
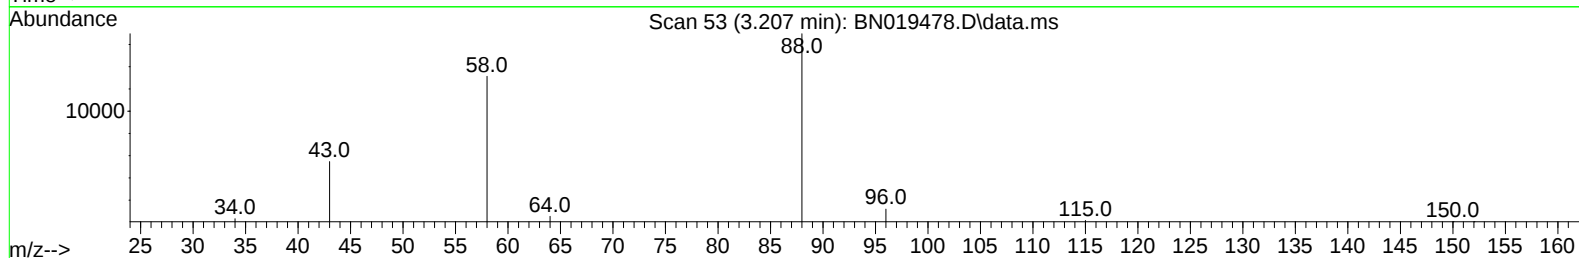


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
Data File : BN019478.D
Acq On : 18 Apr 2022 14:44
Operator : CG/JU
Sample : SST3.228
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Apr 18 15:21:58 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 18 15:02:34 2022
Response via : Initial Calibration

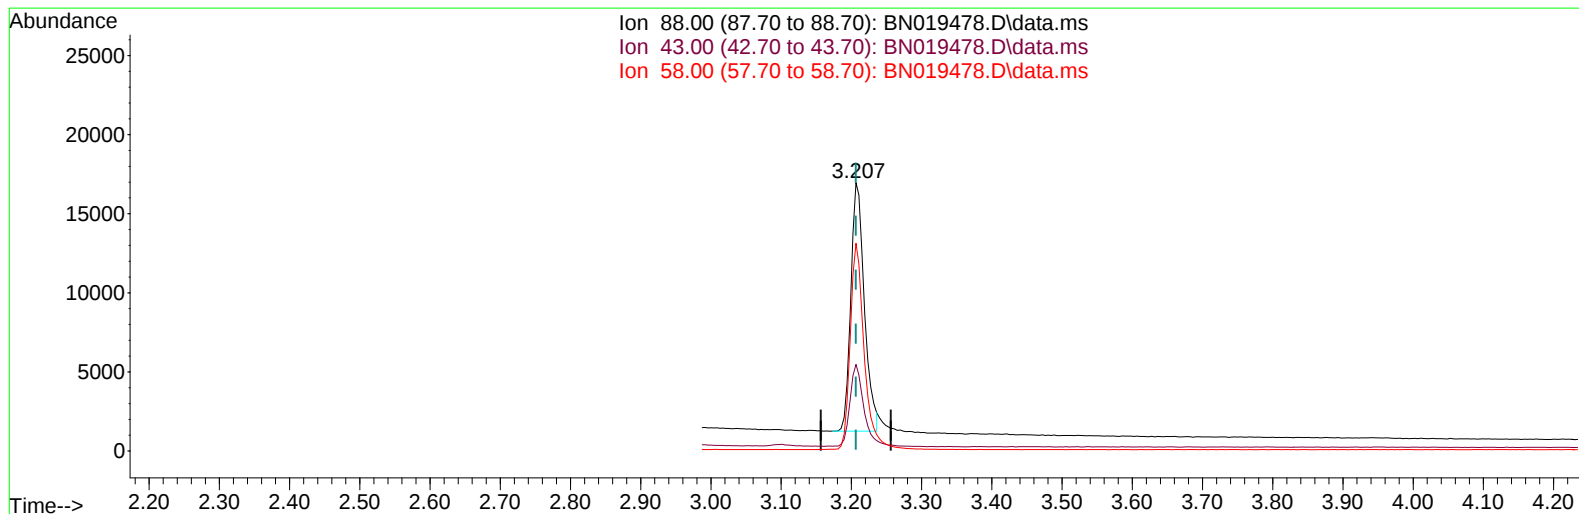

TIC: BN019478.D\data.ms

(2) 1,4-Dioxane

3.207min (-0.000) 2.77 ng/u1

response 21049

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	48.70	32.28#
58.00	49.80	77.41#
0.00	0.00	0.00