




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
 Data File : BN019478.D
 Acq On : 18 Apr 2022 14:44
 Operator : CG/JU
 Sample : SSTD3.228
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD3.2228

Manual IntegrationsAPPROVED

Quant Time: Apr 18 15:21:58 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 18 15:02:34 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/25/2022

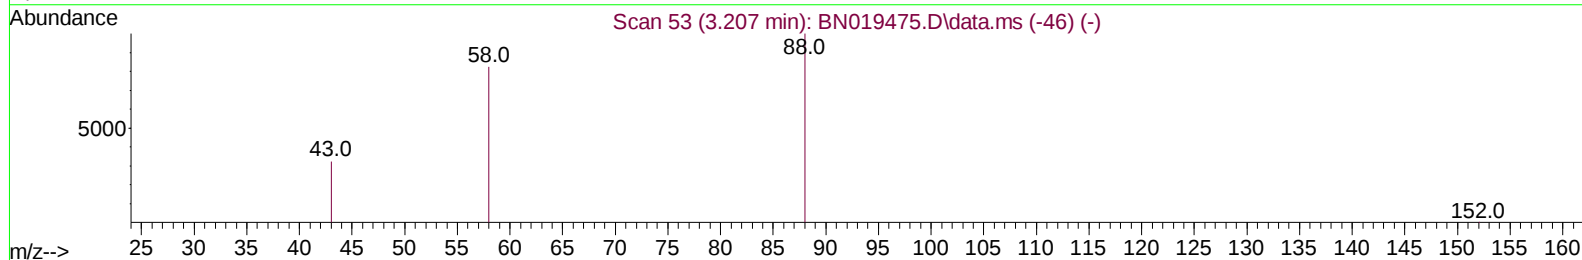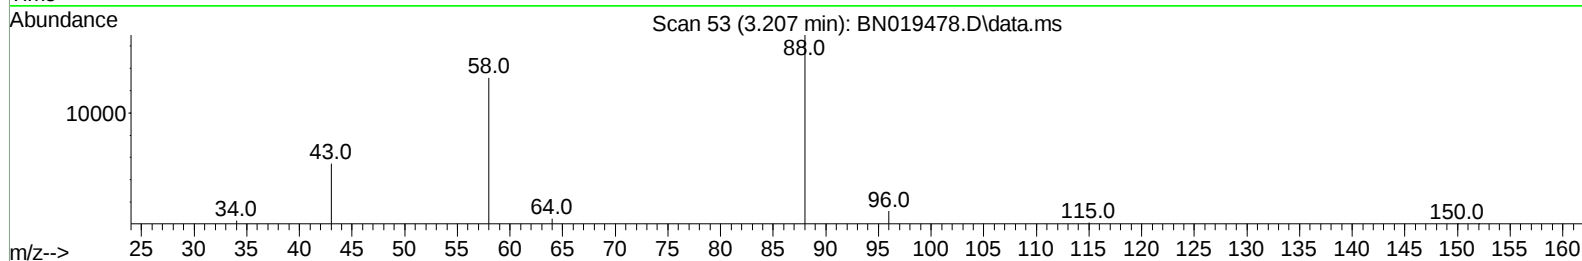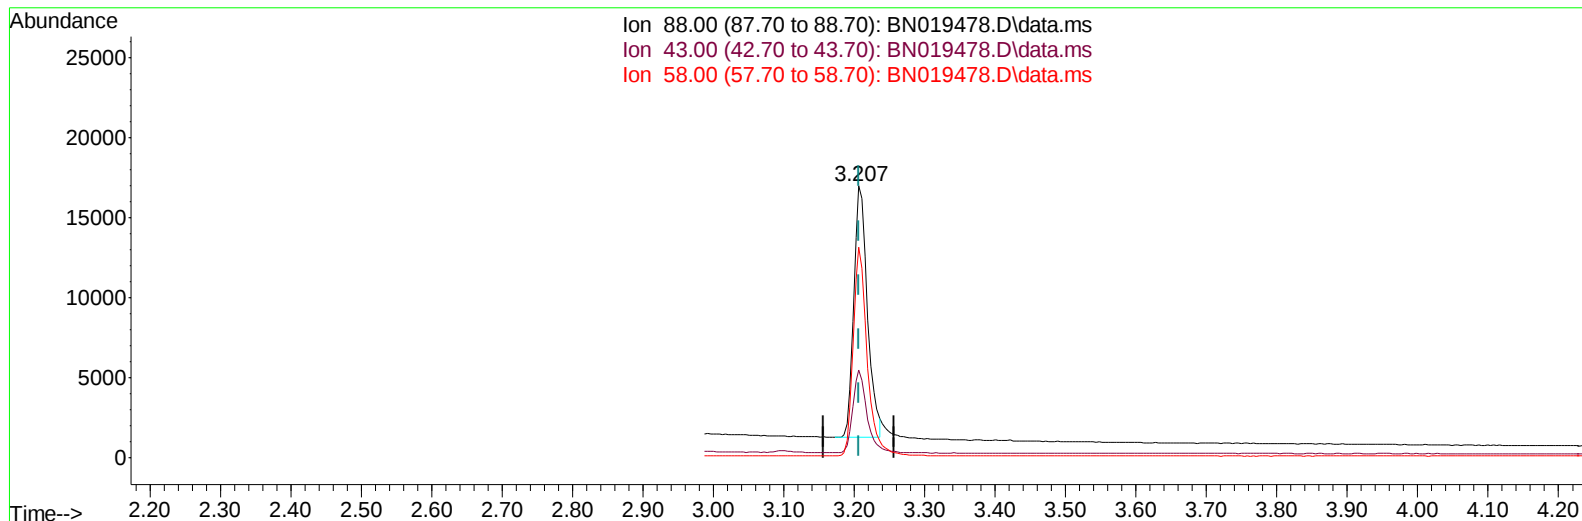

TIC: BN019478.D\data.ms

(2) 1,4-Dioxane

3.207min (-0.000) 2.77 ng/u1

response 21049

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	48.70	32.28#
58.00	49.80	77.41#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
Data File : BN019478.D
Acq On : 18 Apr 2022 14:44
Operator : CG/JU
Sample : SST3.228
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTD3.2228

Manual IntegrationsAPPROVED

Quant Time: Apr 18 15:21:58 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 18 15:02:34 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/25/2022

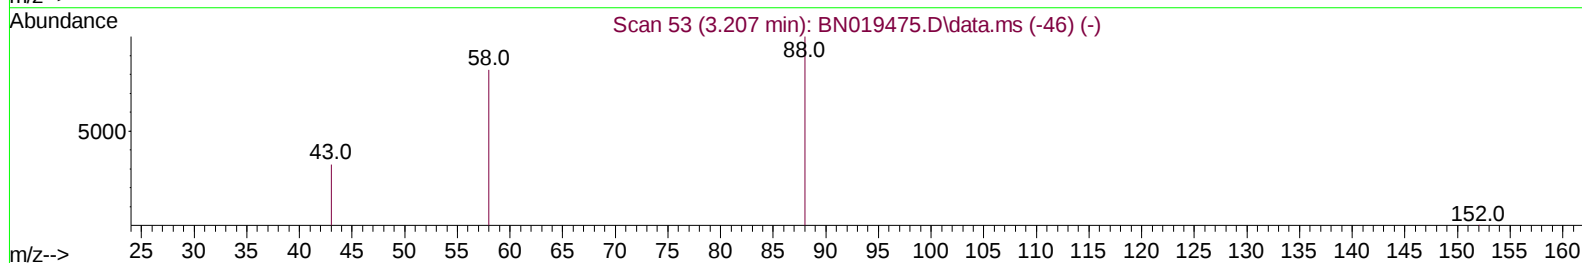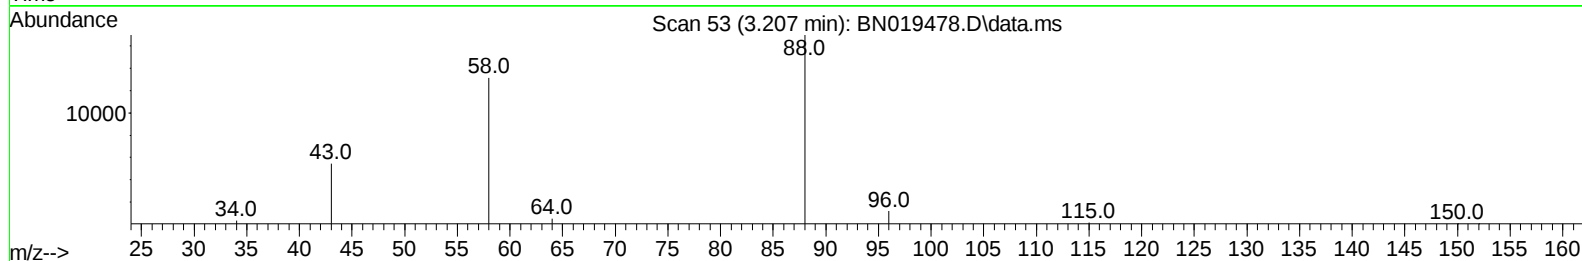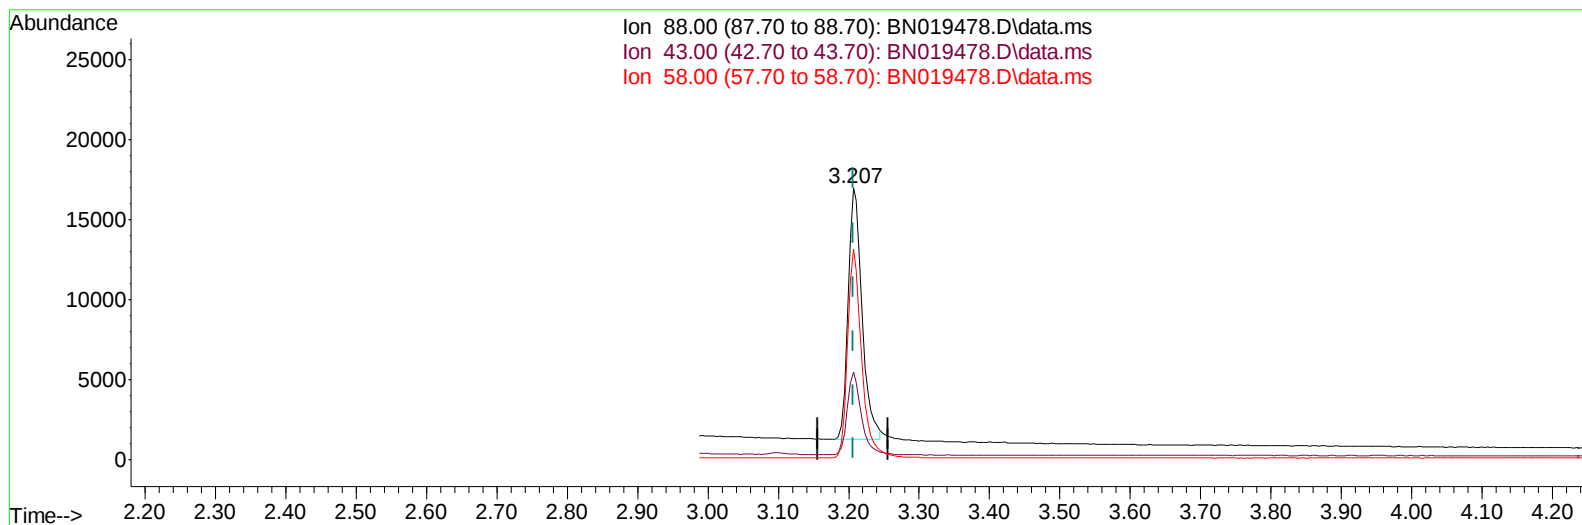

TIC: BN019478.D\data.ms

(2) 1,4-Dioxane

3.207min (-0.000) 2.82 ng/ul m

response 21390

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	48.70	32.28#
58.00	49.80	77.41#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
 Data File : BN019478.D
 Acq On : 18 Apr 2022 14:44
 Operator : CG/JU
 Sample : SSTD3.228
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD3.2228

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 18 15:21:58 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 18 15:02:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.818	152	6122	0.400	ng/ul	0.00
4) Naphthalene-d8	10.613	136	18570	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.457	164	10731	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.197	188	19916	0.400	ng/ul	0.00
17) Chrysene-d12	21.386	240	14662	0.400	ng/ul	0.00
23) Perylene-d12	23.736	264	9812	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.173	96	20592	2.614	ng/ul	0.00
6) 2-Methylnaphthalene-d10	0.000	152	0d	0.000	ng/ul	
18) Fluoranthene-d10	0.000	212	0d	0.000	ng/ul	
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.207	88	21390m	2.818	ng/ul	
14) Pentachlorophenol	16.855	266	10976	3.434	ng/ul	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
Data File : BN019478.D
Acq On : 18 Apr 2022 14:44
Operator : CG/JU
Sample : SSTD3.228
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTD3.2228

Manual IntegrationsAPPROVED

Quant Time: Apr 18 15:21:58 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 18 15:02:34 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/25/2022

