

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
 Data File : BN019480.D
 Acq On : 18 Apr 2022 15:58
 Operator : CG/JU
 Sample : PB144123BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK123

Manual IntegrationsAPPROVED

Quant Time: Apr 19 03:15:35 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 18 15:28:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut




Upadhyay

04/19/2022

Supervised By :Yogesh

Patel

04/25/2022

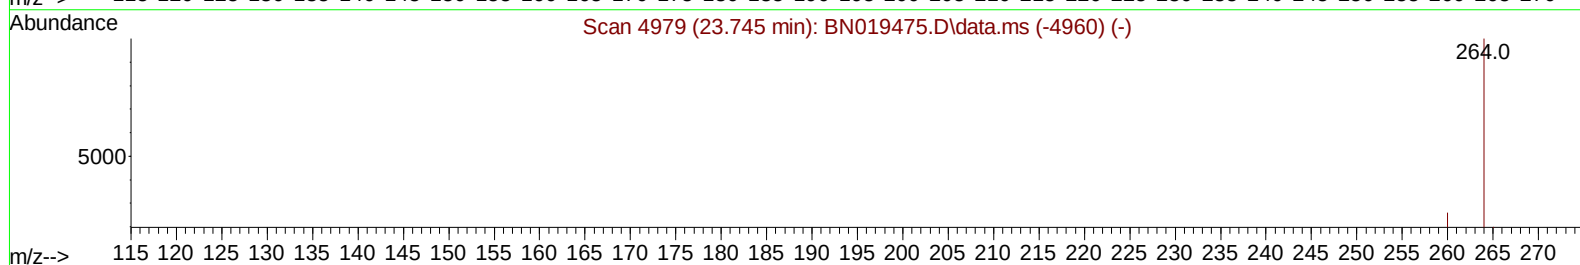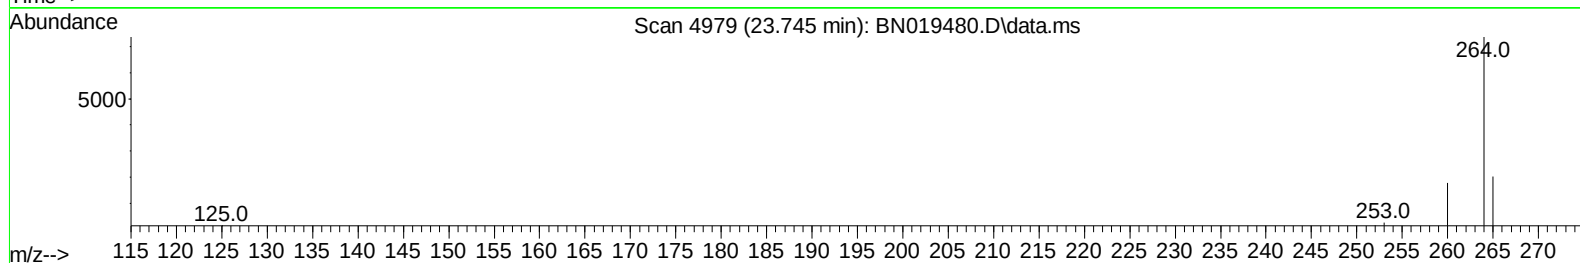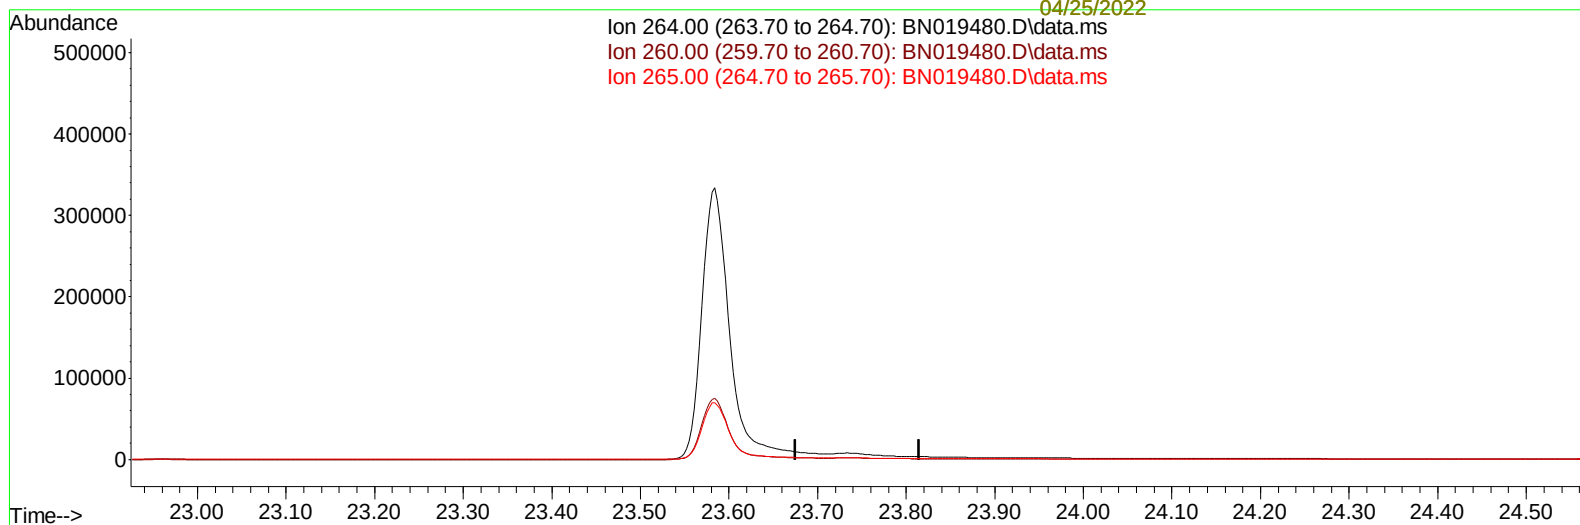

TIC: BN019480.D\data.ms

(23) Perylene-d12 (I)

23.745min (-23.745) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	28.30	0.00#
265.00	45.70	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
 Data File : BN019480.D
 Acq On : 18 Apr 2022 15:58
 Operator : CG/JU
 Sample : PB144123BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK123

Manual IntegrationsAPPROVED

Quant Time: Apr 19 03:15:35 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 18 15:28:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut




Upadhyay

04/19/2022

Supervised By :Yogesh

Patel

04/25/2022

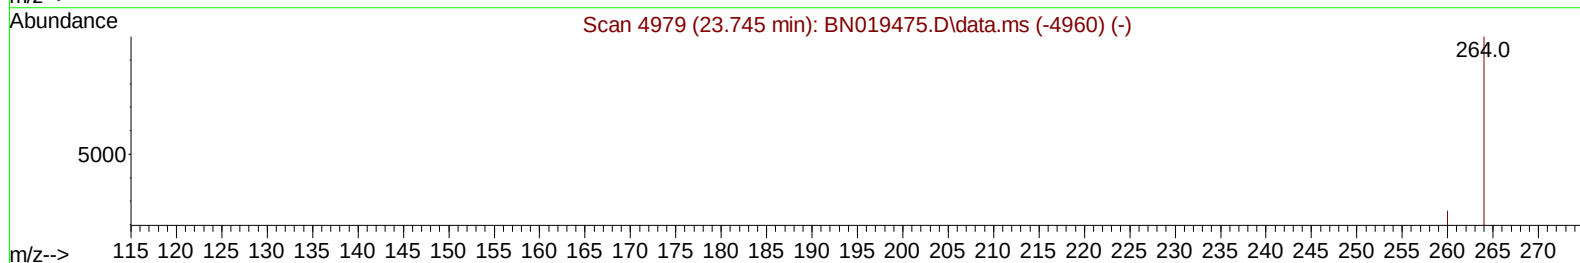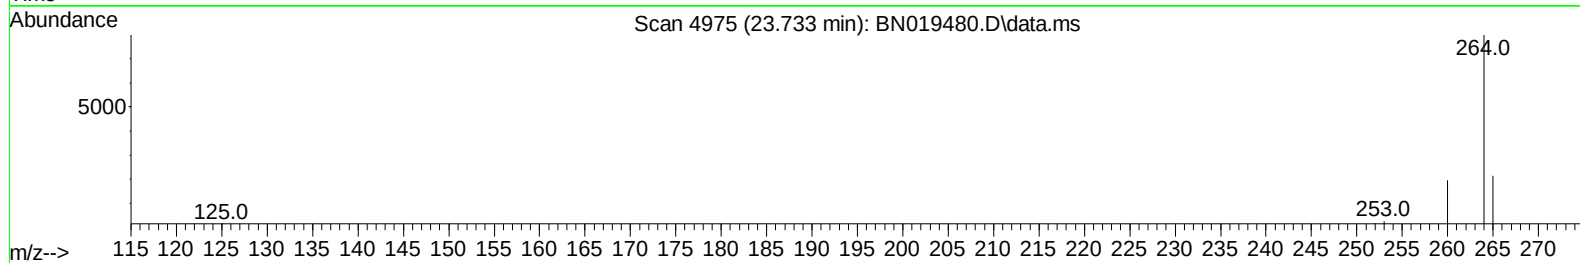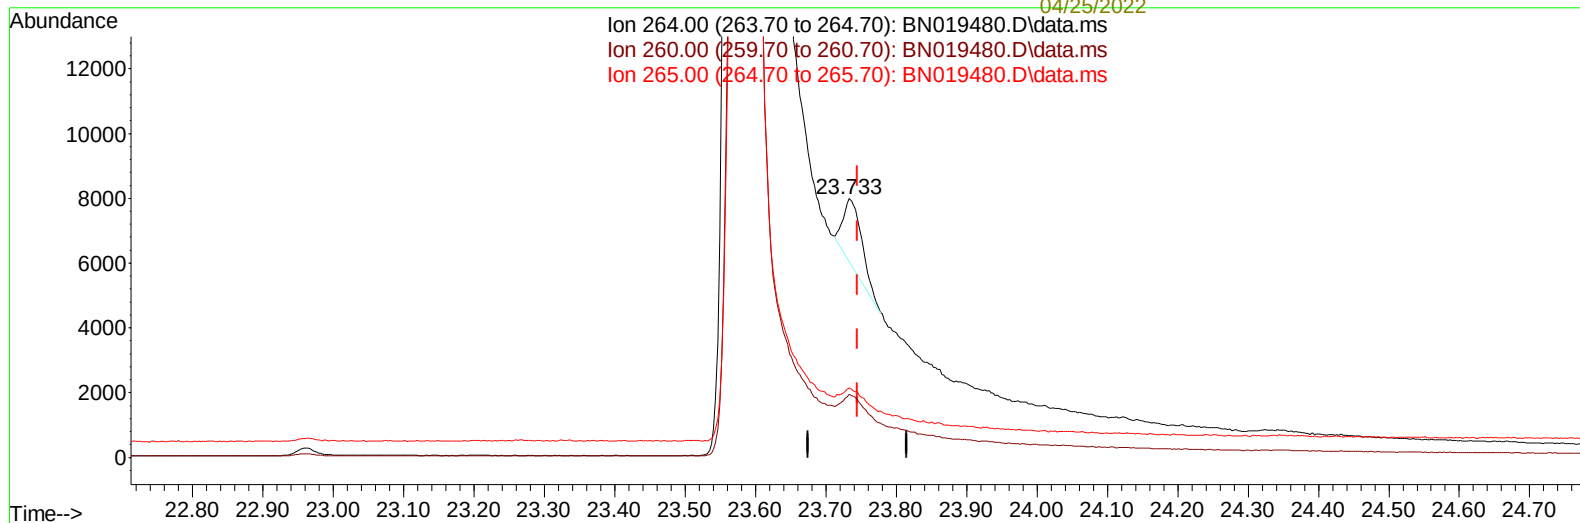

TIC: BN019480.D\data.ms

(23) Perylene-d12 (I)

23.733min (-0.012) 0.40 ng/ul m

response 3646

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	24.31
265.00	45.70	26.80#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
 Data File : BN019480.D
 Acq On : 18 Apr 2022 15:58
 Operator : CG/JU
 Sample : PB144123BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK123

Manual IntegrationsAPPROVED

Reviewed By :Jagrut
 Upadhyay
 04/19/2022

Supervised By :Yogesh
 Patel
 04/25/2022

Quant Time: Apr 19 03:15:35 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 18 15:28:08 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.814	152		4345	0.400	ng/ul	0.00
4) Naphthalene-d8	10.613	136		13103	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.457	164		7906	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.197	188		15123	0.400	ng/ul	0.00
17) Chrysene-d12	21.407	240		7576	0.400	ng/ul	0.01
23) Perylene-d12	23.733	264		3646m	0.400	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.169	96		33995	6.455	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.224	152		6844	0.389	ng/ul	0.00
18) Fluoranthene-d10	19.231	212		14069	0.455	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
Data File : BN019480.D
Acq On : 18 Apr 2022 15:58
Operator : CG/JU
Sample : PB144123BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK123

Manual IntegrationsAPPROVED

Quant Time: Apr 19 03:15:35 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 18 15:28:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut

Upadhyay

04/19/2022

Supervised By :Yogesh

Patel

04/25/2022

