




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
 Data File : BN019485.D
 Acq On : 18 Apr 2022 19:34
 Operator : CG/JU
 Sample : PB144173BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK173

Manual IntegrationsAPPROVED

Quant Time: Apr 19 03:06:08 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 18 15:28:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/25/2022

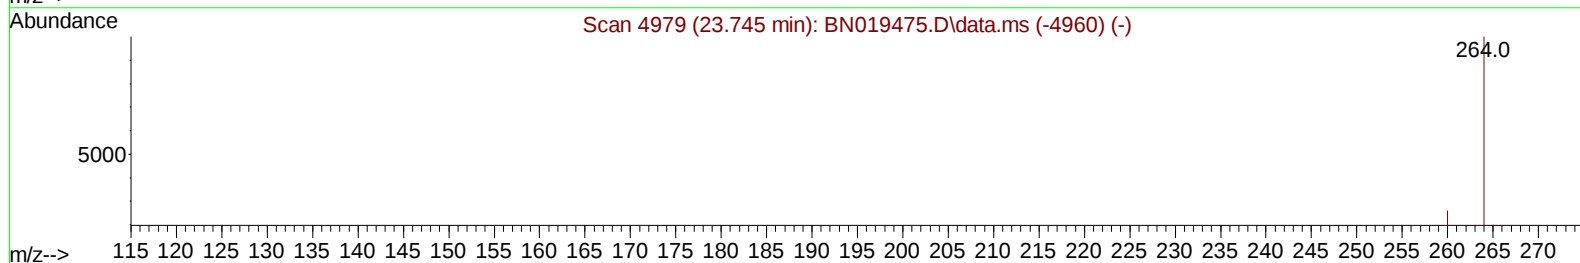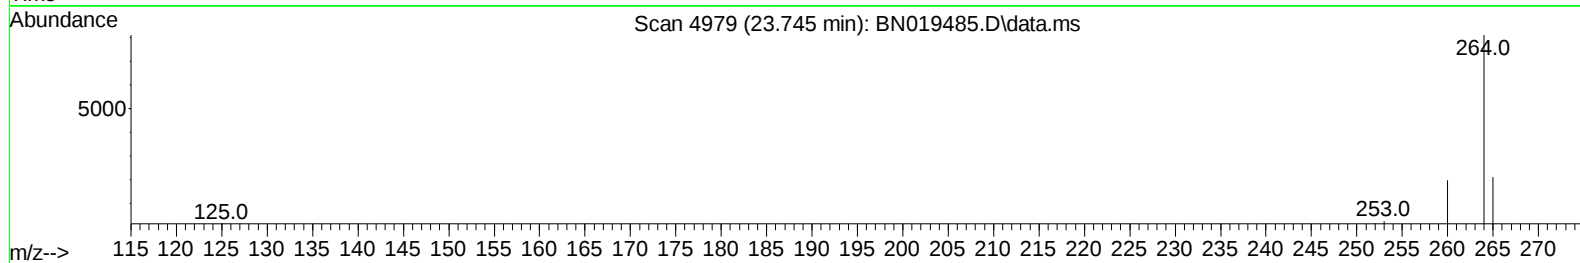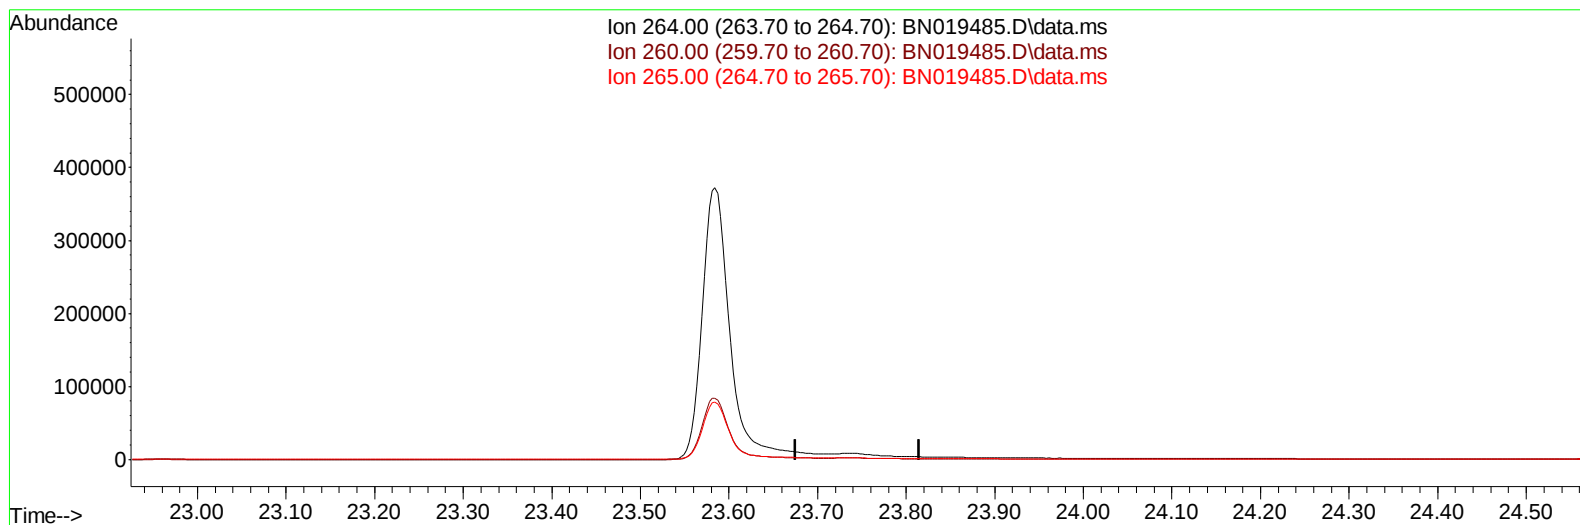

TIC: BN019485.D\data.ms

(23) Perylene-d12 (I)

23.745min (-23.745) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	28.30	0.00#
265.00	45.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
Data File : BN019485.D
Acq On : 18 Apr 2022 19:34
Operator : CG/JU
Sample : PB144173BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK173

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 19 03:06:08 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 18 15:28:08 2022
Response via : Initial Calibration

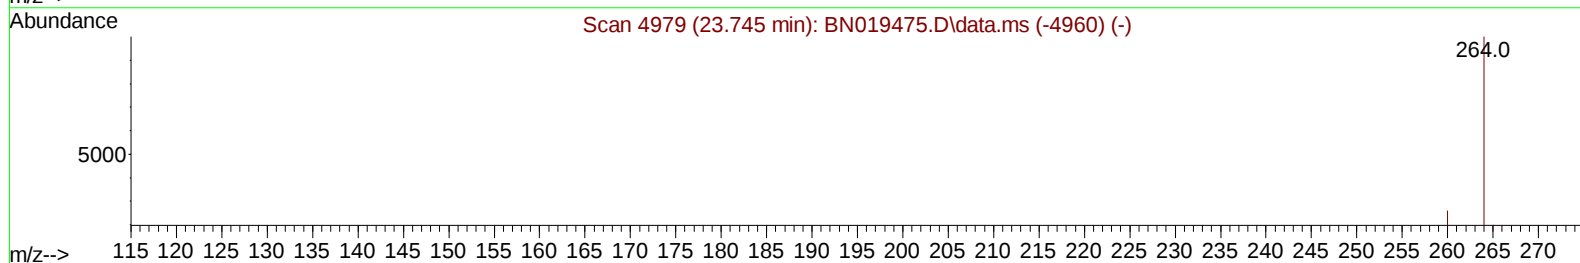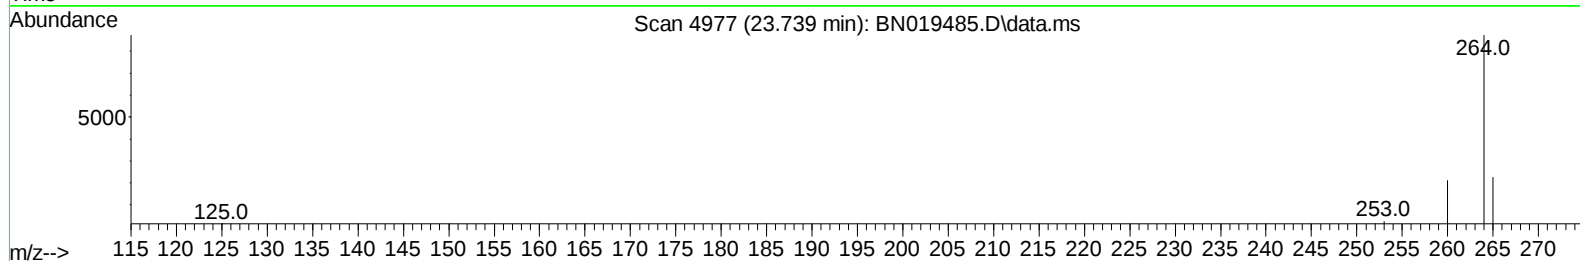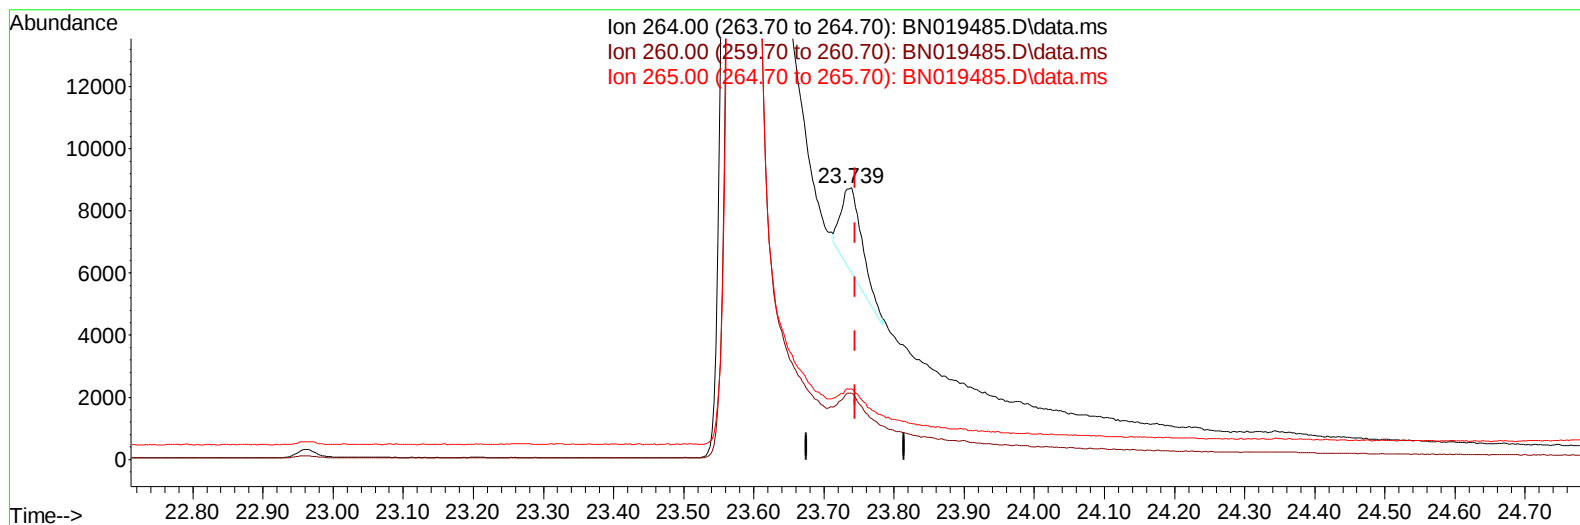

TIC: BN019485.D\data.ms

(23) Perylene-d12 (I)

23.739min (-0.006) 0.40 ng/ul m

response 5575

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	24.43
265.00	45.70	26.04#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
 Data File : BN019485.D
 Acq On : 18 Apr 2022 19:34
 Operator : CG/JU
 Sample : PB144173BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK173

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 19 03:06:08 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 18 15:28:08 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.814	152		5260	0.400	ng/ul	0.00
4) Naphthalene-d8	10.613	136		16044	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.457	164		9795	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.197	188		18813	0.400	ng/ul	0.00
17) Chrysene-d12	21.404	240		9218	0.400	ng/ul	0.00
23) Perylene-d12	23.739	264		5575m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.173	96		36132	5.667	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.224	152		7481	0.347	ng/ul	0.00
18) Fluoranthene-d10	19.231	212		15784	0.420	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
Data File : BN019485.D
Acq On : 18 Apr 2022 19:34
Operator : CG/JU
Sample : PB144173BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK173

Manual IntegrationsAPPROVED

Quant Time: Apr 19 03:06:08 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 18 15:28:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/25/2022

