




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
 Data File : BN019486.D
 Acq On : 18 Apr 2022 20:10
 Operator : CG/JU
 Sample : N2388-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFE5

Manual IntegrationsAPPROVED

Quant Time: Apr 19 03:06:16 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 18 15:28:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/25/2022

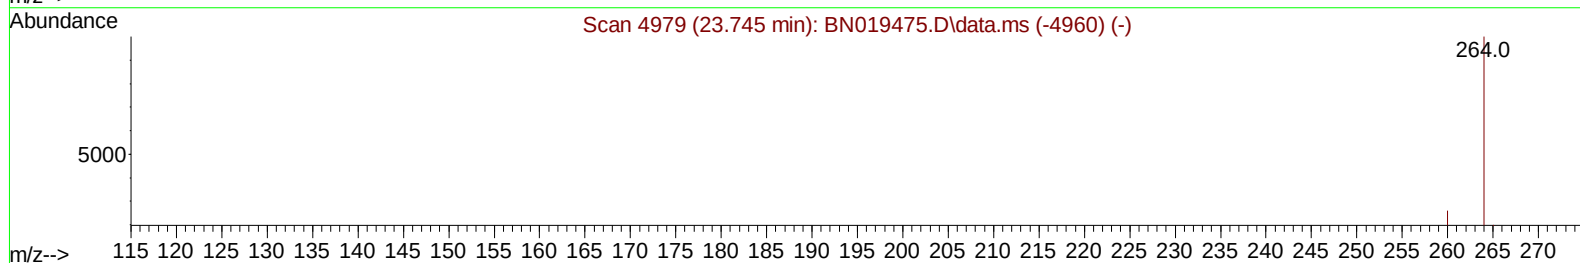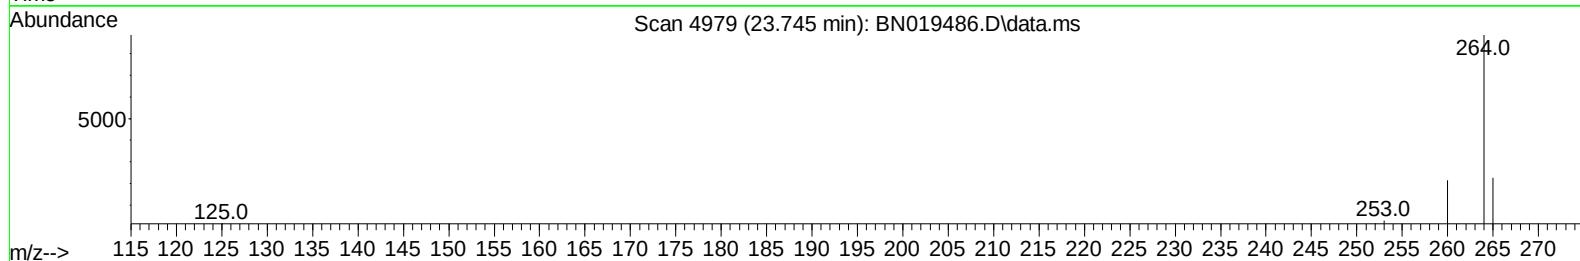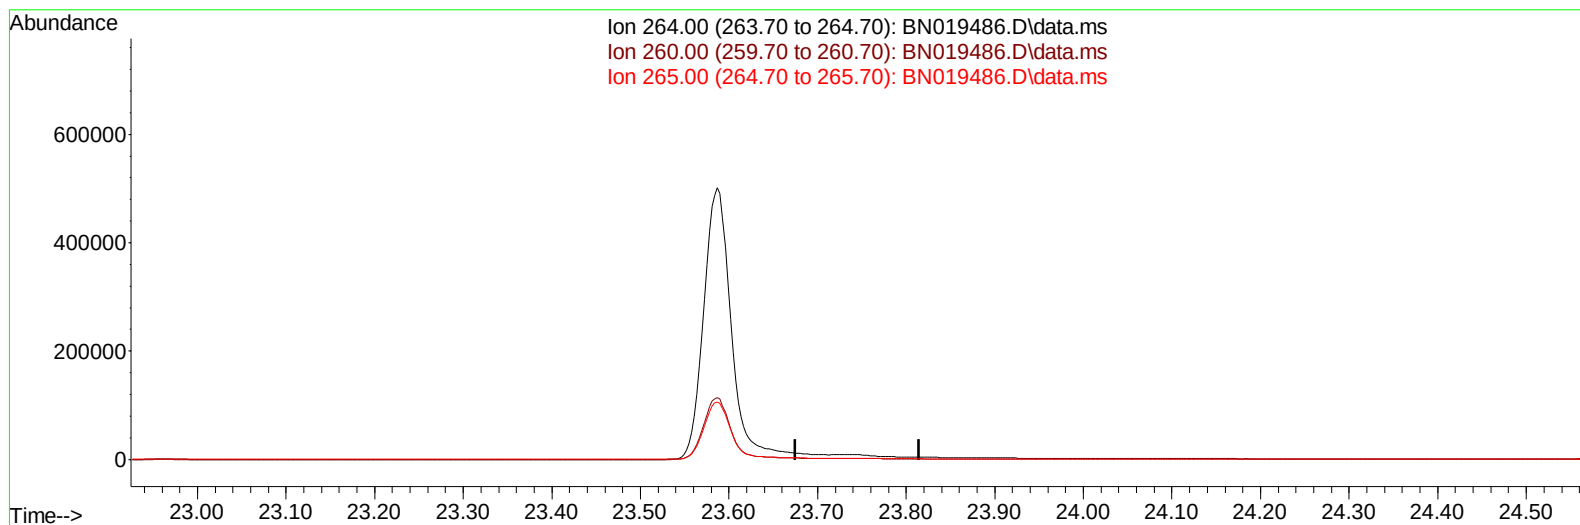

TIC: BN019486.D\data.ms

(23) Perylene-d12 (I)

23.745min (-23.745) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	28.30	0.00#
265.00	45.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
 Data File : BN019486.D
 Acq On : 18 Apr 2022 20:10
 Operator : CG/JU
 Sample : N2388-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFE5

Manual IntegrationsAPPROVED

Quant Time: Apr 19 03:06:16 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 18 15:28:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/25/2022

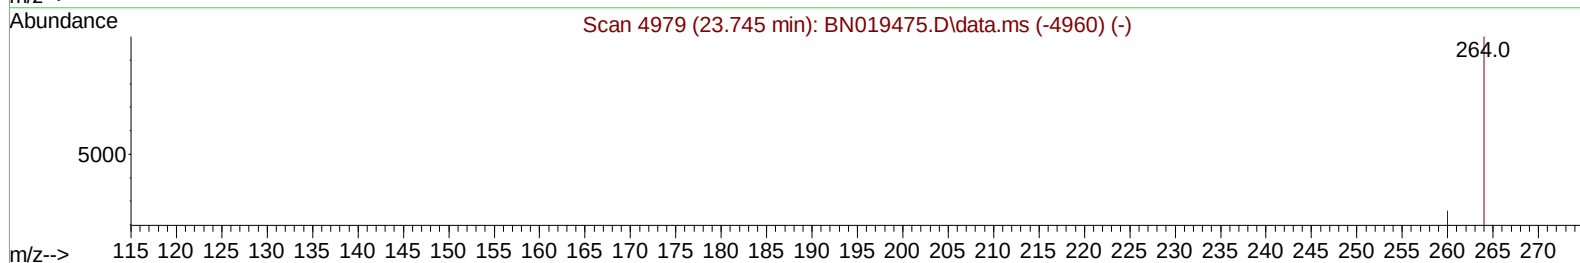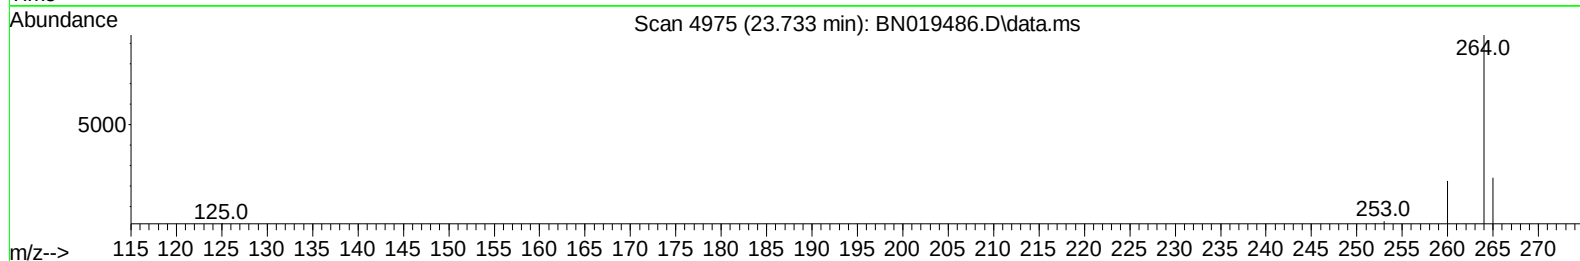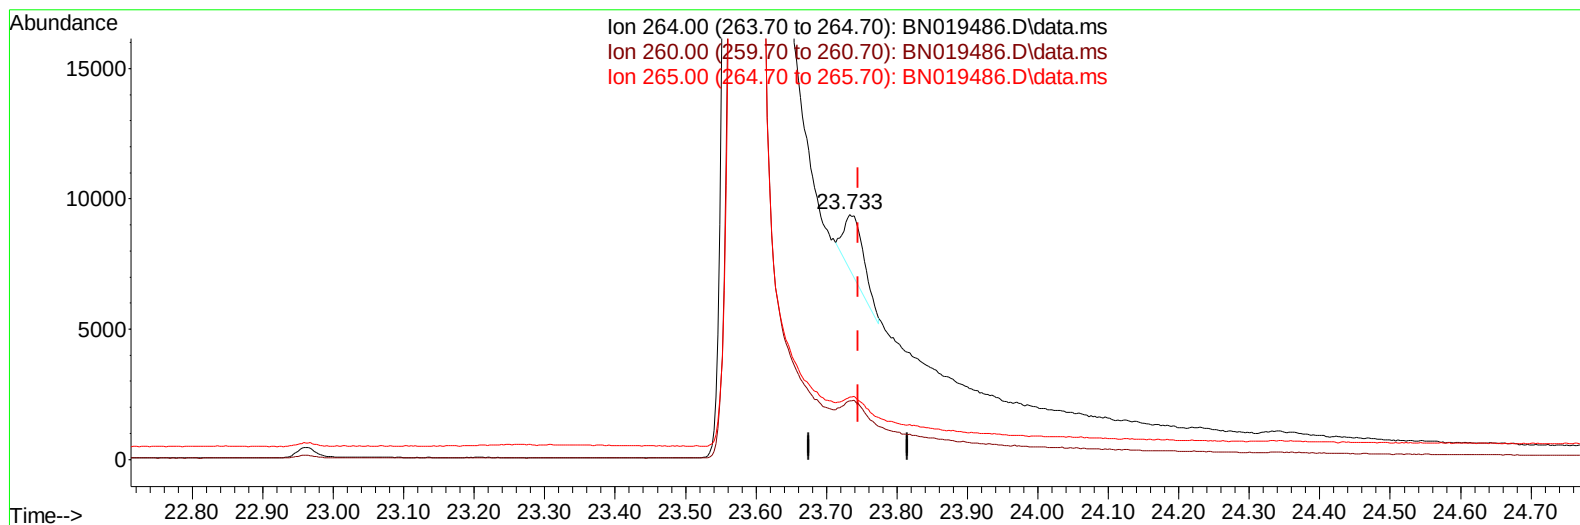

TIC: BN019486.D\data.ms

(23) Perylene-d12 (I)

23.733min (-0.012) 0.40 ng/ul m

response 4354

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	23.91
265.00	45.70	25.52#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
 Data File : BN019486.D
 Acq On : 18 Apr 2022 20:10
 Operator : CG/JU
 Sample : N2388-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFE5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 19 03:06:16 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 18 15:28:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.814	152	4384	0.400	ng/ul	0.00
4) Naphthalene-d8	10.613	136	13267	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.457	164	8590	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.197	188	16393	0.400	ng/ul	0.00
17) Chrysene-d12	21.398	240	8499	0.400	ng/ul	0.00
23) Perylene-d12	23.733	264	4354m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.173	96	35417	6.665	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.213	152	10258	0.576	ng/ul	0.00
18) Fluoranthene-d10	19.231	212	23016	0.664	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.662	128	1522	0.040	ng/ul#	88
7) 2-Methylnaphthalene	12.290	142	526	0.022	ng/ul#	100
27) Indeno(1,2,3-cd)pyrene	26.212	276	550	0.030	ng/ul#	52
28) Dibenzo(a,h)anthracene	26.216	278	486	0.040	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
Data File : BN019486.D
Acq On : 18 Apr 2022 20:10
Operator : CG/JU
Sample : N2388-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFFE5

Manual IntegrationsAPPROVED

Quant Time: Apr 19 03:06:16 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 18 15:28:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/25/2022

