




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
 Data File : BN019490.D
 Acq On : 18 Apr 2022 22:33
 Operator : CG/JU
 Sample : N2388-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFE8

Manual IntegrationsAPPROVED

Quant Time: Apr 19 03:07:06 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 18 15:28:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/25/2022

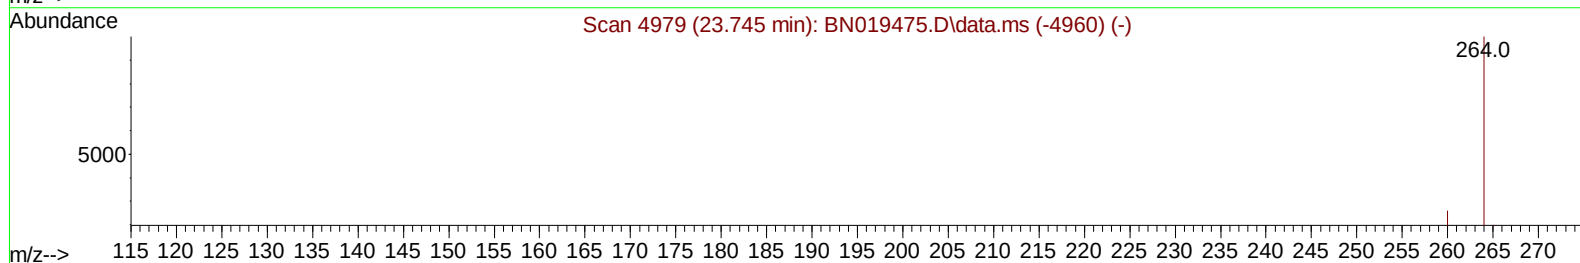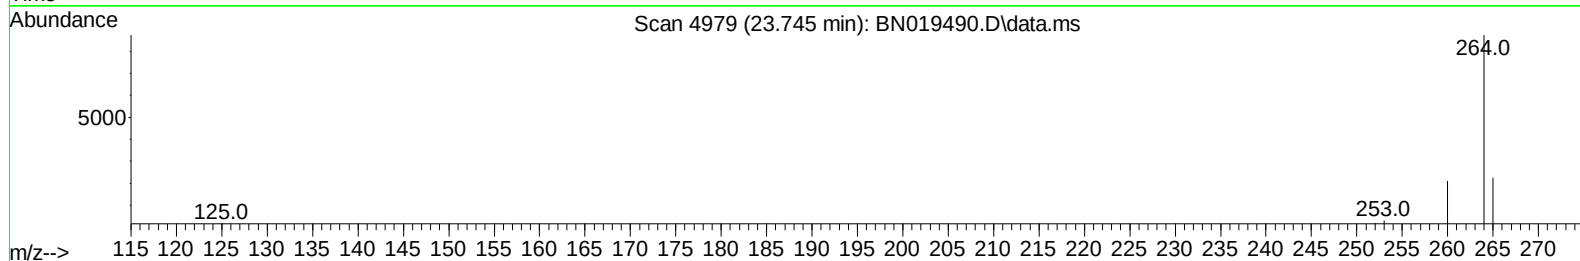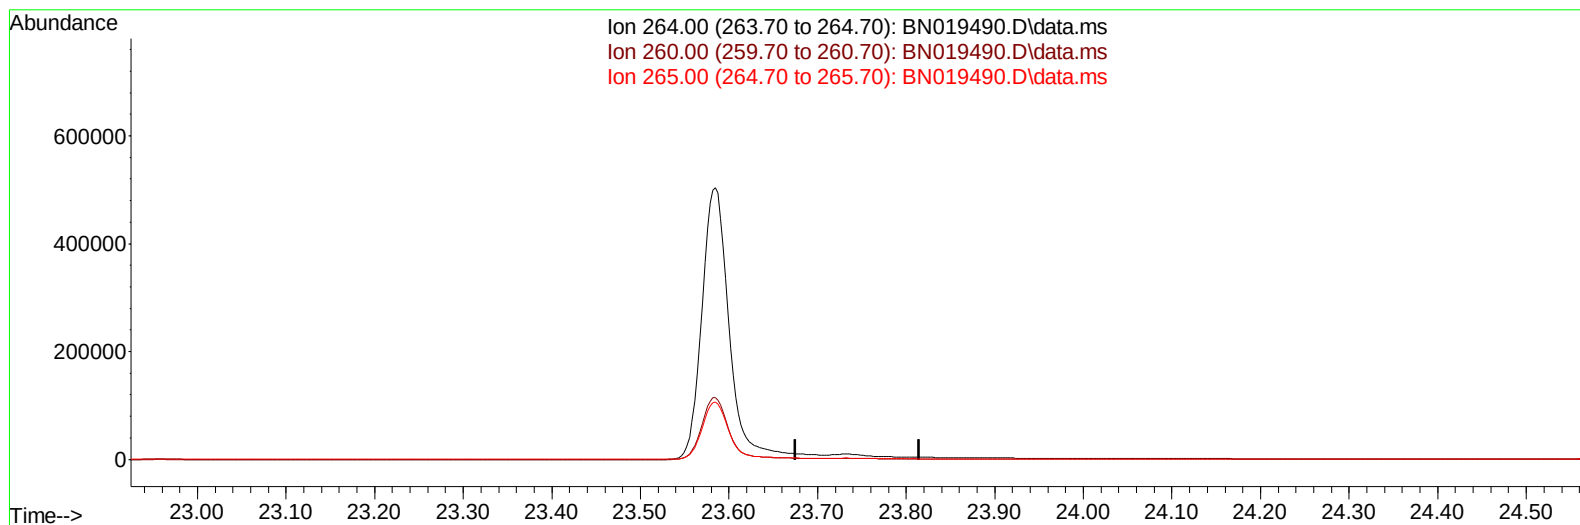

TIC: BN019490.D\data.ms

(23) Perylene-d12 (I)

23.745min (-23.745) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	28.30	0.00#
265.00	45.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
 Data File : BN019490.D
 Acq On : 18 Apr 2022 22:33
 Operator : CG/JU
 Sample : N2388-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFE8

Manual IntegrationsAPPROVED

Quant Time: Apr 19 03:07:06 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 18 15:28:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/25/2022

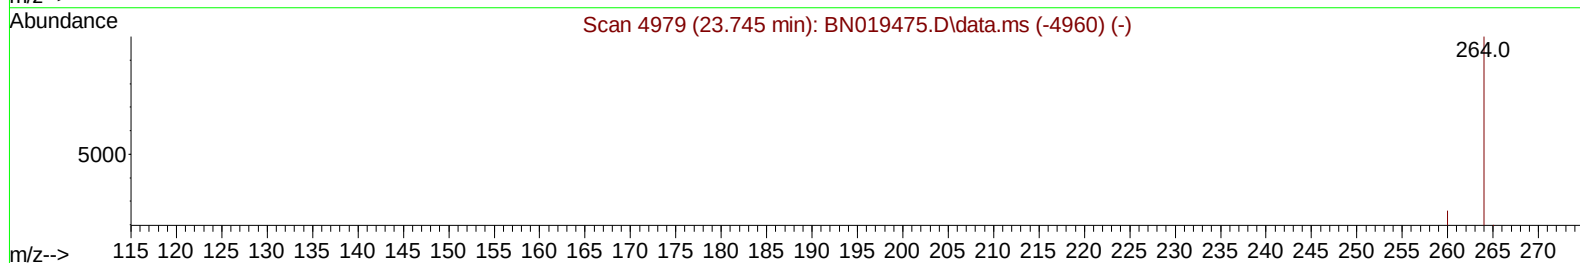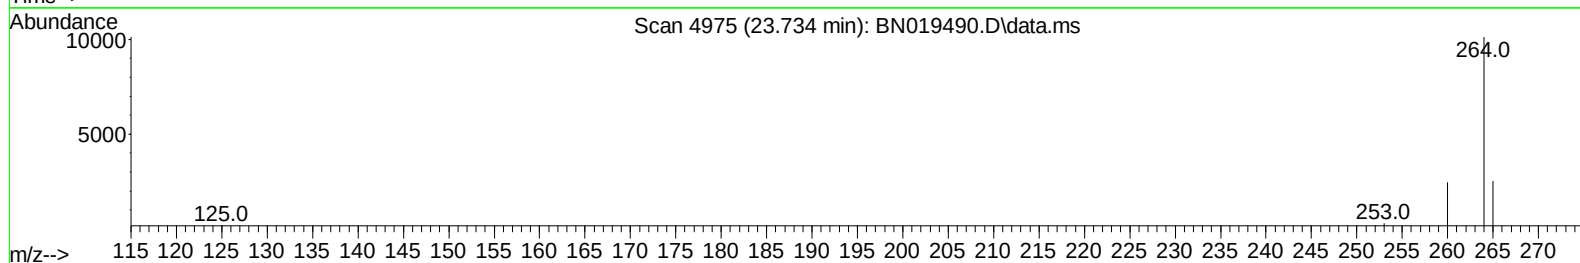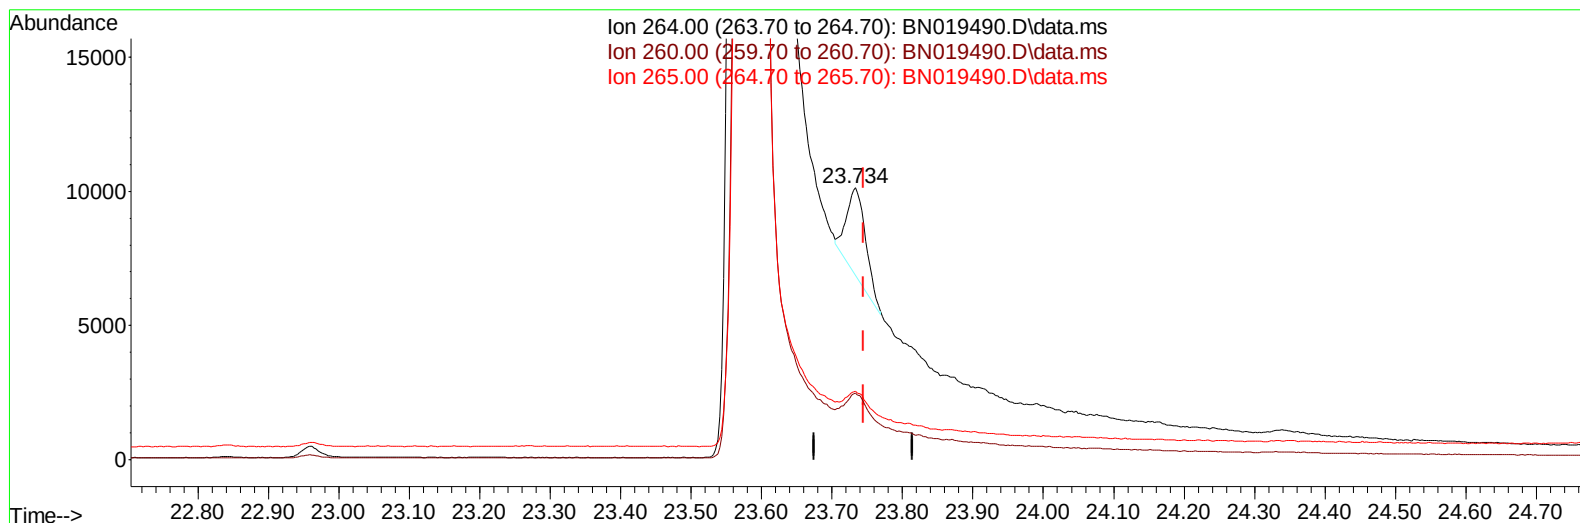

TIC: BN019490.D\data.ms

(23) Perylene-d12 (I)

23.734min (-0.011) 0.40 ng/ul m

response 5928

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	24.42
265.00	45.70	25.08#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
 Data File : BN019490.D
 Acq On : 18 Apr 2022 22:33
 Operator : CG/JU
 Sample : N2388-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFFE8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/19/2022
 Supervised By :Yogesh Patel 04/25/2022

Quant Time: Apr 19 03:07:06 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 18 15:28:08 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.814	152		3465	0.400	ng/ul	0.00
4) Naphthalene-d8	10.611	136		10635	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.455	164		6967	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.200	188		14509	0.400	ng/ul	0.00
17) Chrysene-d12	21.395	240		9277	0.400	ng/ul	0.00
23) Perylene-d12	23.734	264		5928m	0.400	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.169	96		24052	5.727	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.217	152		6889	0.483	ng/ul	0.00
18) Fluoranthene-d10	19.229	212		19071	0.504	ng/ul	0.00
Target Compounds							Qvalue
5) Naphthalene	10.666	128		1002	0.033	ng/ul#	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041822\
Data File : BN019490.D
Acq On : 18 Apr 2022 22:33
Operator : CG/JU
Sample : N2388-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFFE8

Manual IntegrationsAPPROVED

Quant Time: Apr 19 03:07:06 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 18 15:28:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/19/2022
Supervised By :Yogesh Patel 04/25/2022

