

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041823\
 Data File : BN024984.D
 Acq On : 18 Apr 2023 18:31
 Operator : CG/JU
 Sample : 02355-02DL 2X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BP-TT-RW5B-20230413DL

Quant Time: Apr 18 19:02:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN040523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 18 05:29:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.933	152	11544	0.400	ng	0.00
7) Naphthalene-d8	10.750	136	34944	0.400	ng	0.00
13) Acenaphthene-d10	14.576	164	18907	0.400	ng	0.00
19) Phenanthrene-d10	17.323	188	38990	0.400	ng	0.00
29) Chrysene-d12	21.518	240	31650	0.400	ng	# 0.00
35) Perylene-d12	23.968	264	26584	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.492	112	1820	0.068	ng	0.00
5) Phenol-d6	7.109	99	1226	0.036	ng	0.00
8) Nitrobenzene-d5	9.106	82	4194	0.149	ng	0.00
11) 2-Methylnaphthalene-d10	12.332	152	7688	0.166	ng	0.00
14) 2,4,6-Tribromophenol	16.070	330	1241	0.146	ng	0.00
15) 2-Fluorobiphenyl	13.208	172	11800	0.163	ng	0.00
27) Fluoranthene-d10	19.355	212	18031	0.204	ng	0.00
31) Terphenyl-d14	19.953	244	16899	0.236	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.339	88	39986	3.152	ng	Qvalue 97
6) bis(2-Chloroethyl)ether	7.362	93	848	0.025	ng	93
20) 4,6-Dinitro-2-methylph...	15.699	198	2	0.175	ng	# 1
24) Pentachlorophenol	16.988	266	44	0.222	ng	# 70
34) Bis(2-ethylhexyl)phtha...	21.428	149	6104	0.106	ng	# 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041823\
Data File : BN024984.D
Acq On : 18 Apr 2023 18:31
Operator : CG/JU
Sample : 02355-02DL 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BP-TT-RW5B-20230413DL


Quant Time: Apr 18 19:02:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN040523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 05:29:26 2023
Response via : Initial Calibration

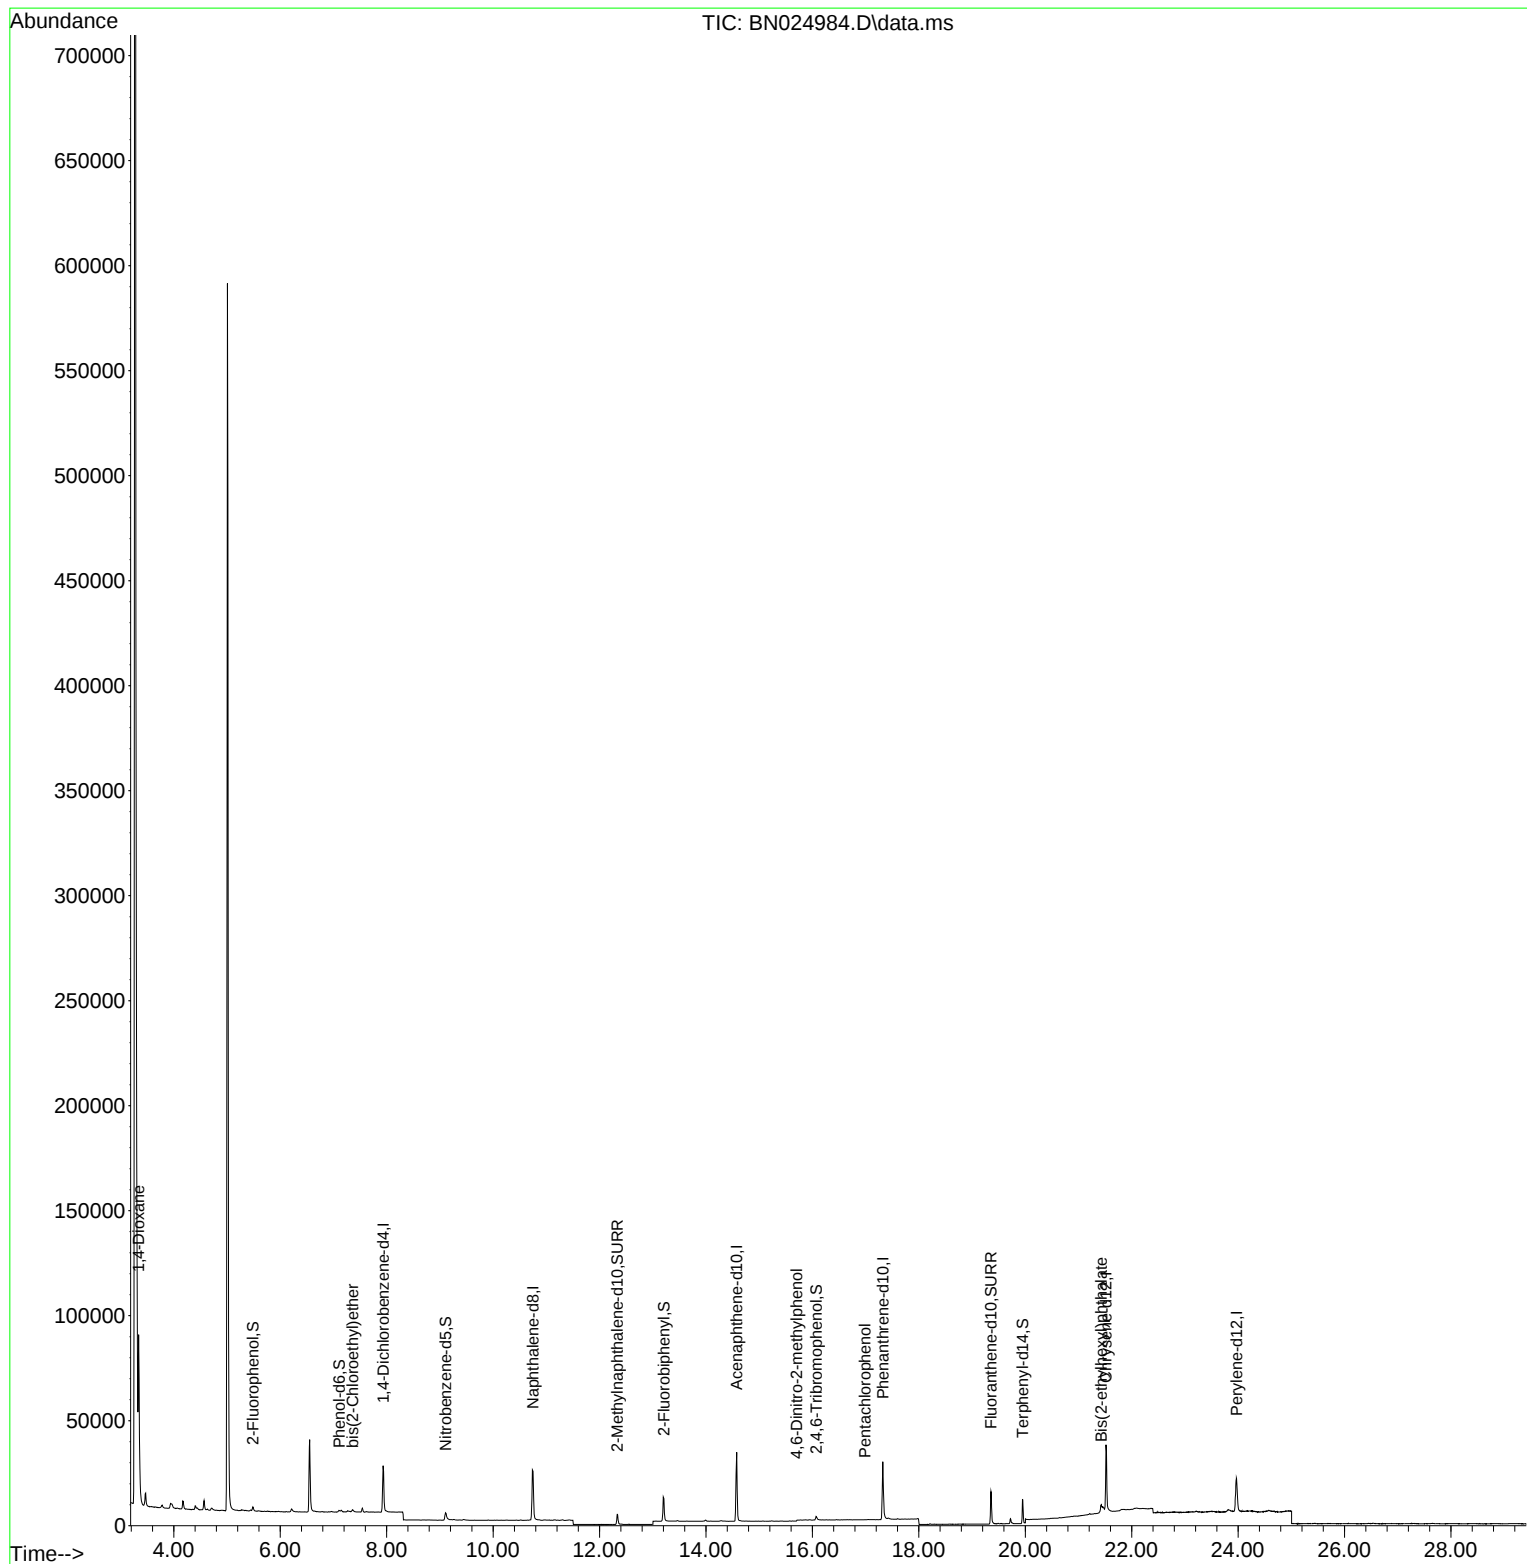



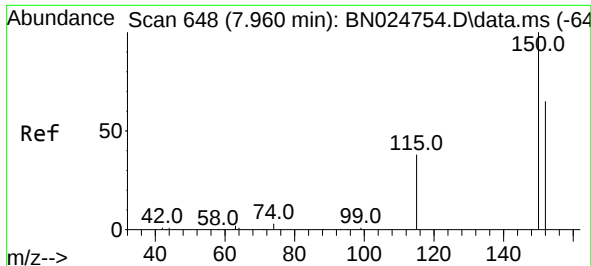


#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.933 min Scan# 61
Delta R.T. -0.007 min
Lab File: BN024984.D
Acq: 18 Apr 2023 18:31

Instrument :
BNA_N
ClientSampleId :
BP-TT-RW5B-20230413DL



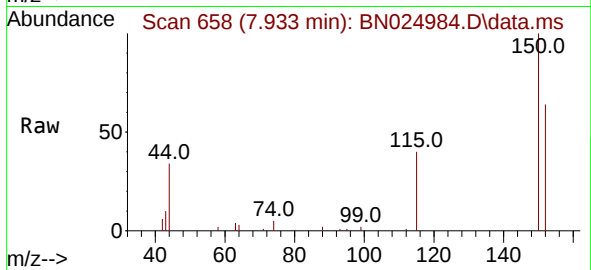



Tgt Ion:152 Resp: 11544
Ion Ratio Lower Upper
152 100
150 156.6 121.8 182.8
115 62.6 48.3 72.5

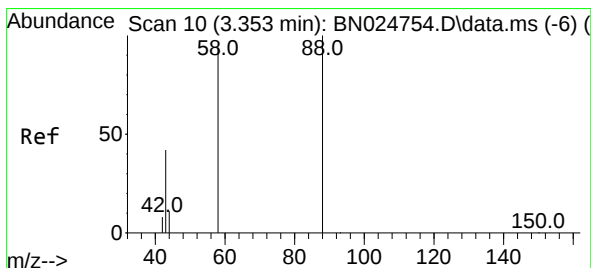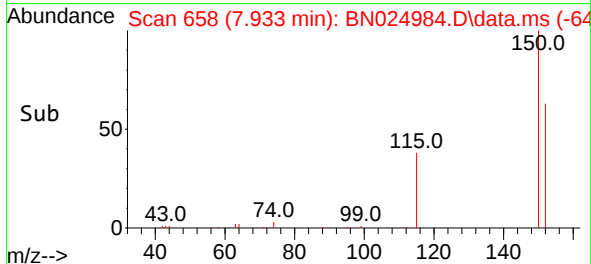

#2
1,4-Dioxane
Concen: 3.152 ng
RT: 3.339 min Scan# 22
Delta R.T. -0.007 min
Lab File: BN024984.D
Acq: 18 Apr 2023 18:31

Tgt Ion: 88 Resp: 39986
Ion Ratio Lower Upper
88 100
43 40.7 35.2 52.8
58 88.1 71.4 107.2


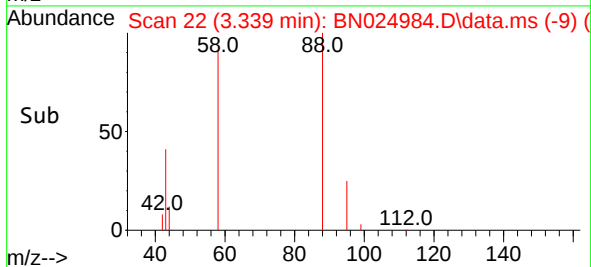

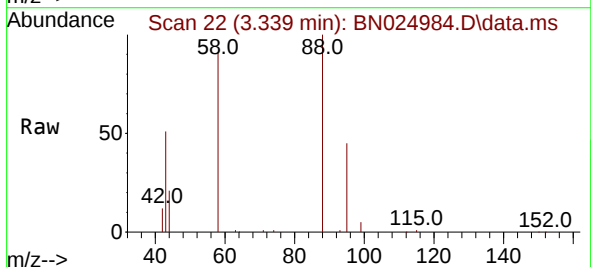


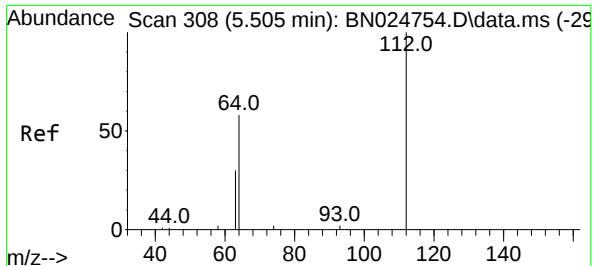

#4
2-Fluorophenol
Concen: 0.068 ng
RT: 5.492 min Scan# 31
Delta R.T. -0.000 min
Lab File: BN024984.D
Acq: 18 Apr 2023 18:31




Instrument :
BNA_N
ClientSampleId :
BP-TT-RW5B-20230413DL


Tgt Ion:	112	Resp:	1820
Ion	Ratio	Lower	Upper
112	100		
64	64.9	52.5	78.7
63	38.4	27.9	41.9

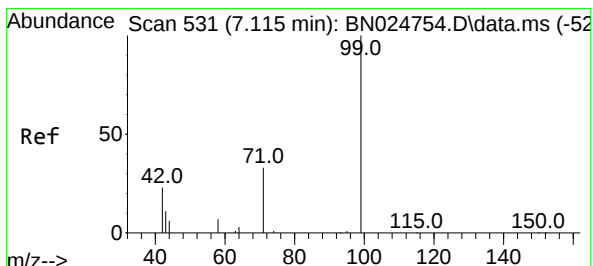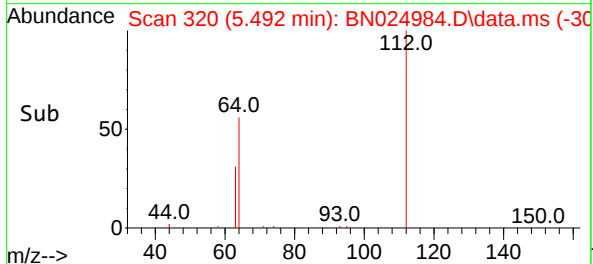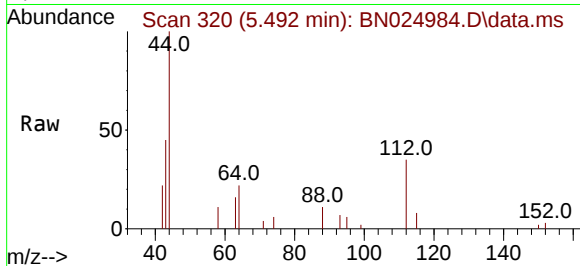

#5
Phenol-d6
Concen: 0.036 ng
RT: 7.109 min Scan# 544
Delta R.T. 0.007 min
Lab File: BN024984.D
Acq: 18 Apr 2023 18:31

Tgt Ion:	99	Resp:	1226
Ion	Ratio	Lower	Upper
99	100		
42	25.0	22.8	34.2
71	39.9	28.2	42.2


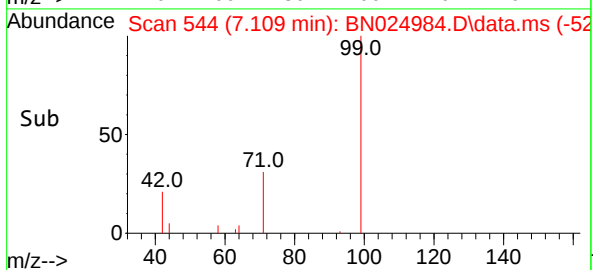

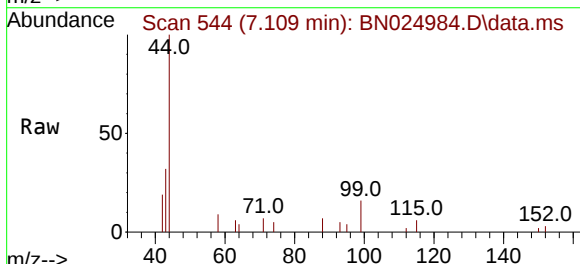


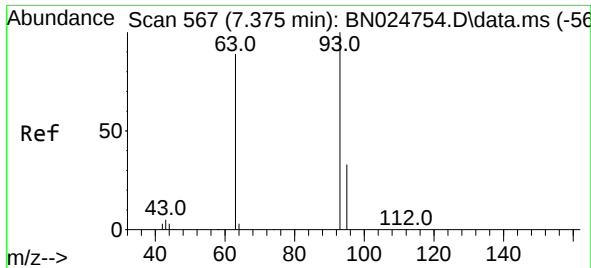

#6
bis(2-Chloroethyl)ether
Concen: 0.025 ng
RT: 7.362 min Scan# 51
Delta R.T. -0.000 min
Lab File: BN024984.D
Acq: 18 Apr 2023 18:31




Instrument :
BNA_N
ClientSampleId :
BP-TT-RW5B-20230413DL


Tgt Ion: 93 Resp: 848
Ion Ratio Lower Upper
93 100
63 79.0 68.8 103.2
95 33.8 25.4 38.2

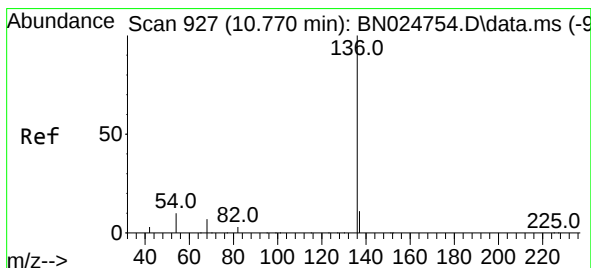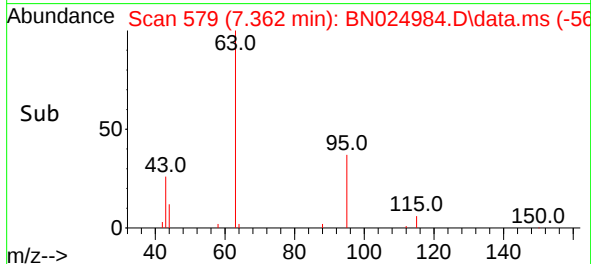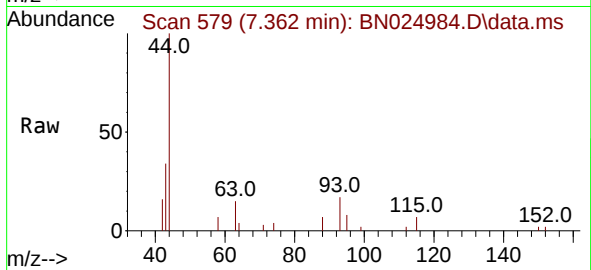

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.750 min Scan# 939
Delta R.T. -0.000 min
Lab File: BN024984.D
Acq: 18 Apr 2023 18:31

Tgt Ion:136 Resp: 34944
Ion Ratio Lower Upper
136 100
137 11.0 8.9 13.3
54 9.4 8.2 12.4
68 6.3 5.8 8.6


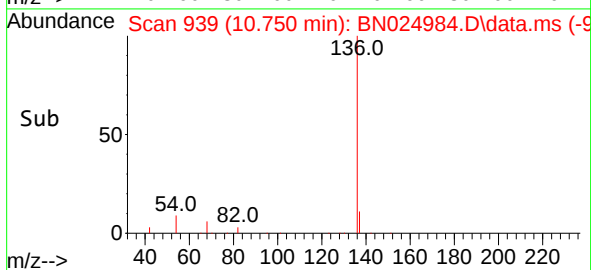

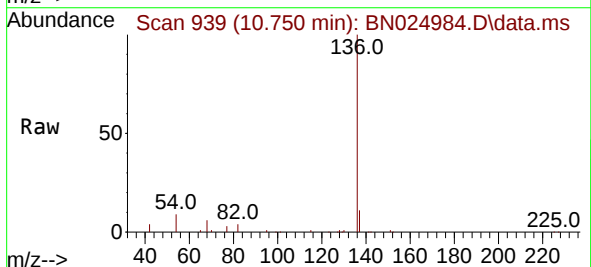


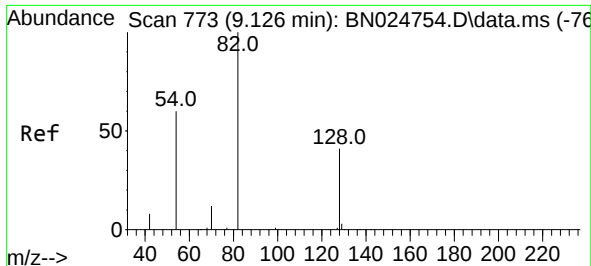

#8
Nitrobenzene-d5
Concen: 0.149 ng
RT: 9.106 min Scan# 71
Delta R.T. -0.000 min
Lab File: BN024984.D
Acq: 18 Apr 2023 18:31




Instrument :
BNA_N
ClientSampleId :
BP-TT-RW5B-20230413DL


Tgt Ion: 82 Resp: 4194
Ion Ratio Lower Upper
82 100
128 40.4 33.8 50.6
54 74.1 49.4 74.0#

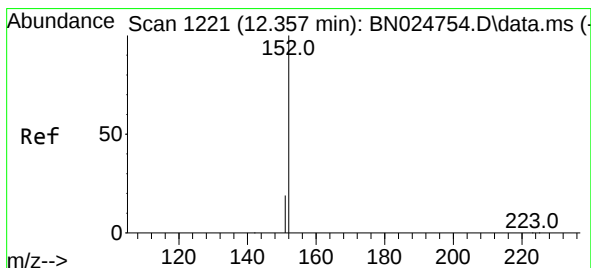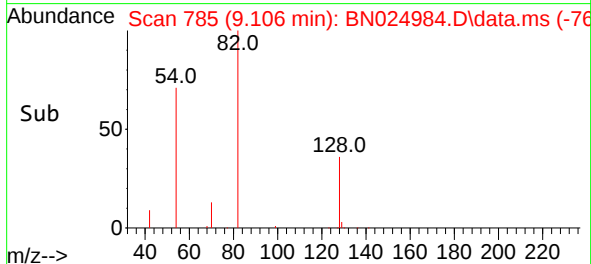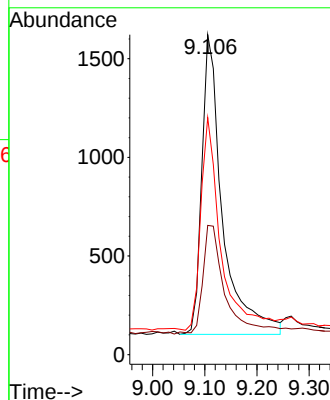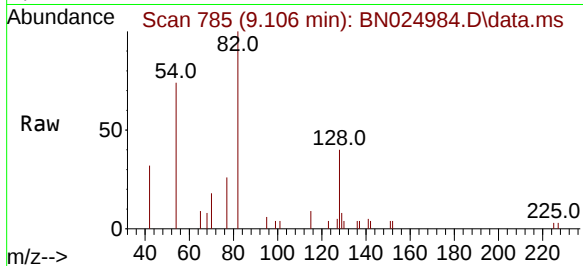

#11
2-Methylnaphthalene-d10
Concen: 0.166 ng
RT: 12.332 min Scan# 1228
Delta R.T. -0.004 min
Lab File: BN024984.D
Acq: 18 Apr 2023 18:31

Tgt Ion: 152 Resp: 7688
Ion Ratio Lower Upper
152 100
151 21.5 16.6 25.0


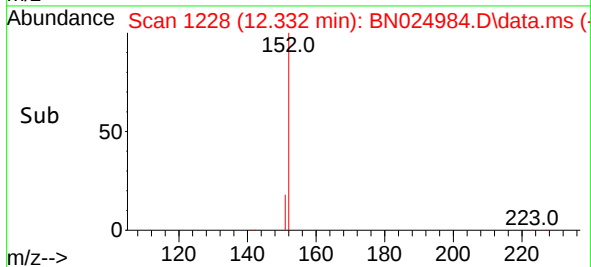
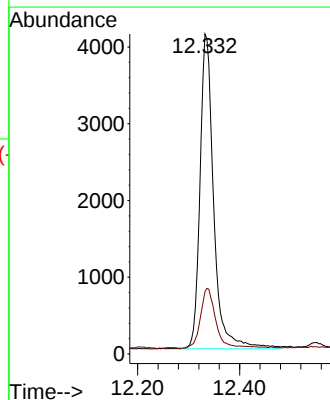
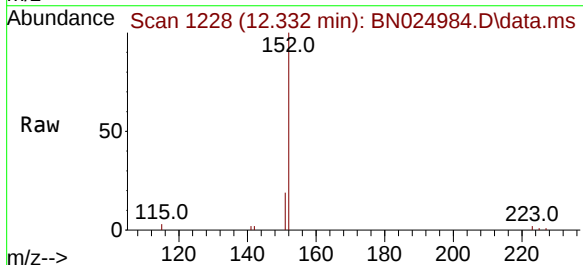


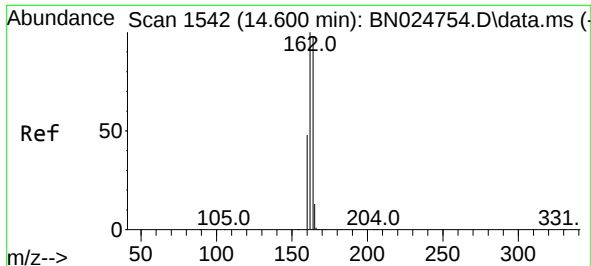

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.576 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN024984.D
Acq: 18 Apr 2023 18:31




Instrument :
BNA_N
ClientSampleId :
BP-TT-RW5B-20230413DL


Tgt Ion:164 Resp: 18907
Ion Ratio Lower Upper
164 100
162 104.2 81.9 122.9
160 49.1 39.2 58.8

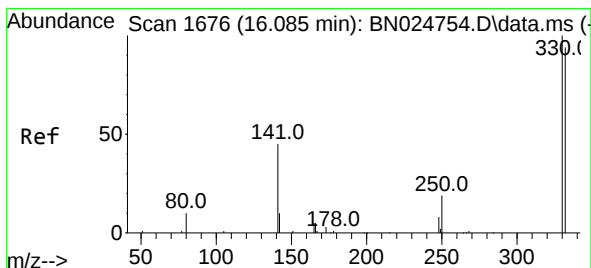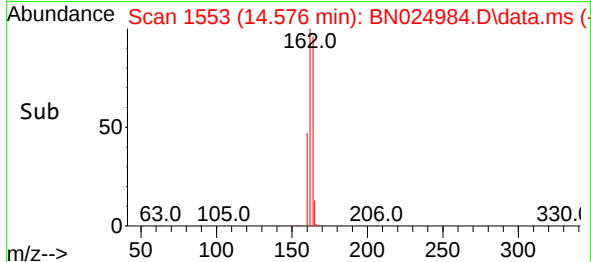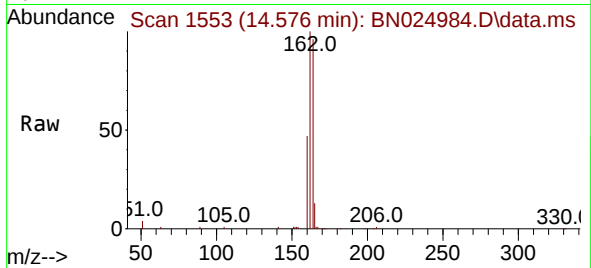

#14
2,4,6-Tribromophenol
Concen: 0.146 ng
RT: 16.070 min Scan# 1688
Delta R.T. -0.000 min
Lab File: BN024984.D
Acq: 18 Apr 2023 18:31

Tgt Ion:330 Resp: 1241
Ion Ratio Lower Upper
330 100
332 98.0 77.9 116.9
141 41.2 31.0 46.6


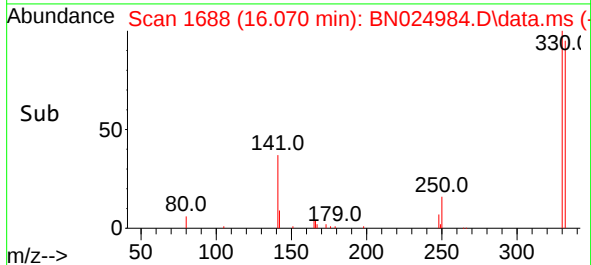

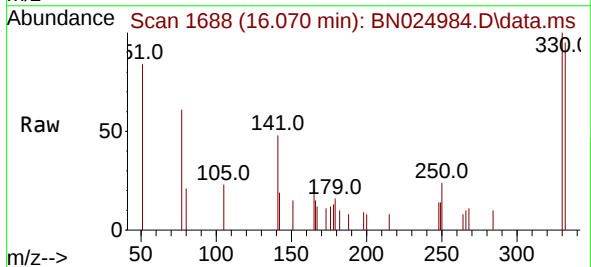


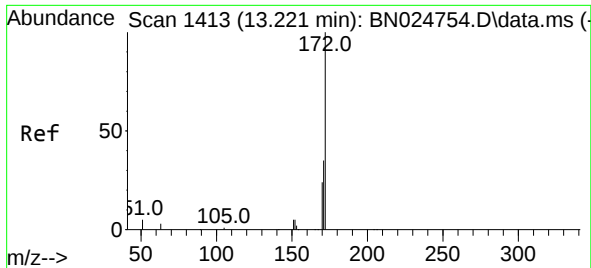

#15
2-Fluorobiphenyl
Concen: 0.163 ng
RT: 13.208 min Scan# 1413
Delta R.T. -0.000 min
Lab File: BN024984.D
Acq: 18 Apr 2023 18:31




Instrument :
BNA_N
ClientSampleId :
BP-TT-RW5B-20230413DL


Tgt Ion:172	Resp:	11800
Ion Ratio	Lower	Upper
172	100	
171	34.1	28.2 42.2
170	22.7	19.2 28.8

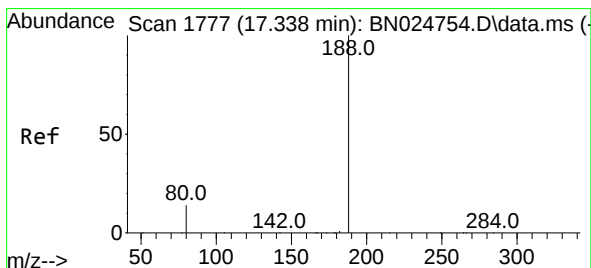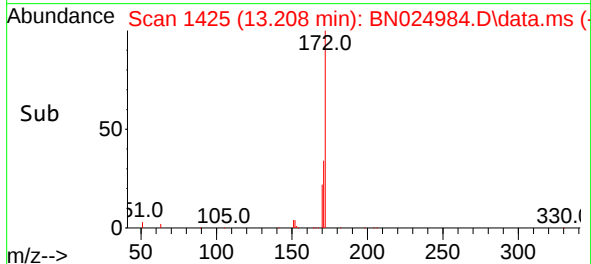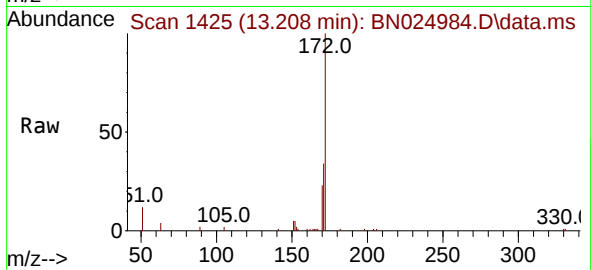

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.323 min Scan# 1789
Delta R.T. -0.000 min
Lab File: BN024984.D
Acq: 18 Apr 2023 18:31

Tgt Ion:188	Resp:	38990
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0 0.0
80	12.6	11.3 16.9


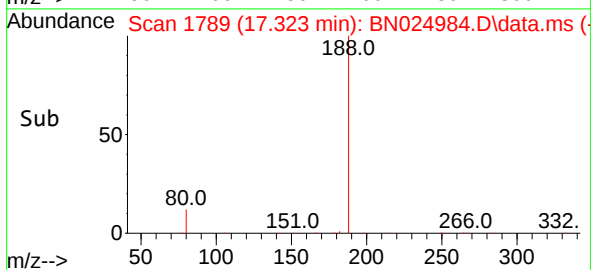

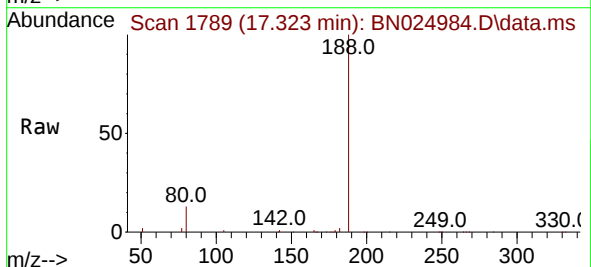


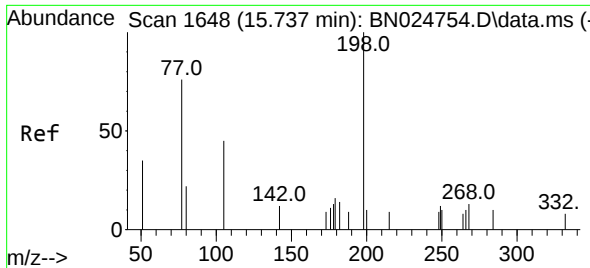

#20
4,6-Dinitro-2-methylphenol
Concen: 0.175 ng
RT: 15.699 min Scan# 1762
Delta R.T. -0.011 min
Lab File: BN024984.D
Acq: 18 Apr 2023 18:31




Instrument :
BNA_N
ClientSampleId :
BP-TT-RW5B-20230413DL


Tgt Ion:198 Resp: 2
Ion Ratio Lower Upper
198 100
51 1074.5 99.8 149.8#
105 252.9 49.4 74.0#

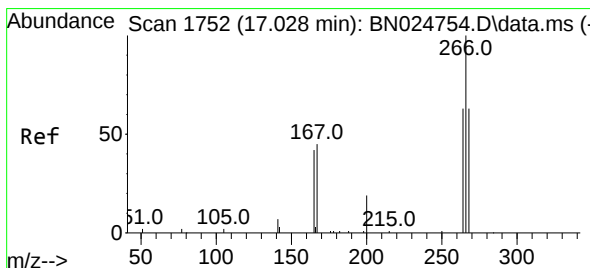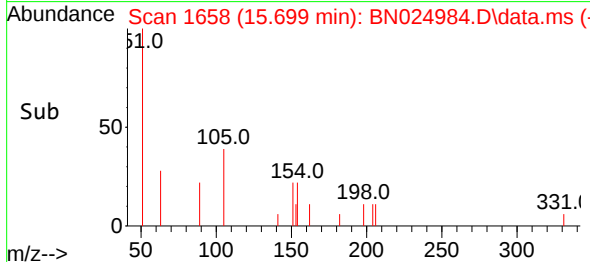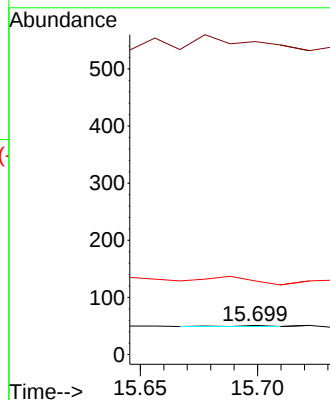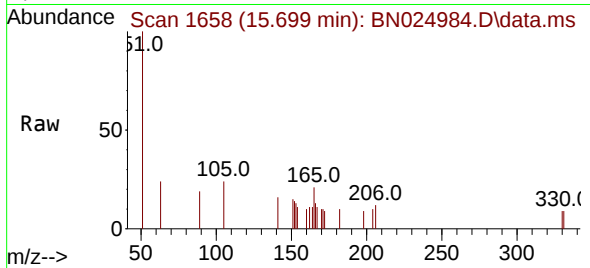

#24
Pentachlorophenol
Concen: 0.222 ng
RT: 16.988 min Scan# 1762
Delta R.T. 0.012 min
Lab File: BN024984.D
Acq: 18 Apr 2023 18:31

Tgt Ion:266 Resp: 44
Ion Ratio Lower Upper
266 100
264 36.4 46.1 69.1#
268 81.8 46.7 70.1#


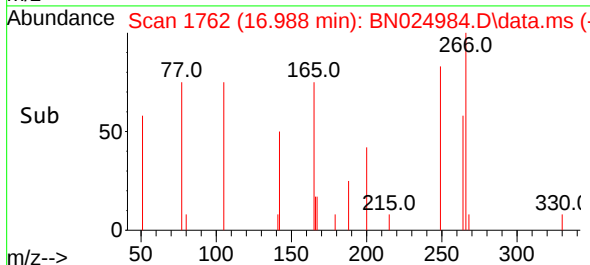
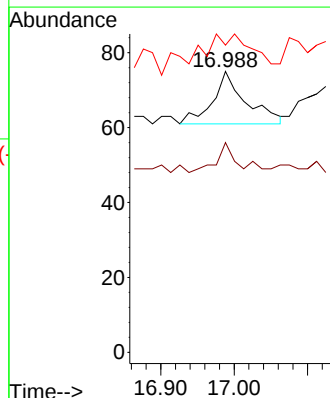
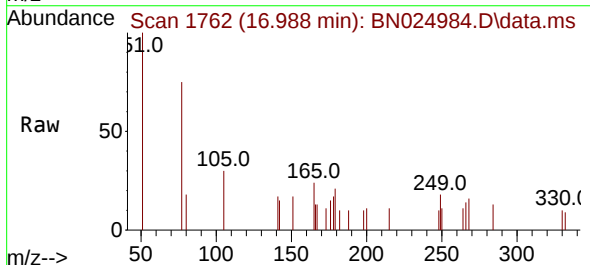


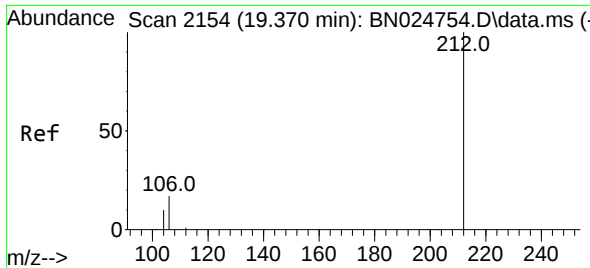

#27
Fluoranthene-d10
Concen: 0.204 ng
RT: 19.355 min Scan# 2164
Delta R.T. -0.004 min
Lab File: BN024984.D
Acq: 18 Apr 2023 18:31




Instrument :
BNA_N
ClientSampleId :
BP-TT-RW5B-20230413DL


Tgt Ion:212 Resp: 18031
Ion Ratio Lower Upper
212 100
106 15.9 13.2 19.8
104 9.4 7.6 11.4

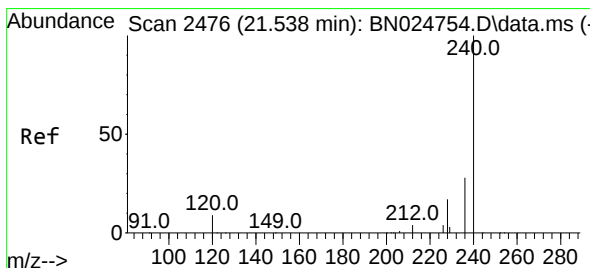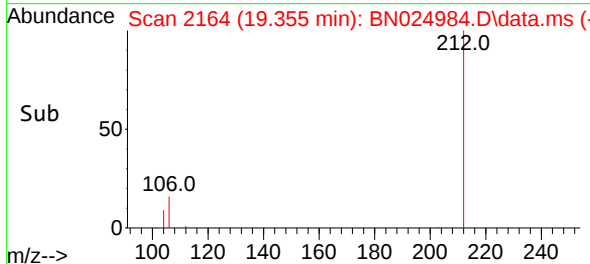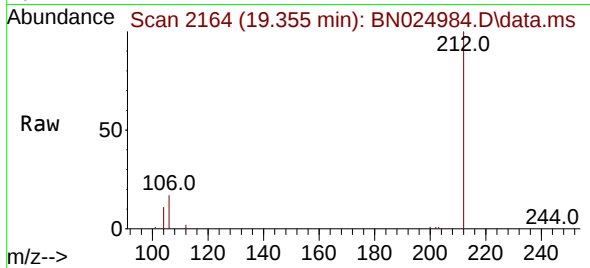

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.518 min Scan# 2487
Delta R.T. -0.004 min
Lab File: BN024984.D
Acq: 18 Apr 2023 18:31

Tgt Ion:240 Resp: 31650
Ion Ratio Lower Upper
240 100
120 19.3 8.8 13.2#
236 28.8 22.6 34.0


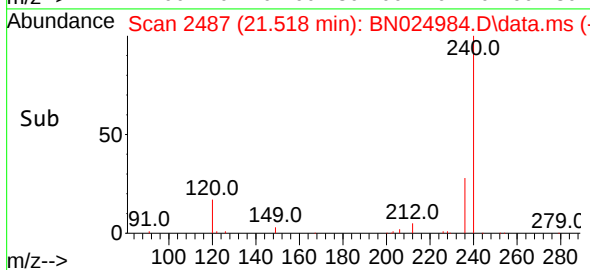

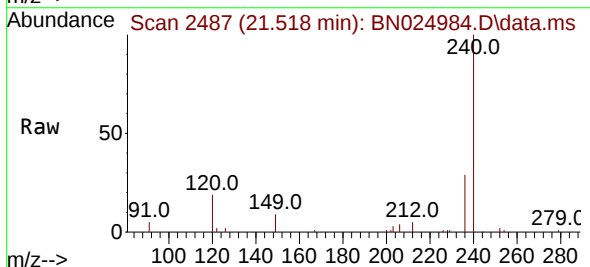


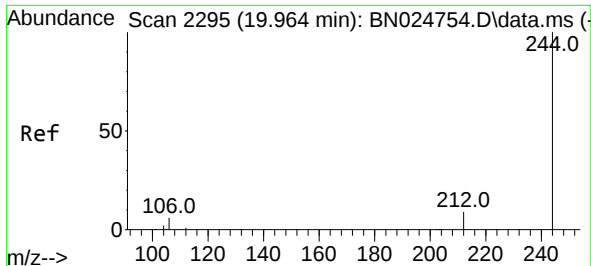

#31
 Terphenyl-d14
 Concen: 0.236 ng
 RT: 19.953 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN024984.D
 Acq: 18 Apr 2023 18:31




Instrument :
 BNA_N
 ClientSampleId :
 BP-TT-RW5B-20230413DL


Tgt Ion:244 Resp: 16899
 Ion Ratio Lower Upper
 244 100
 212 8.9 7.4 11.0
 122 0.0 0.0 0.0

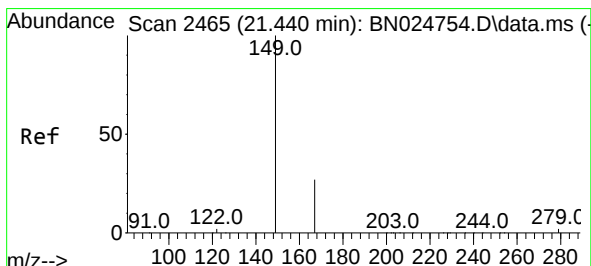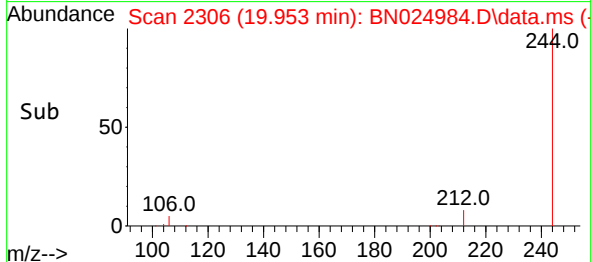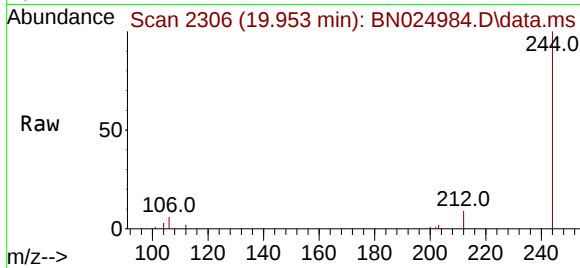

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.106 ng
 RT: 21.428 min Scan# 2477
 Delta R.T. 0.005 min
 Lab File: BN024984.D
 Acq: 18 Apr 2023 18:31


Tgt Ion:149 Resp: 6104
 Ion Ratio Lower Upper
 149 100
 167 11.2 21.4 32.2#
 279 2.1 2.6 4.0#

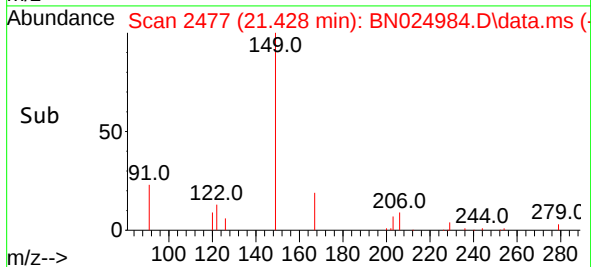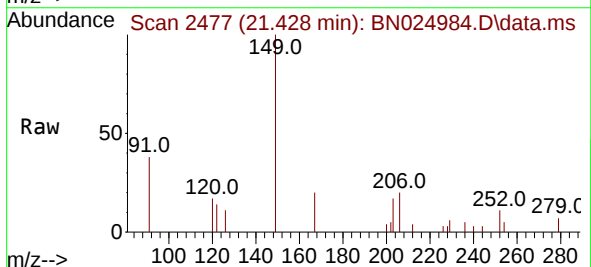

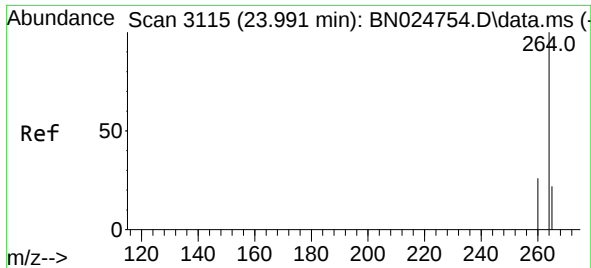

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.968 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BN024984.D
 Acq: 18 Apr 2023 18:31

Instrument :
 BNA_N
 ClientSampleId :
 BP-TT-RW5B-20230413DL

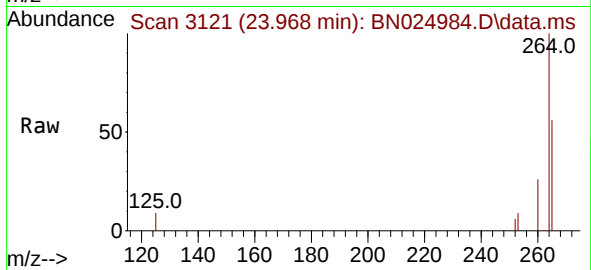

Tgt Ion:264 Resp: 26584

Ion	Ratio	Lower	Upper
264	100		
260	25.9	20.8	31.2
265	55.6	46.5	69.7

