
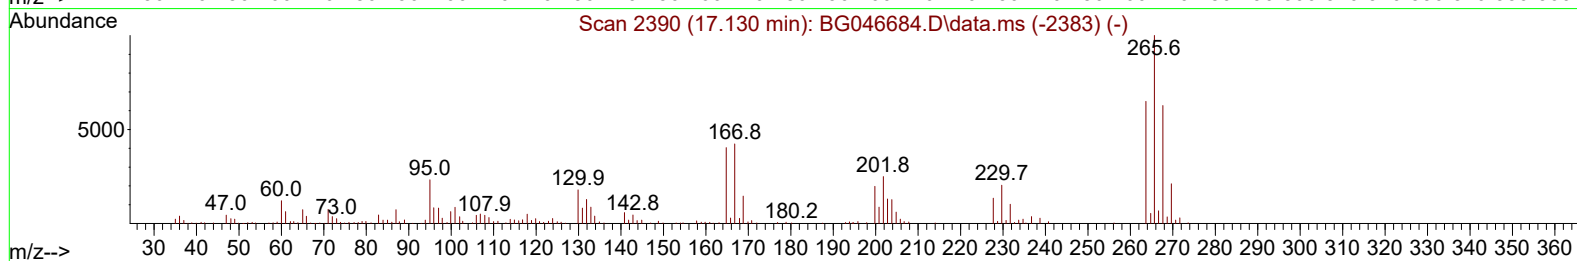
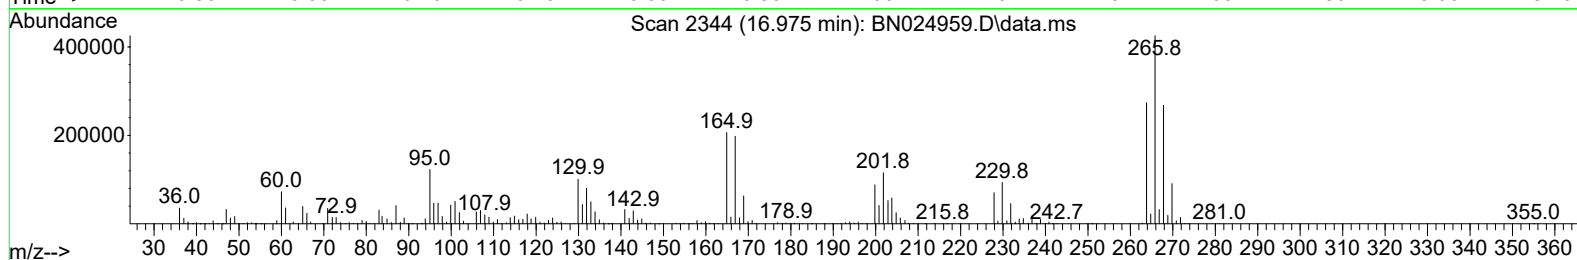


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041823\
Data File : BN024959.D
Acq On : 17 Apr 2023 17:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 07:14:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 07:14:27 2023
Response via : Initial Calibration

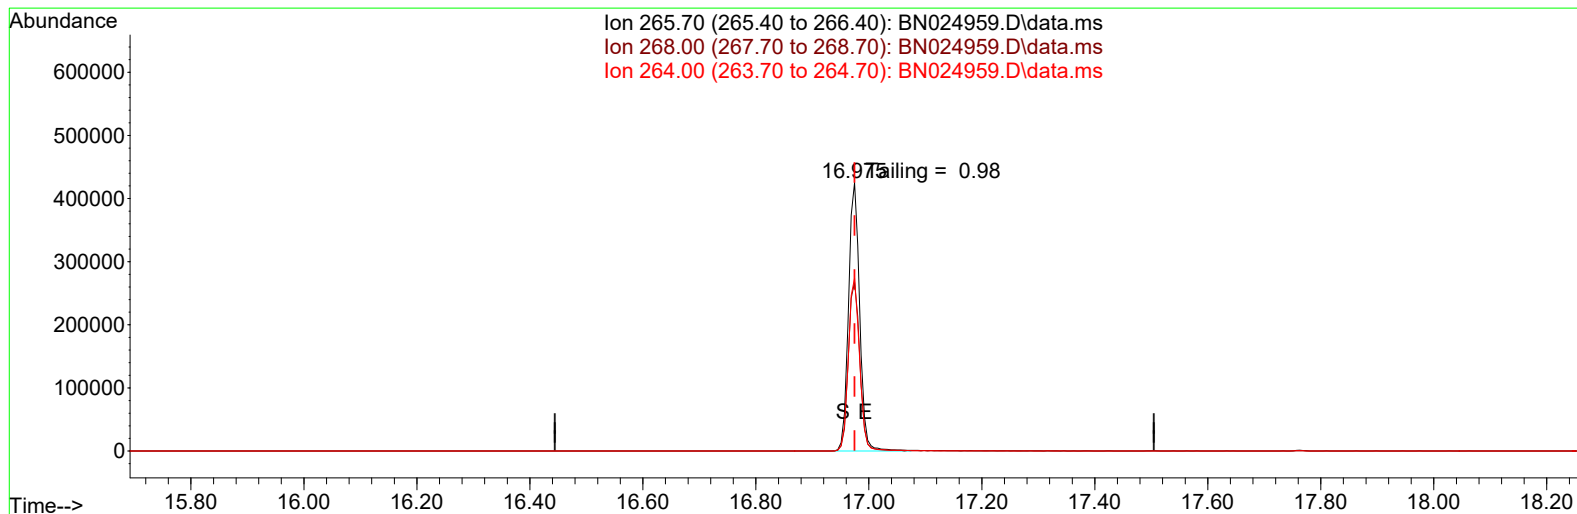

TIC: BN024959.D\data.ms

(70) Pentachlorophenol (C)




16.975min (0.000) 159595.82 ng

response 583650

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.99
264.00	61.60	64.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041823\
Data File : BN024959.D
Acq On : 17 Apr 2023 17:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 07:14:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 18 07:14:27 2023
Response via : Initial Calibration

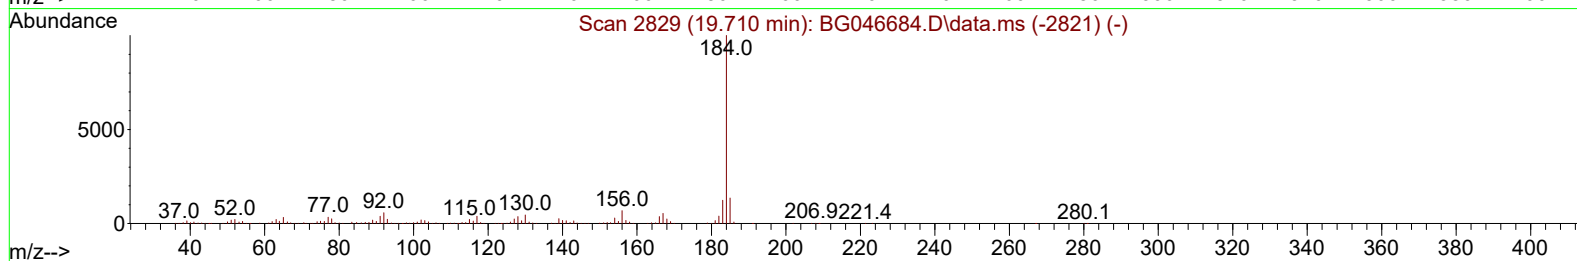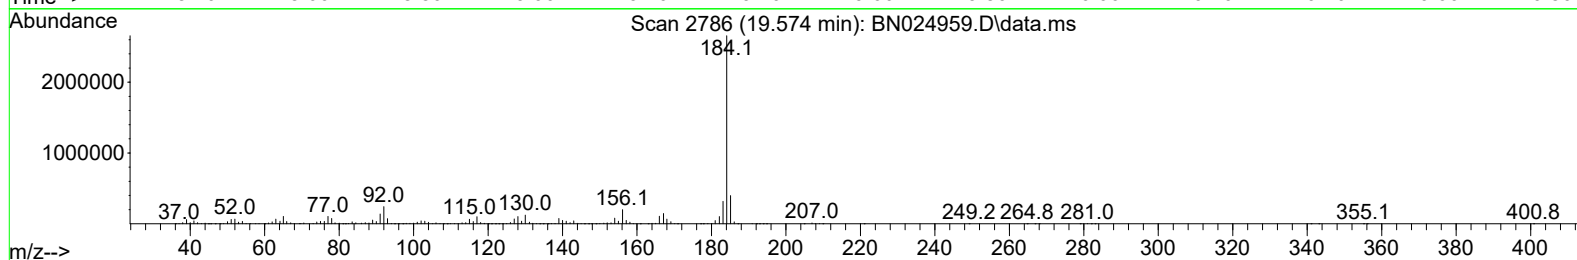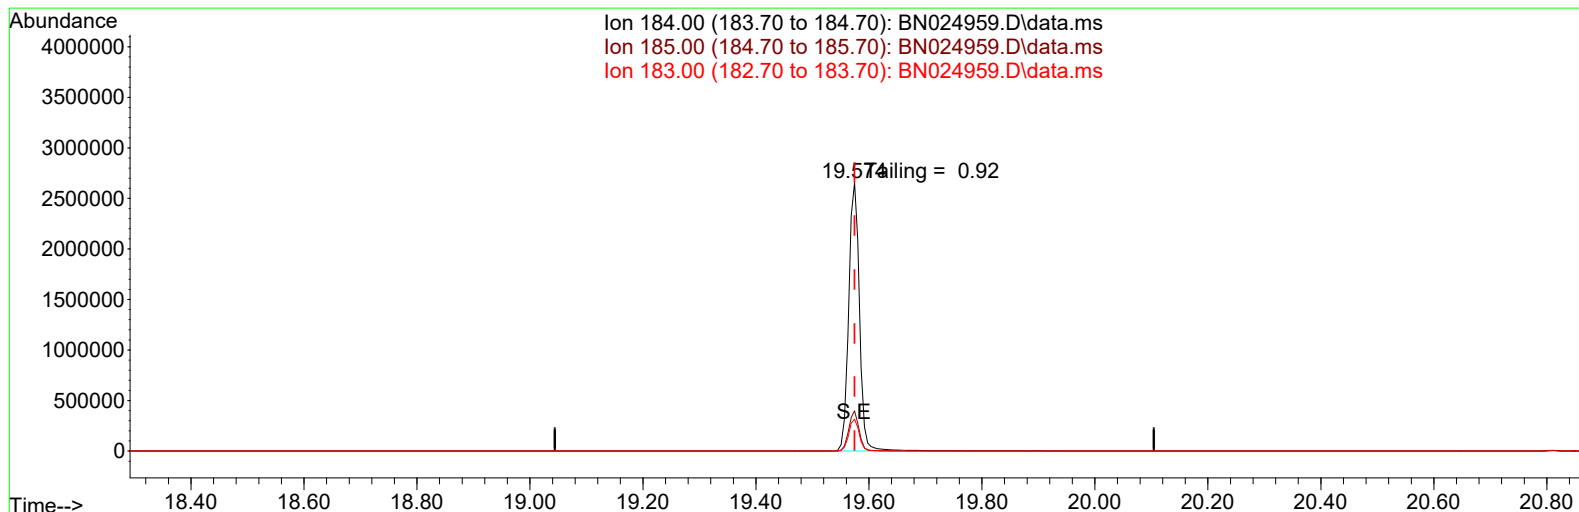

TIC: BN024959.D\data.ms

(77) Benzidine**19.574min (0.000) 127895.12 ng****response 3528461**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.98
183.00	13.20	11.90
0.00	0.00	0.00