
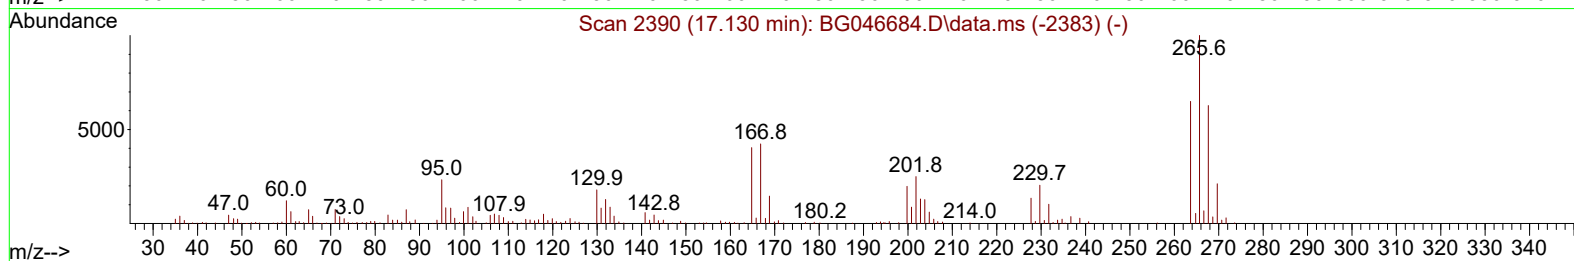
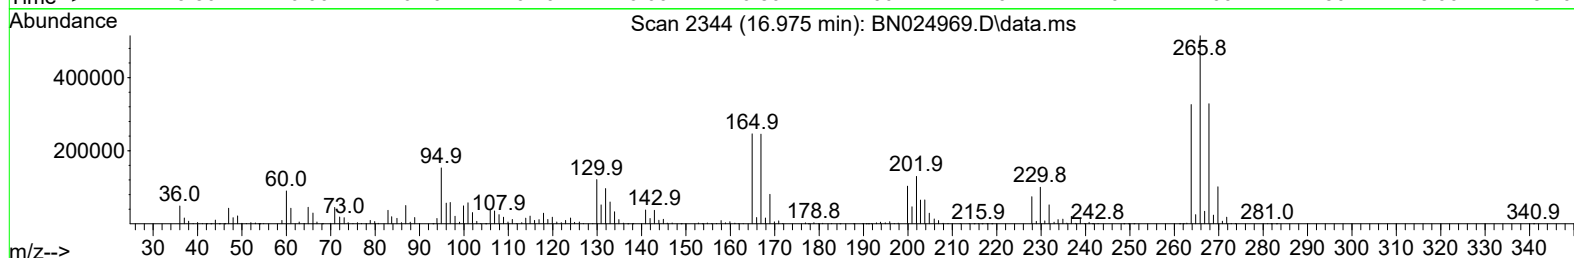


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN041823\  
Data File : BN024969.D  
Acq On : 18 Apr 2023 09:12  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 07:28:39 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Apr 19 07:28:34 2023  
Response via : Initial Calibration

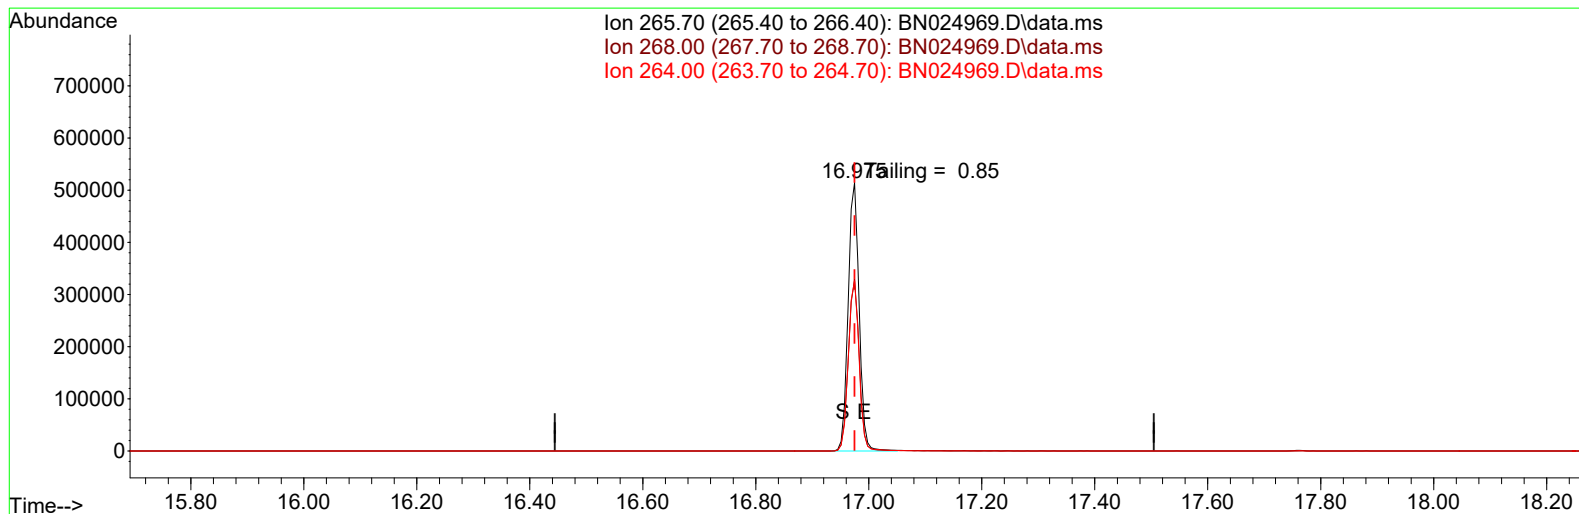

TIC: BN024969.D\data.ms

**(70) Pentachlorophenol (C)**




16.975min ( 0.000) 22837.95 ng

response 697191

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 63.82  |
| 264.00 | 61.60  | 63.46  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN041823\  
Data File : BN024969.D  
Acq On : 18 Apr 2023 09:12  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 07:28:39 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Apr 19 07:28:34 2023  
Response via : Initial Calibration

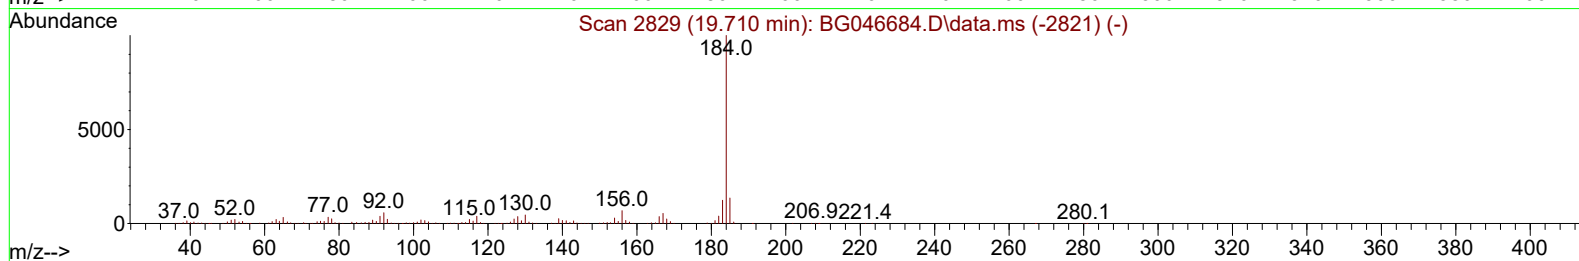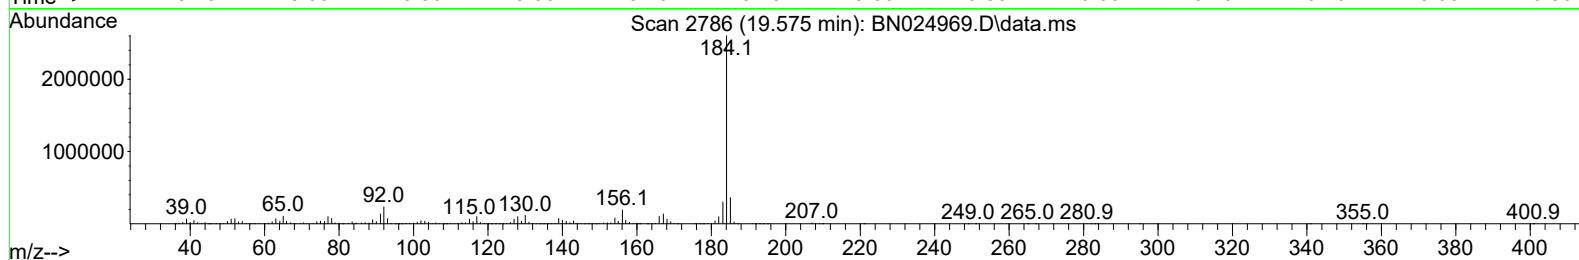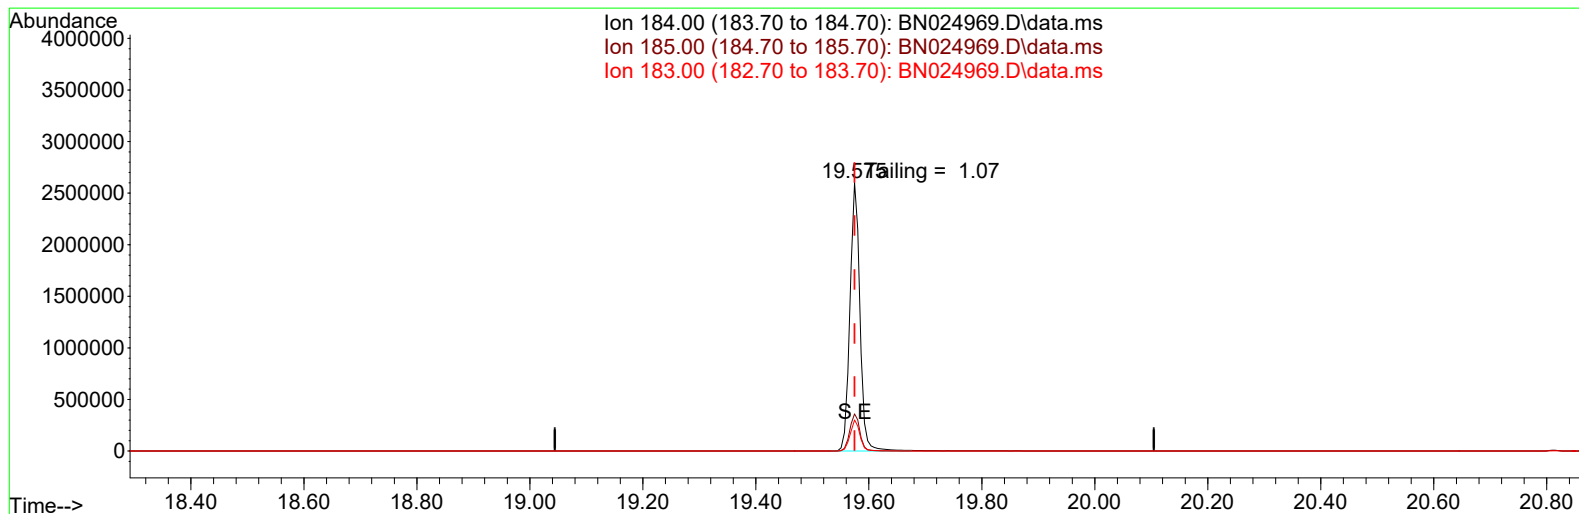

TIC: BN024969.D\data.ms

**(77) Benzidine****19.575min ( 0.000) 1784831.23 ng****response 3191049**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.87  |
| 183.00 | 13.20  | 11.59  |
| 0.00   | 0.00   | 0.00   |