
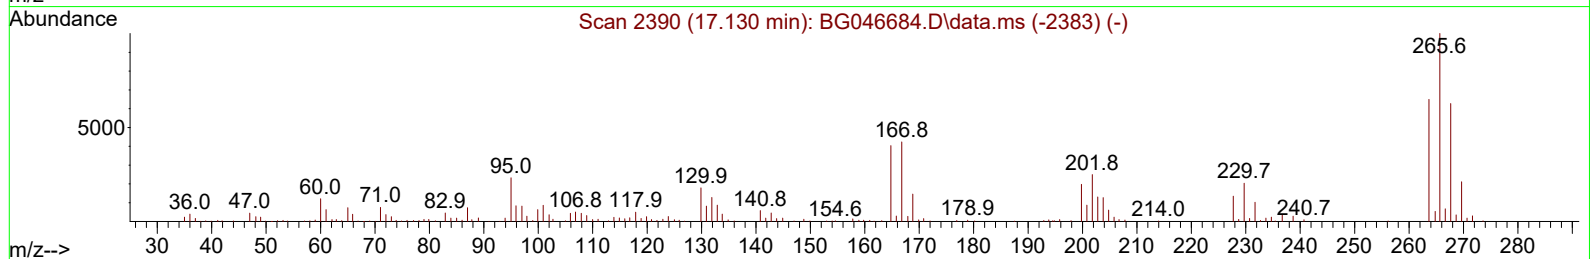
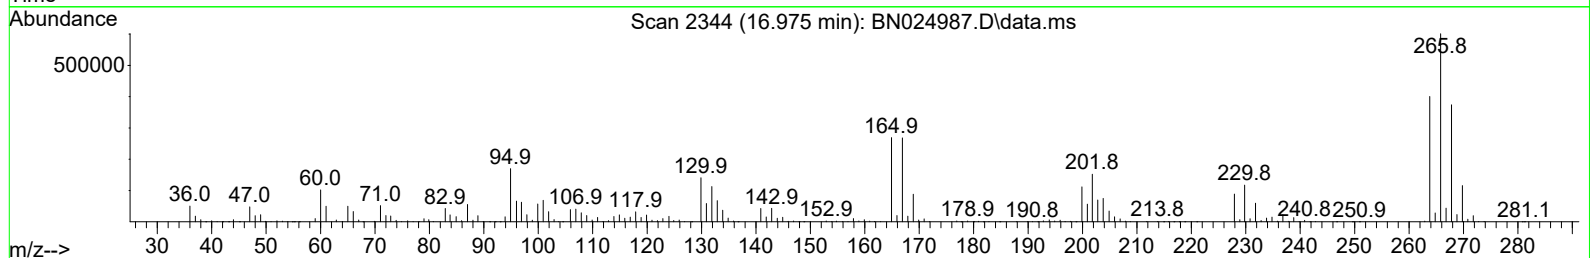


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041823\
Data File : BN024987.D
Acq On : 18 Apr 2023 21:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 07:29:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 19 07:28:34 2023
Response via : Initial Calibration

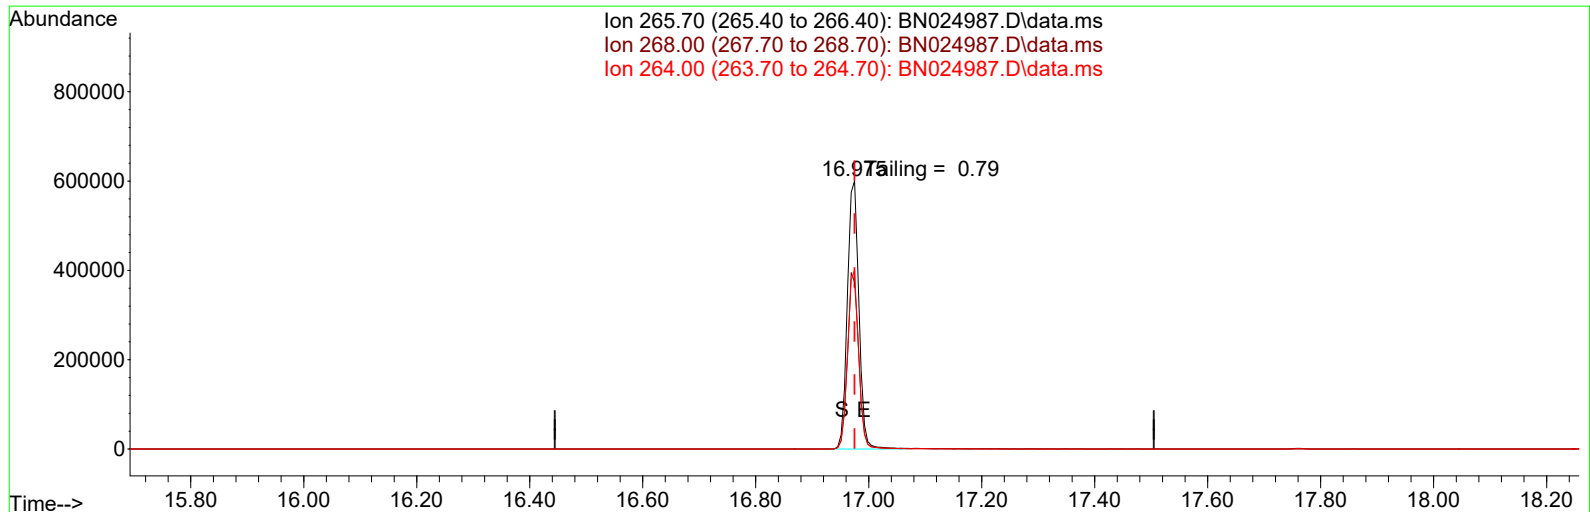

TIC: BN024987.D\data.ms

(70) Pentachlorophenol (C)




16.975min (+ 0.000) 24148.56 ng

response 851287

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.26
264.00	61.60	66.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041823\
Data File : BN024987.D
Acq On : 18 Apr 2023 21:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 07:29:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 19 07:28:34 2023
Response via : Initial Calibration

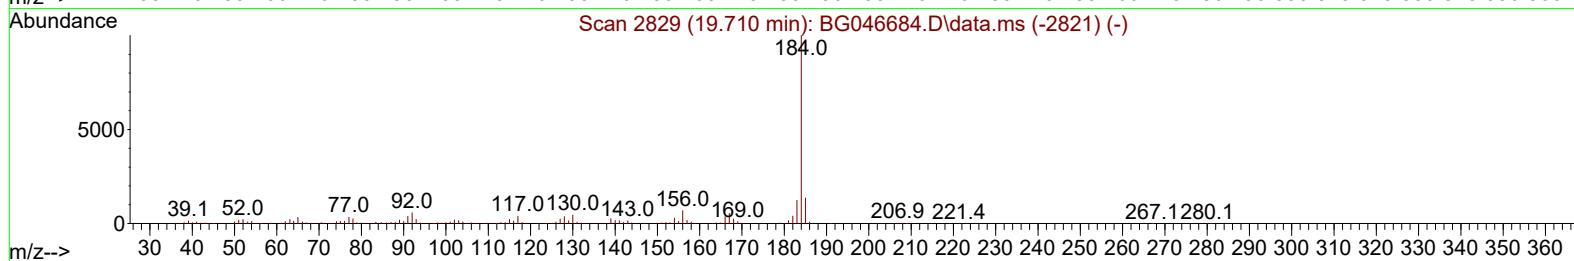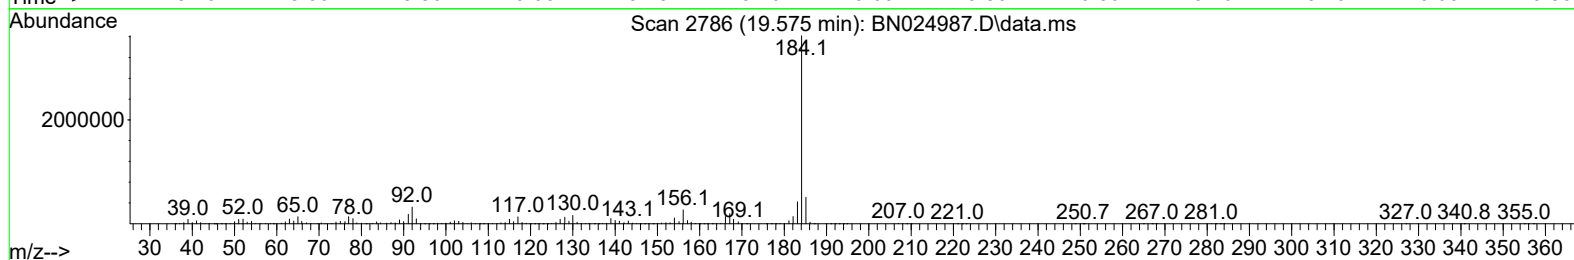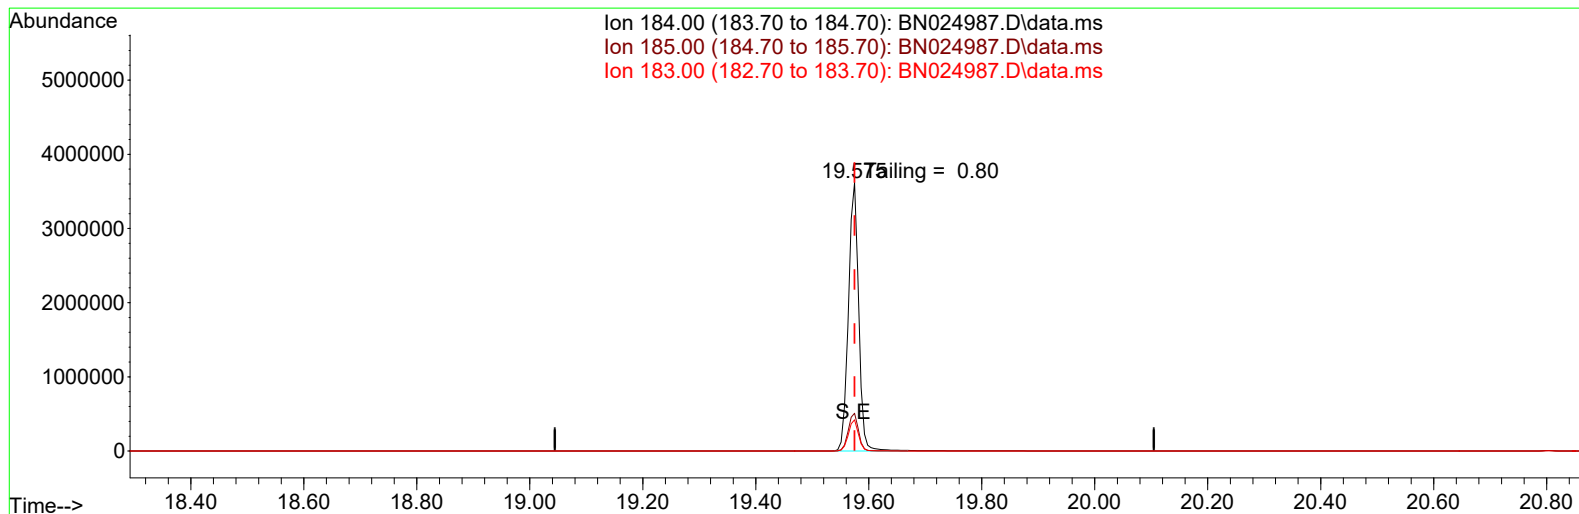

TIC: BN024987.D\data.ms

(77) Benzidine**19.575min (+ 0.000) 0.00 ng****response 4579985**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.06
183.00	13.20	11.67
0.00	0.00	0.00