


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041823\
Data File : BN024959.D
Acq On : 17 Apr 2023 17:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN040523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 19 05:45:45 2023

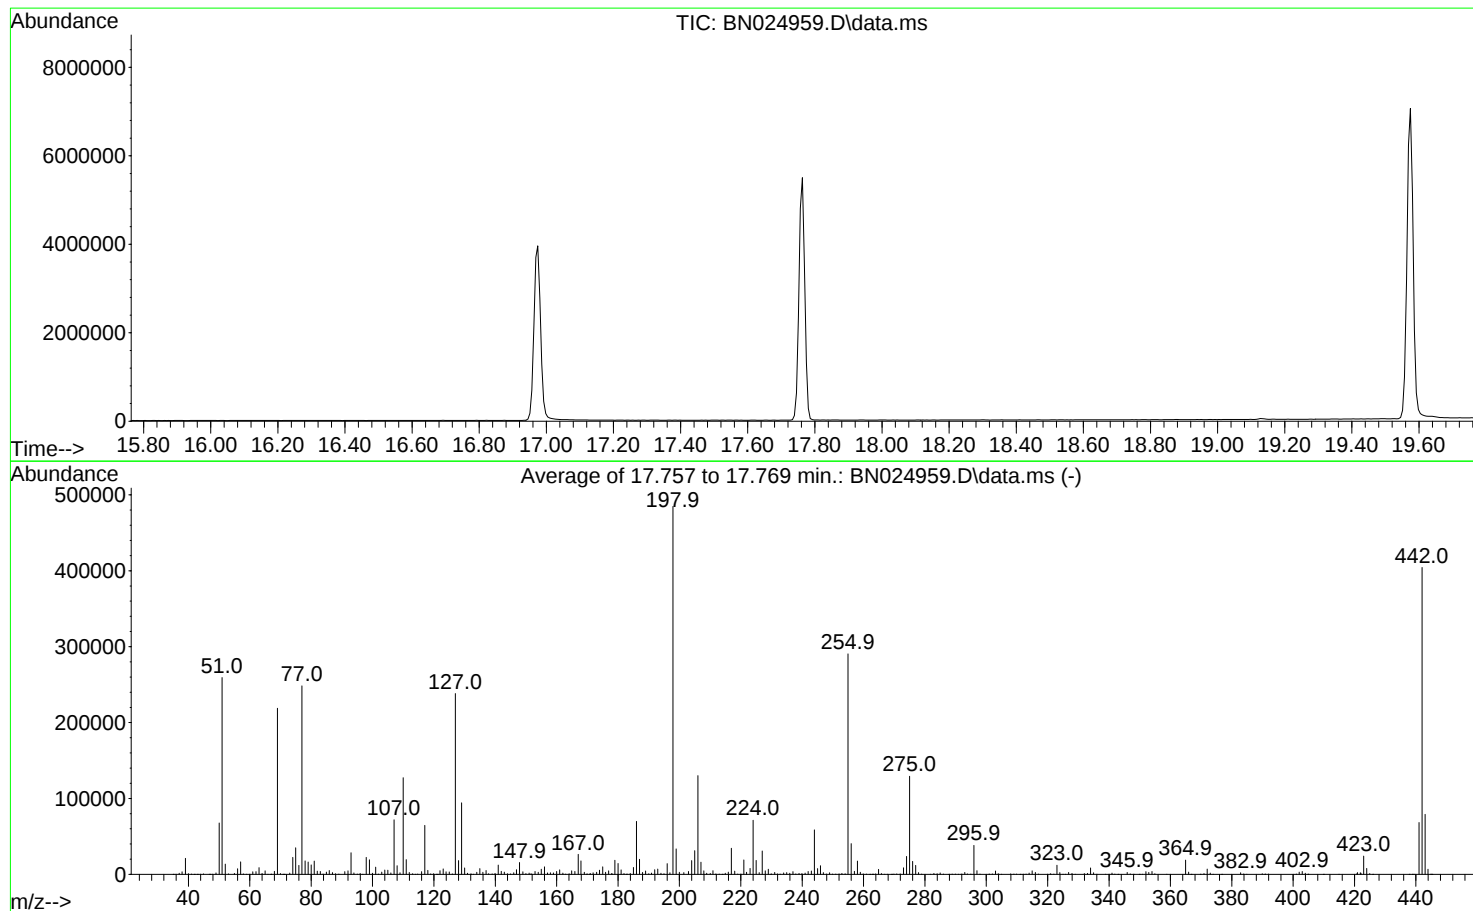




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.5	259385	PASS
68	69	0.00	2	1.8	3937	PASS
69	198	0.00	100	45.2	218880	PASS
70	69	0.00	2	0.5	1112	PASS
127	198	10	80	49.2	238251	PASS
197	198	0.00	2	0.4	2100	PASS
198	198	100	100	100.0	484693	PASS
199	198	5	9	6.9	33563	PASS
275	198	10	60	26.7	129293	PASS
365	198	1	100	3.9	18688	PASS
441	198	0.01	100	14.1	68347	PASS
442	442	50	100	100.0	404437	PASS
443	442	15	24	19.6	79155	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041823\
 Data File : BN024959.D
 Acq On : 17 Apr 2023 17:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Apr 18 07:14:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 18 07:14:27 2023
 Response via : Initial Calibration

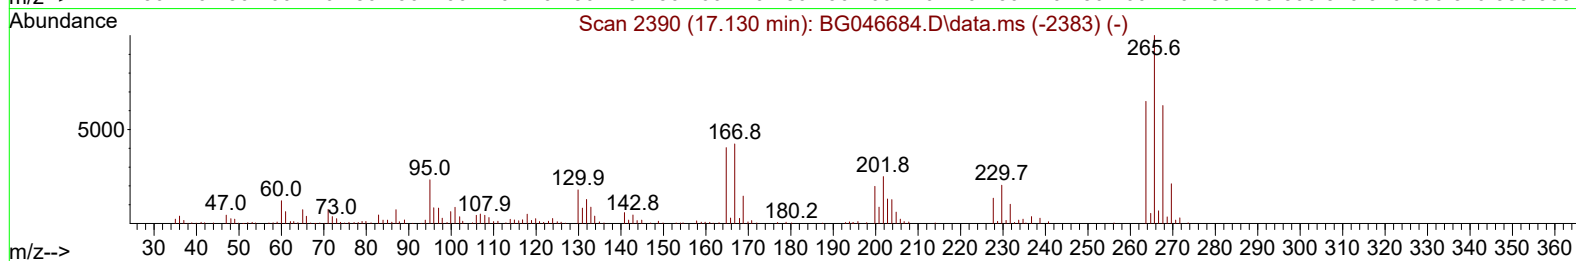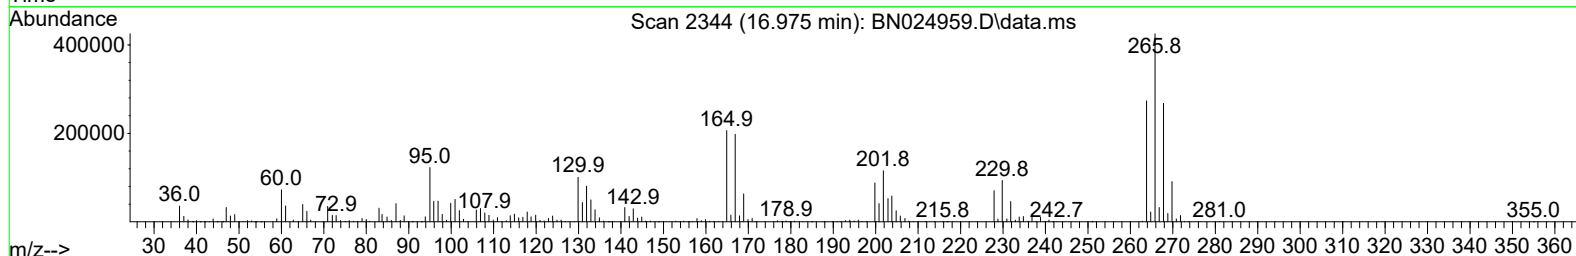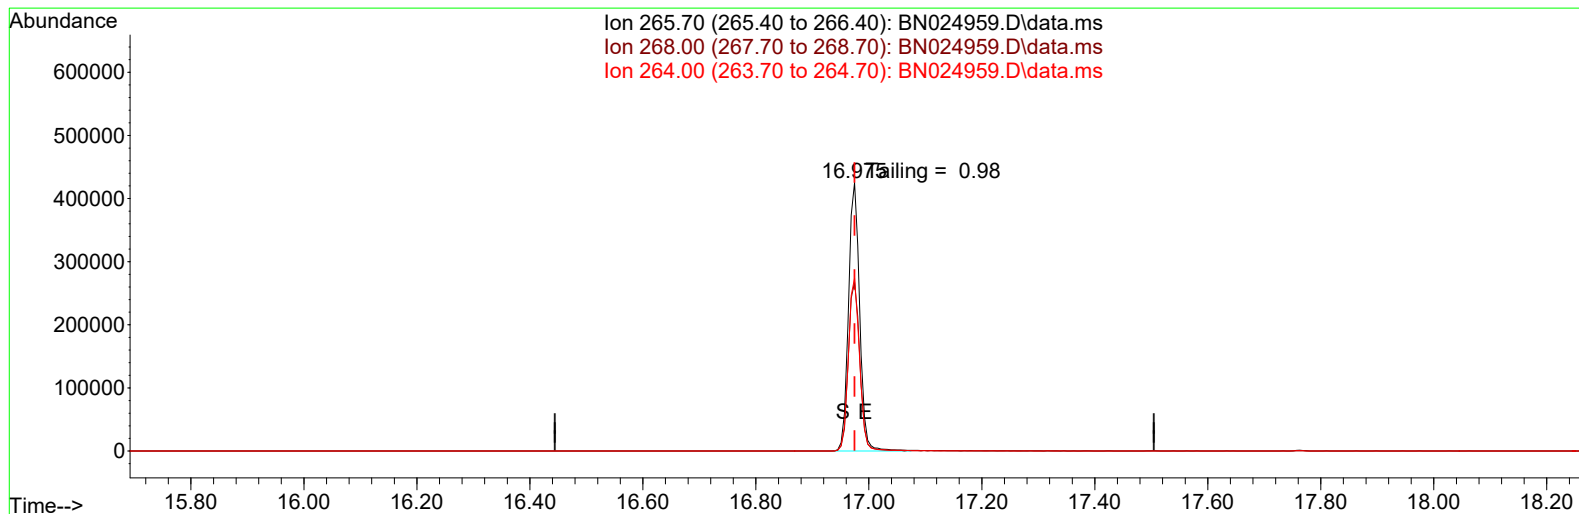

TIC: BN024959.D\data.ms

(70) Pentachlorophenol (C)

16.975min (0.000) 159595.82 ng




response 583650

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.99
264.00	61.60	64.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041823\
 Data File : BN024959.D
 Acq On : 17 Apr 2023 17:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Apr 18 07:14:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 18 07:14:27 2023
 Response via : Initial Calibration

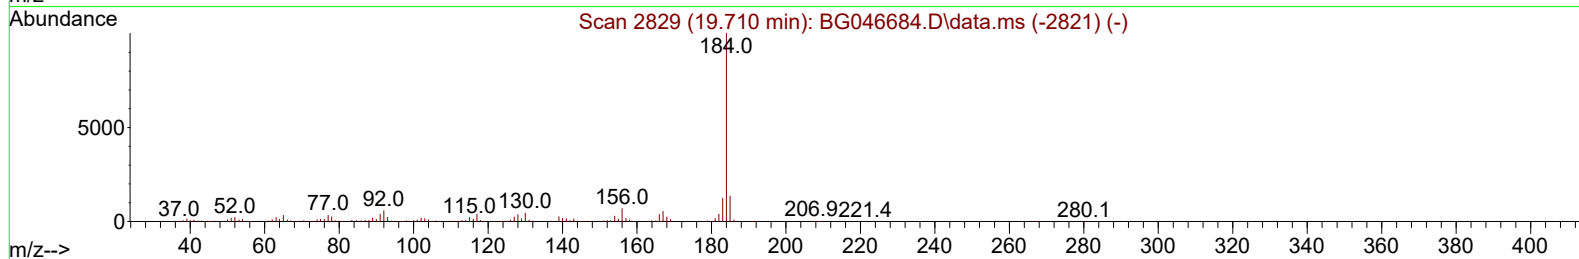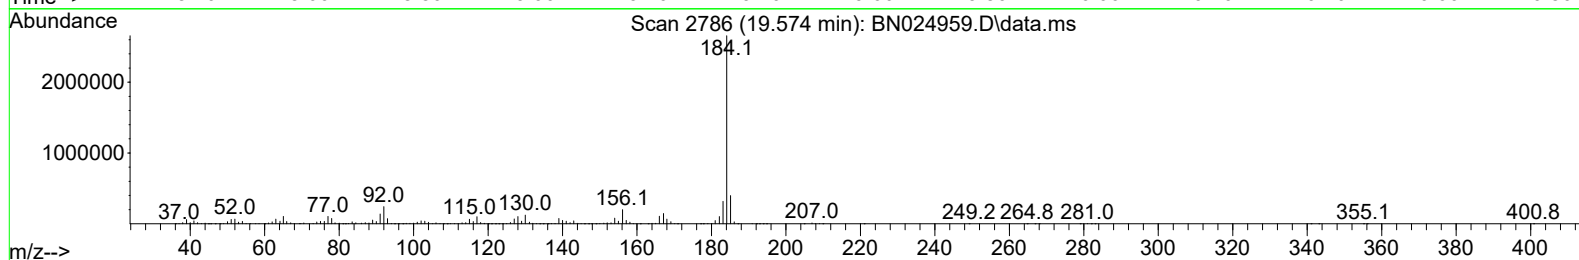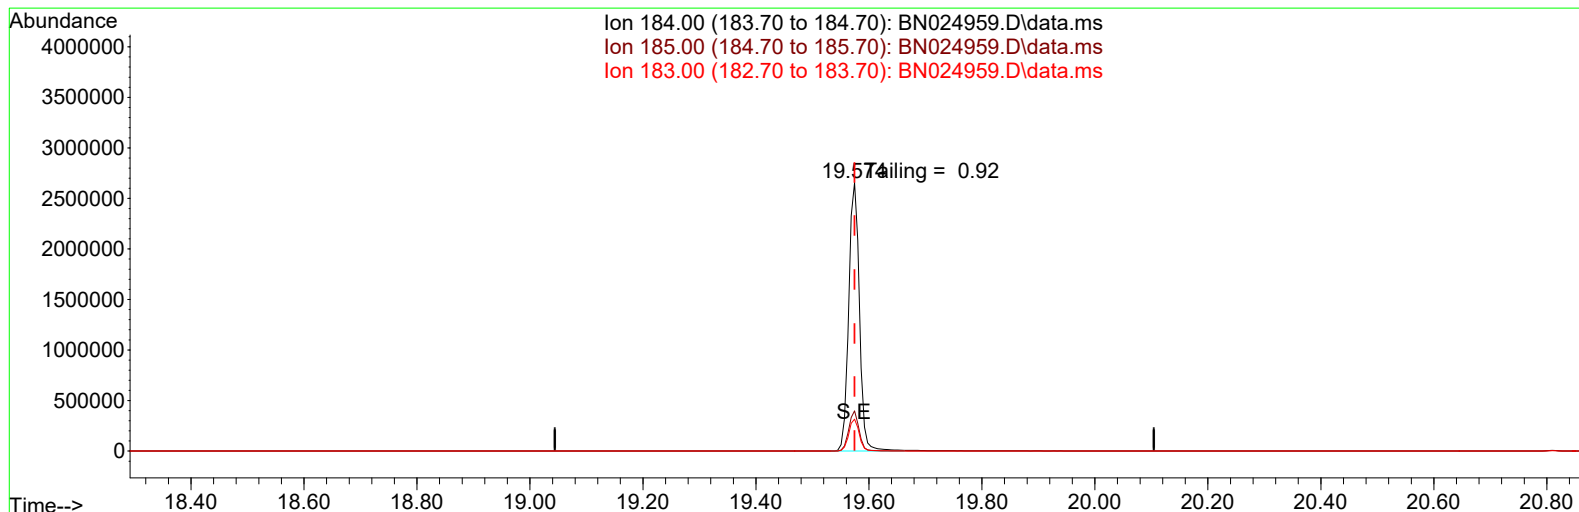

TIC: BN024959.D\data.ms

(77) Benzidine

19.574min (0.000) 127895.12 ng

response 3528461

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.98
183.00	13.20	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/18/2023	BNA_N	<u>BN024959.D</u>
Compound Name	Response	Retention Time
DDT	1724758	20.81
DDD	41851	20.368
DDE	4529	19.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
46380	1771138	2.62

Instrument :
BNA_N
ClientSampleId :
DFTPP