

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042021\
 Data File : BN014328.D
 Acq On : 19 Apr 2021 17:21
 Operator : CG/JU
 Sample : PB135369BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK369

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	19	22	33	rVB	63834	93949	1.67%	0.194%
2	3.610	87	89	109	rBV	690298	1145916	20.40%	2.371%
3	6.851	634	640	652	rBV	922973	1395761	24.85%	2.888%
4	7.022	663	669	680	rBV	744089	1159479	20.65%	2.399%
5	7.222	696	703	713	rVB	960370	1500964	26.73%	3.106%
6	7.687	775	782	790	rVB	575001	898601	16.00%	1.859%
7	8.381	894	900	911	rBV	1092418	1669819	29.73%	3.455%
8	8.834	970	977	992	rBV	821257	1317461	23.46%	2.726%
9	9.551	1092	1099	1107	rBV	616642	947323	16.87%	1.960%
10	10.086	1183	1190	1201	rBV	1066825	1692251	30.13%	3.501%
11	10.463	1247	1254	1266	rVB	733542	1224630	21.81%	2.534%
12	10.598	1269	1277	1290	rBV	1068626	1726227	30.74%	3.572%
13	12.057	1519	1525	1530	rBV	15710	23075	0.41%	0.048%
14	13.739	1804	1811	1822	rVB	1872331	2417541	43.05%	5.002%
15	14.016	1851	1858	1873	rBV	2088859	3022841	53.83%	6.254%
16	14.327	1903	1911	1921	rBV2	1046407	1519484	27.06%	3.144%
17	14.522	1938	1944	1957	rBV	810663	1088953	19.39%	2.253%
18	15.321	2073	2080	2091	rBV	2678004	3710964	66.08%	7.678%
19	15.433	2094	2099	2108	rBV	633875	842487	15.00%	1.743%
20	15.563	2116	2121	2127	rVB	24648	31849	0.57%	0.066%
21	16.110	2208	2214	2217	rBV3	6316	7936	0.14%	0.016%
22	17.074	2371	2378	2385	rBV	1244337	1716969	30.57%	3.552%
23	17.174	2388	2395	2413	rVB	2944686	4077842	72.61%	8.437%
24	19.104	2719	2723	2728	rBV	21917	30488	0.54%	0.063%
25	19.362	2762	2767	2772	rBV	19006	24067	0.43%	0.050%
26	19.421	2773	2777	2780	rVV	32099	33909	0.60%	0.070%
27	19.474	2780	2786	2794	rVV	3847494	5012972	89.26%	10.372%
28	19.539	2794	2797	2803	rVB4	9204	11801	0.21%	0.024%
29	20.474	2952	2956	2958	rBV2	25570	31893	0.57%	0.066%
30	20.539	2964	2967	2971	rBV2	9003	11378	0.20%	0.024%
31	21.274	3086	3092	3098	rBV	1575288	2021710	36.00%	4.183%
32	23.362	3440	3447	3462	rBV	3214558	5615987	100.00%	11.620%
33	23.503	3464	3471	3485	rVB	1195997	2208250	39.32%	4.569%
34	24.056	3562	3565	3574	rVB2	56528	96719	1.72%	0.200%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042021\
Data File : BN014328.D
Acq On : 19 Apr 2021 17:21
Operator : CG/JU
Sample : PB135369BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK369

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Title : SVOA CALIBRATION


Sum of corrected areas: 48331496

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042021\
Data File : BN014328.D
Acq On : 19 Apr 2021 17:21
Operator : CG/JU
Sample : PB135369BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK369

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

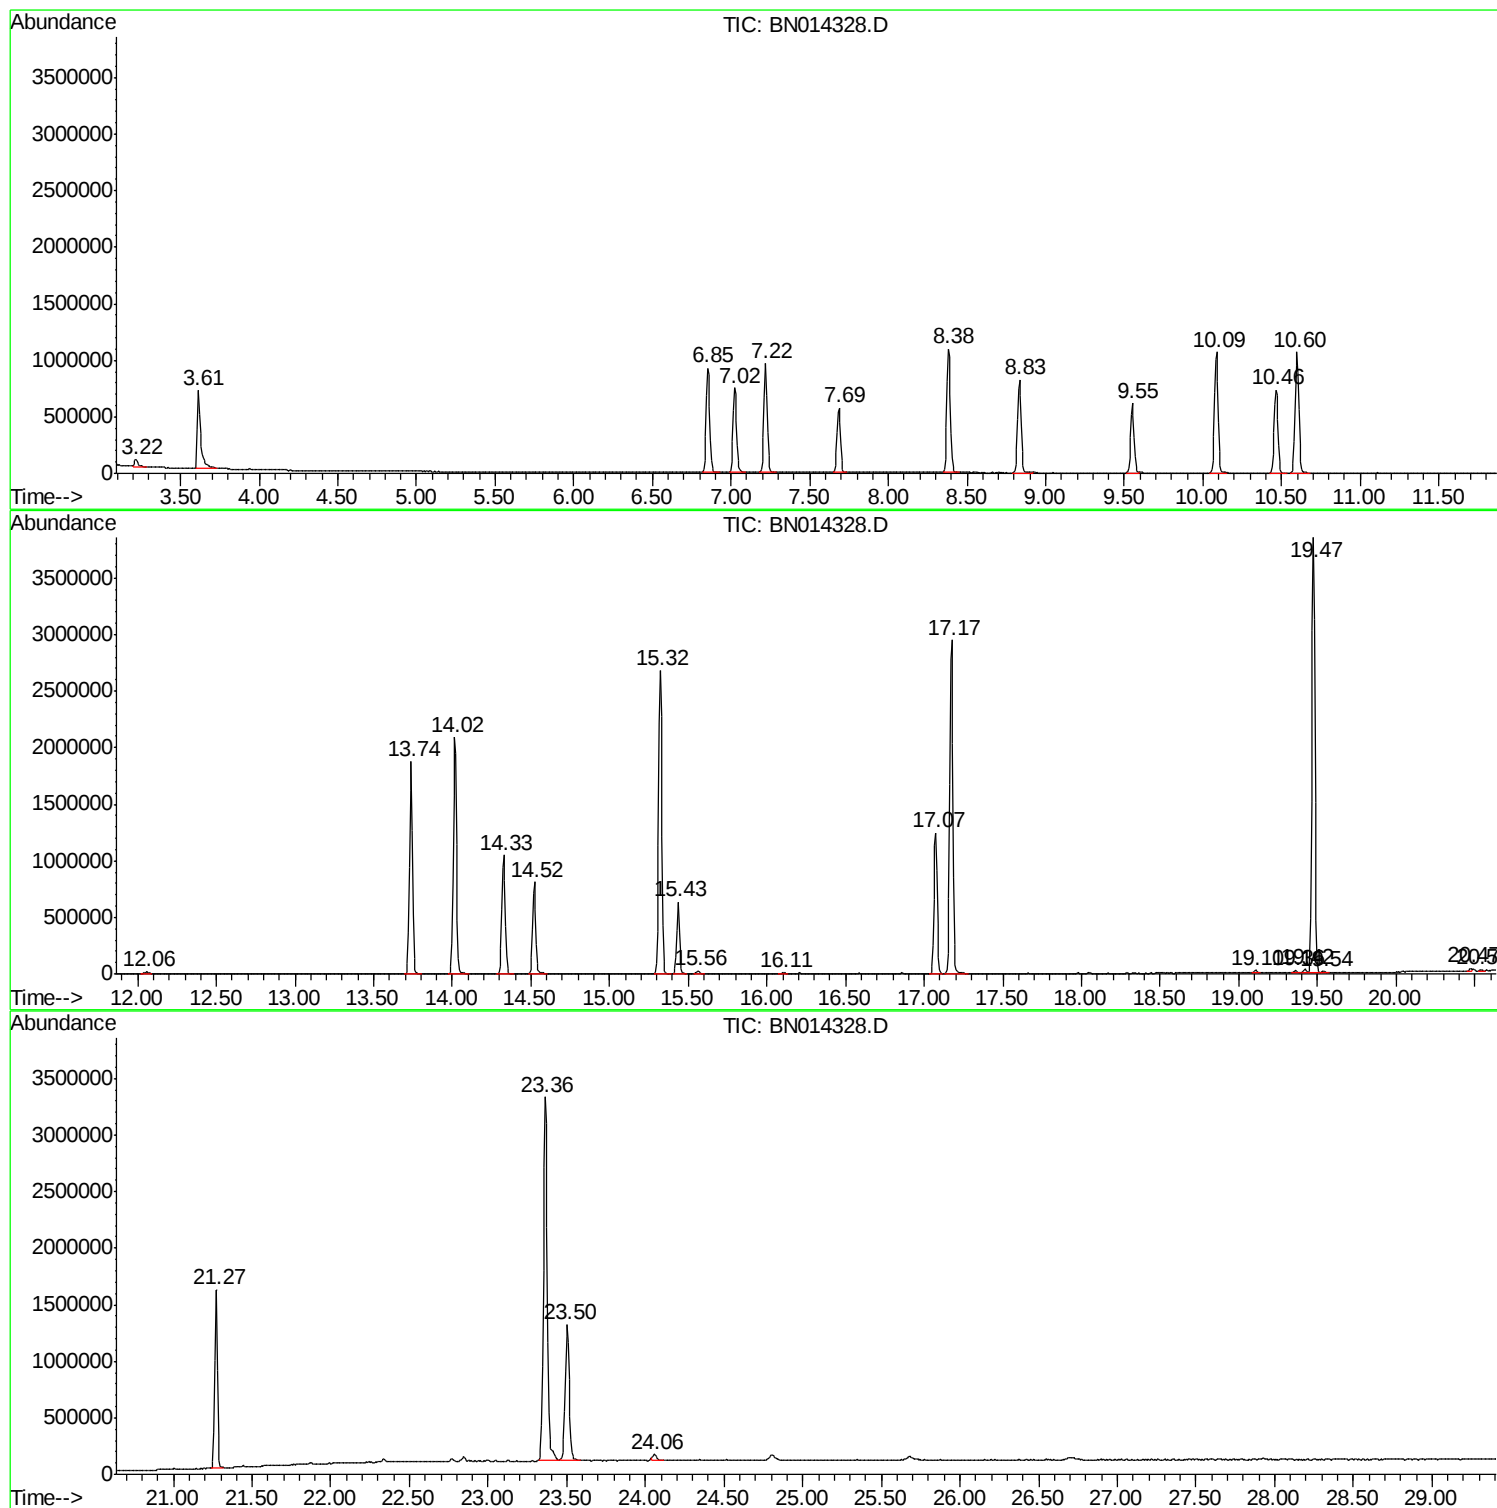

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042021\
Data File : BN014328.D
Acq On : 19 Apr 2021 17:21
Operator : CG/JU
Sample : PB135369BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK369

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042021\
Data File : BN014328.D
Acq On : 19 Apr 2021 17:21
Operator : CG/JU
Sample : PB135369BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK369

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc