

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042021\
 Data File : BN014331.D
 Acq On : 19 Apr 2021 19:46
 Operator : CG/JU
 Sample : K4649-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ATCLP

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.952	143	147	152	rVB2	6457	9688	0.54%	0.111%
2	7.693	777	783	797	rVB	558713	852289	47.13%	9.749%
3	10.469	1248	1255	1262	rBV	696390	1149152	63.55%	13.144%
4	14.328	1905	1911	1924	rVB2	1013776	1434515	79.33%	16.408%
5	16.863	2337	2342	2345	rVB2	2180	2895	0.16%	0.033%
6	17.075	2372	2378	2387	rVV	1246074	1671667	92.45%	19.121%
7	17.175	2391	2395	2400	rVB	2162	3108	0.17%	0.036%
8	17.651	2471	2476	2480	rBV2	1446	3140	0.17%	0.036%
9	21.269	3086	3091	3098	rBV	1578742	1808016	99.99%	20.680%
10	23.498	3463	3470	3482	rVB	998521	1808253	100.00%	20.683%


Sum of corrected areas: 8742723

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042021\
Data File : BN014331.D
Acq On : 19 Apr 2021 19:46
Operator : CG/JU
Sample : K4649-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ATCLP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

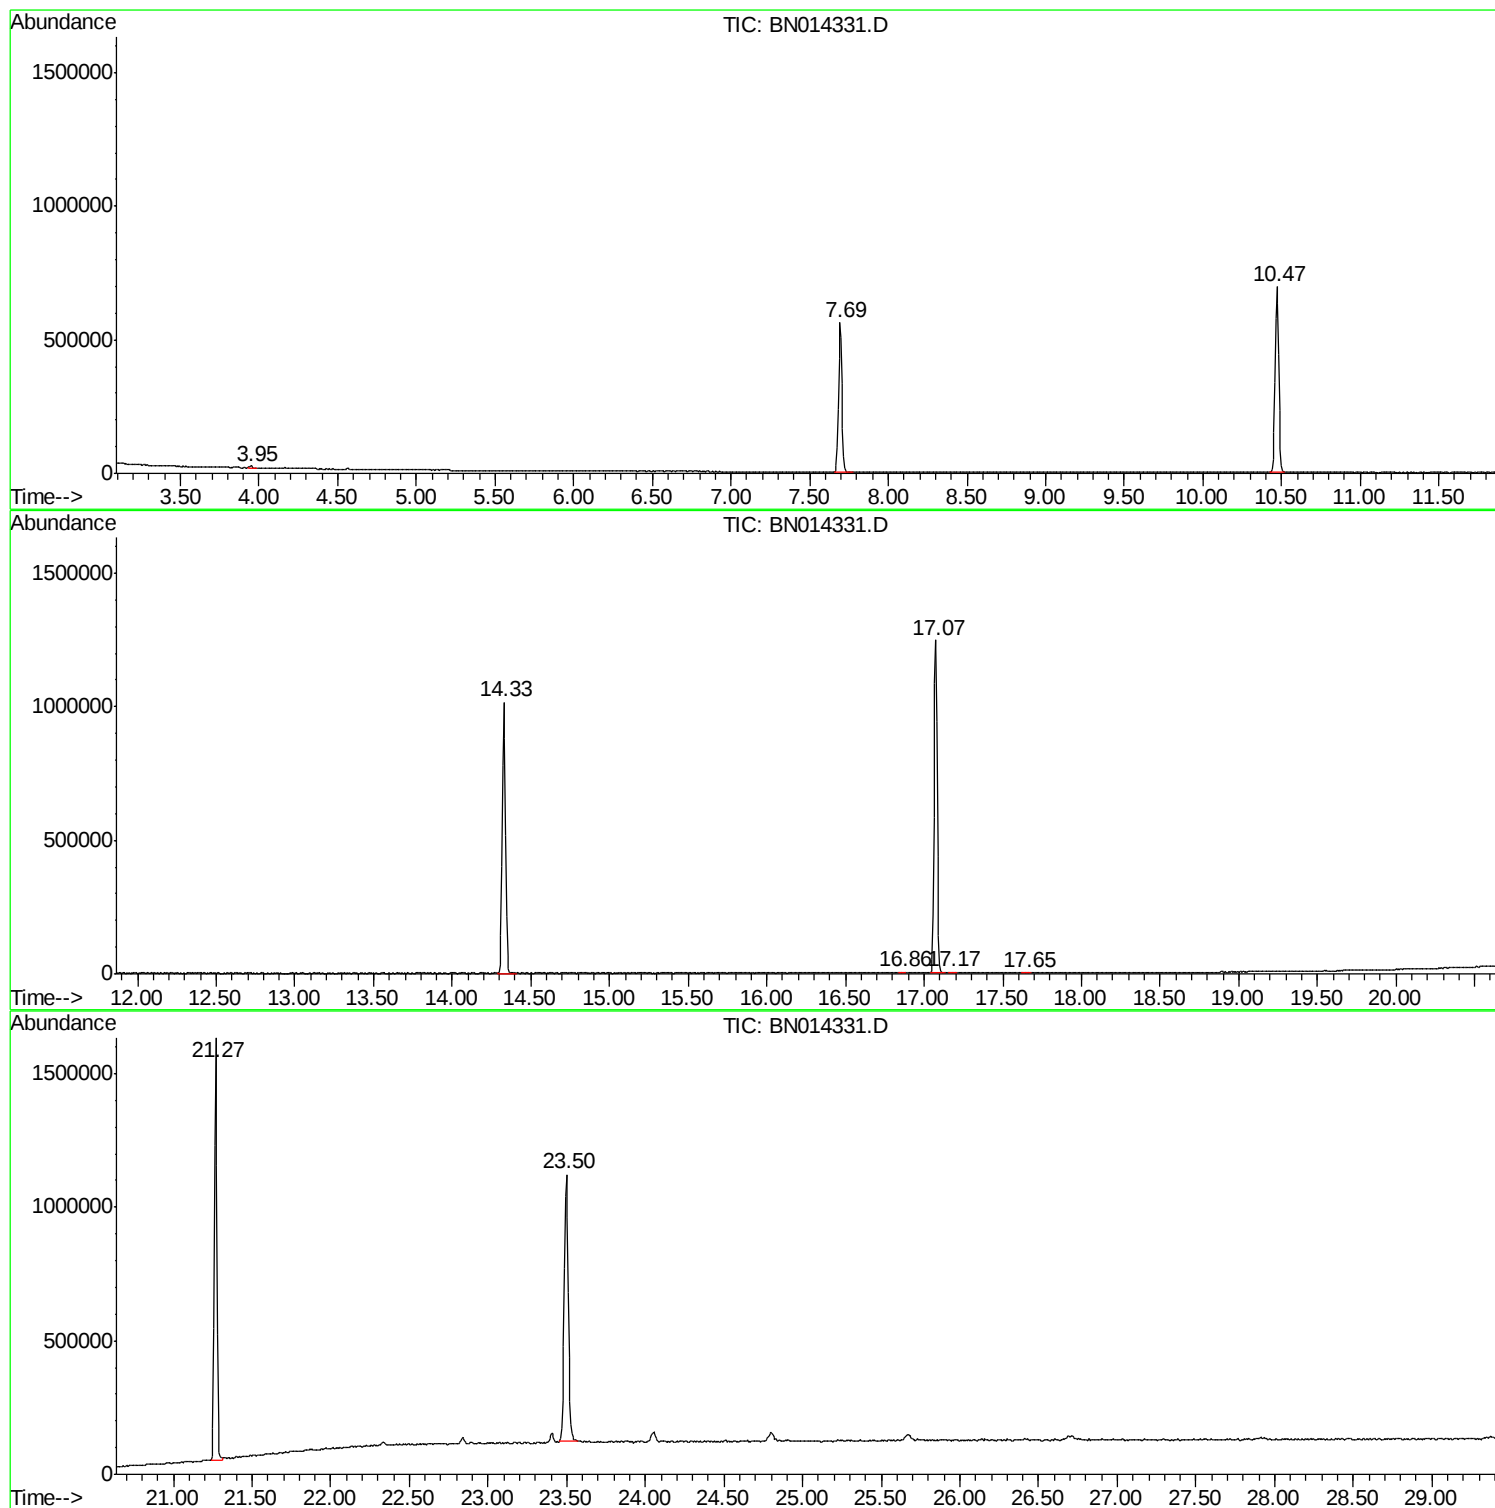

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042021\
Data File : BN014331.D
Acq On : 19 Apr 2021 19:46
Operator : CG/JU
Sample : K4649-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ATCLP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042021\
Data File : BN014331.D
Acq On : 19 Apr 2021 19:46
Operator : CG/JU
Sample : K4649-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ATCLP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc