
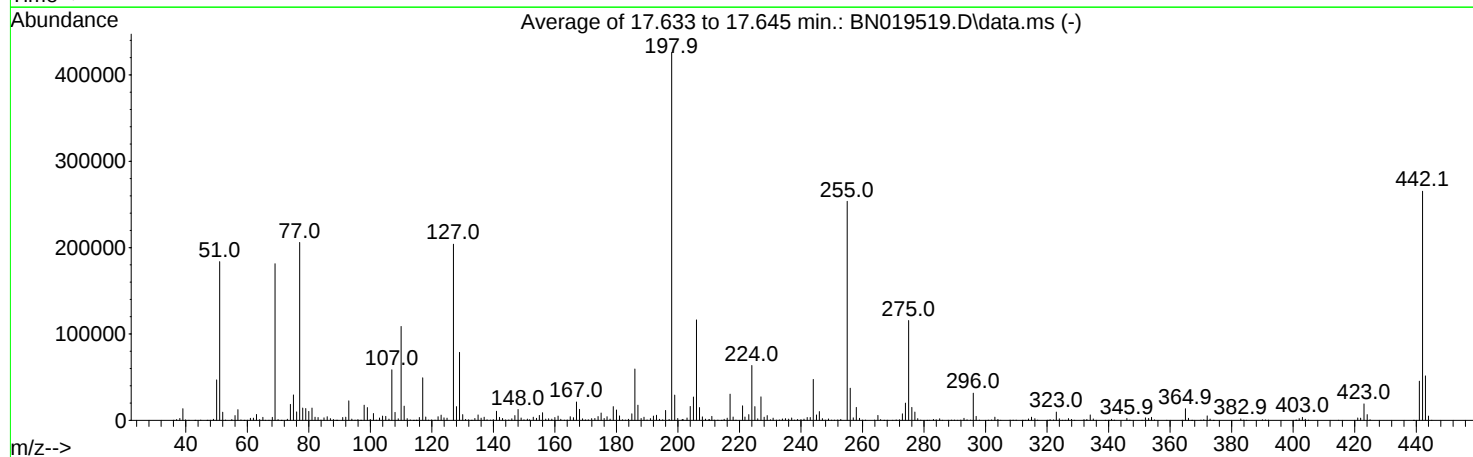


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042222\
 Data File : BN019519.D
 Acq On : 22 Apr 2022 13:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN042122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 20 17:50:10 2022

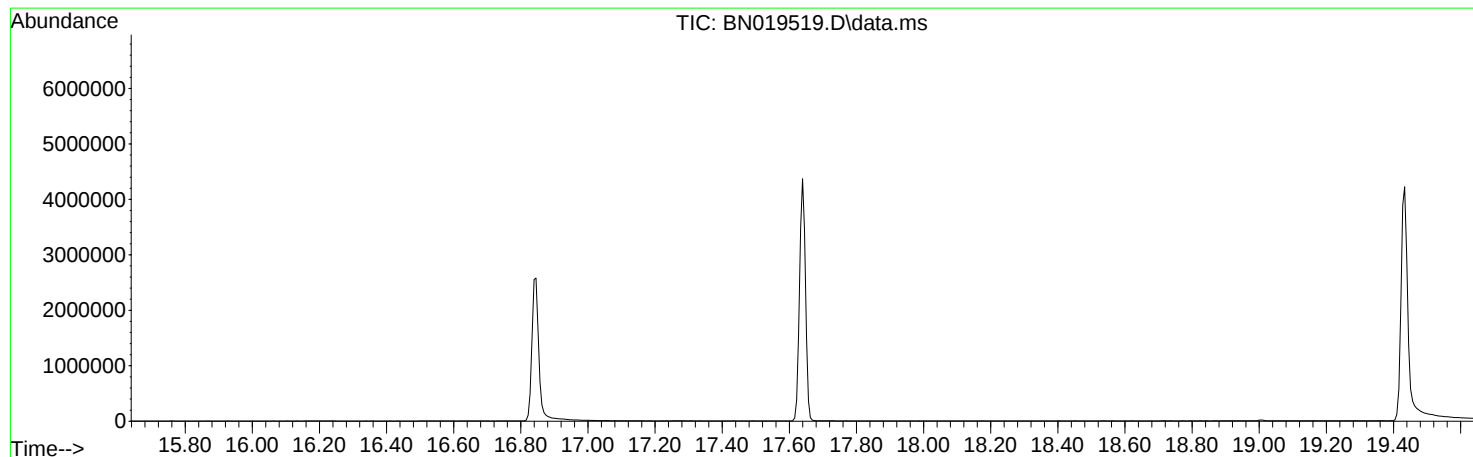

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	183829	PASS
68	69	0.00	2	1.9	3490	PASS
69	198	0.00	100	42.6	181419	PASS
70	69	0.00	2	0.6	1039	PASS
127	198	10	80	47.9	204032	PASS
197	198	0.00	2	0.3	1099	PASS
198	198	100	100	100.0	425963	PASS
199	198	5	9	6.9	29304	PASS
275	198	10	60	27.1	115613	PASS
365	198	1	100	3.2	13618	PASS
441	198	0.01	100	10.7	45387	PASS
442	442	50	100	100.0	265323	PASS
443	442	15	24	19.4	51515	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/22/2022	BNA_N	<u>BN019519.D</u>
Compound Name	Response	Retention Time
DDT	1538909	20.674
DDD	7660	20.286
DDE	456	19.735
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8116	1547025	0.52

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042222\
Data File : BN019519.D
Acq On : 22 Apr 2022 13:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 23 07:36:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

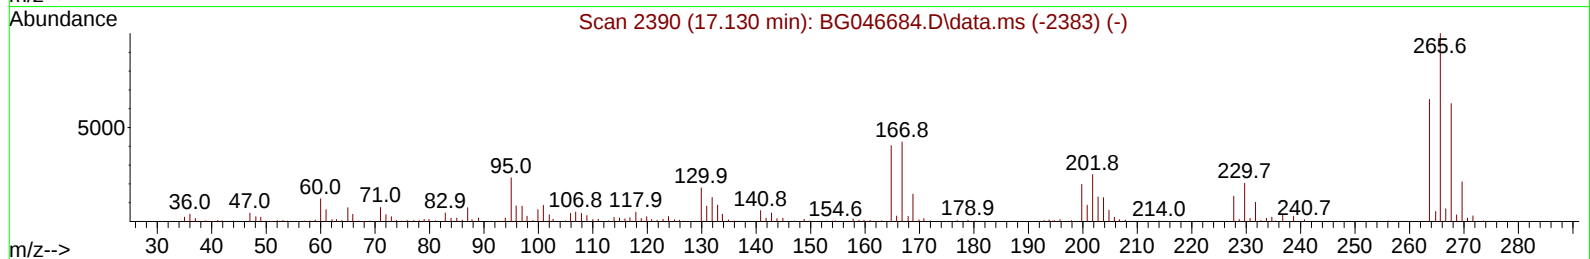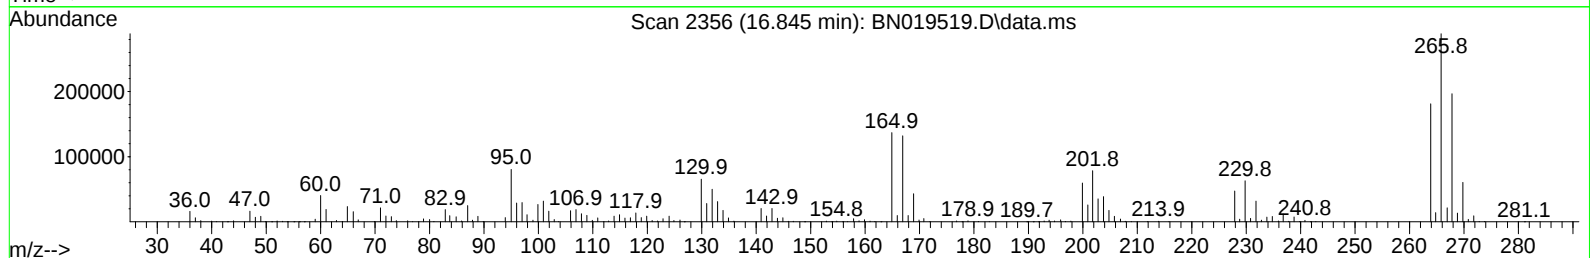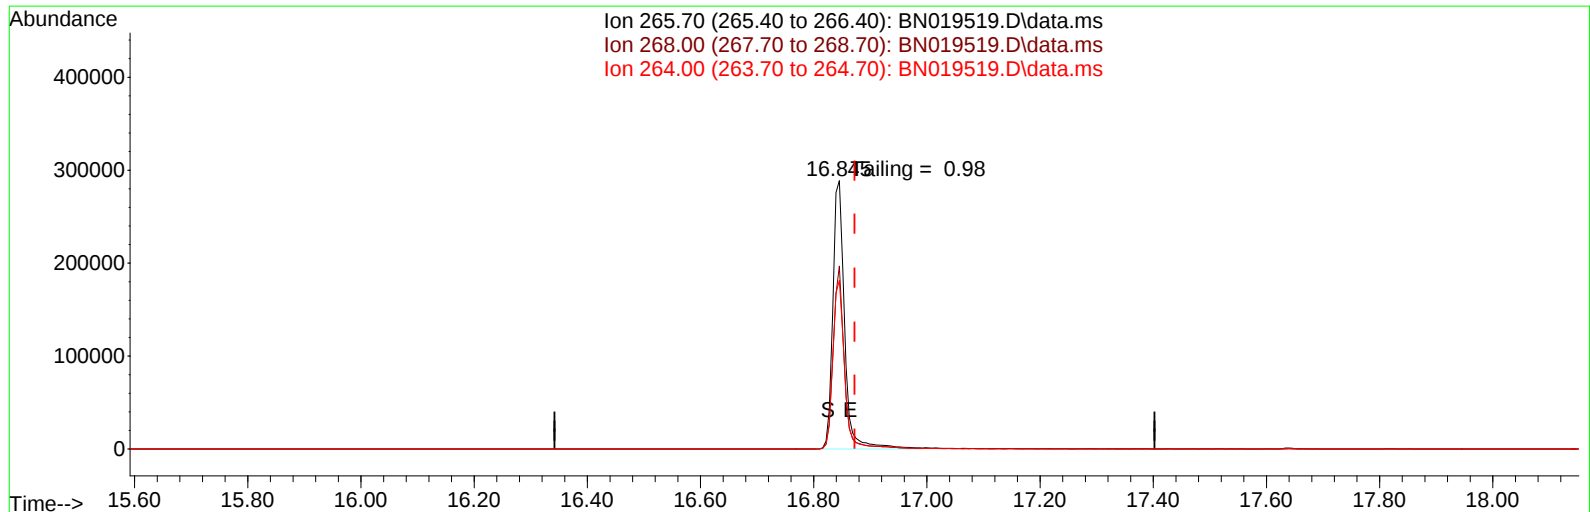

TIC: BN019519.D\data.ms

(70) Pentachlorophenol (C)

16.845min (-0.027) 17585.42 ng




response 419952

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.13
264.00	61.60	62.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042222\
Data File : BN019519.D
Acq On : 22 Apr 2022 13:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 23 07:36:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

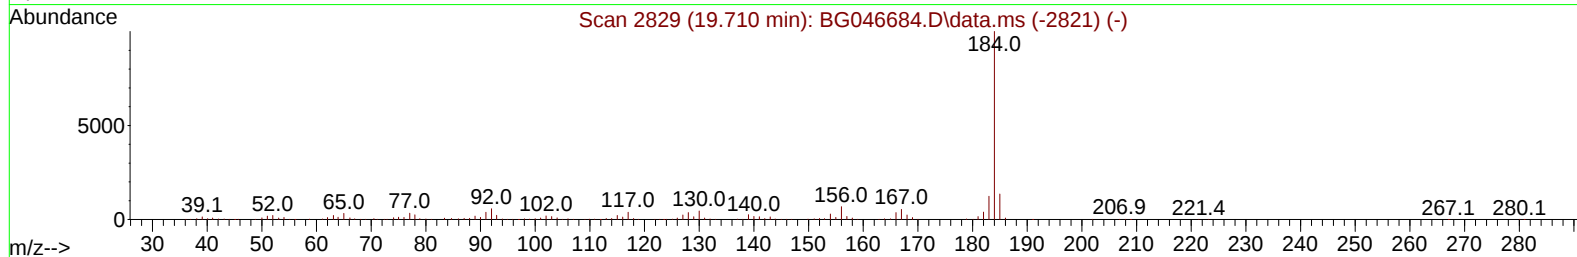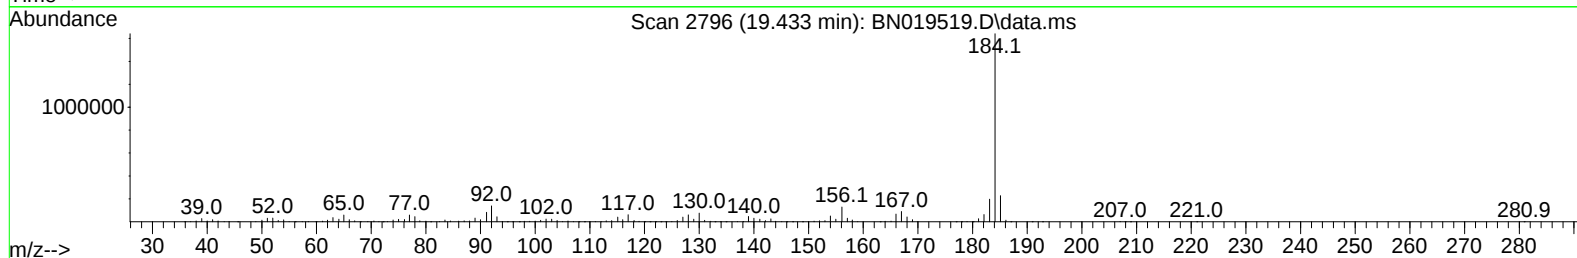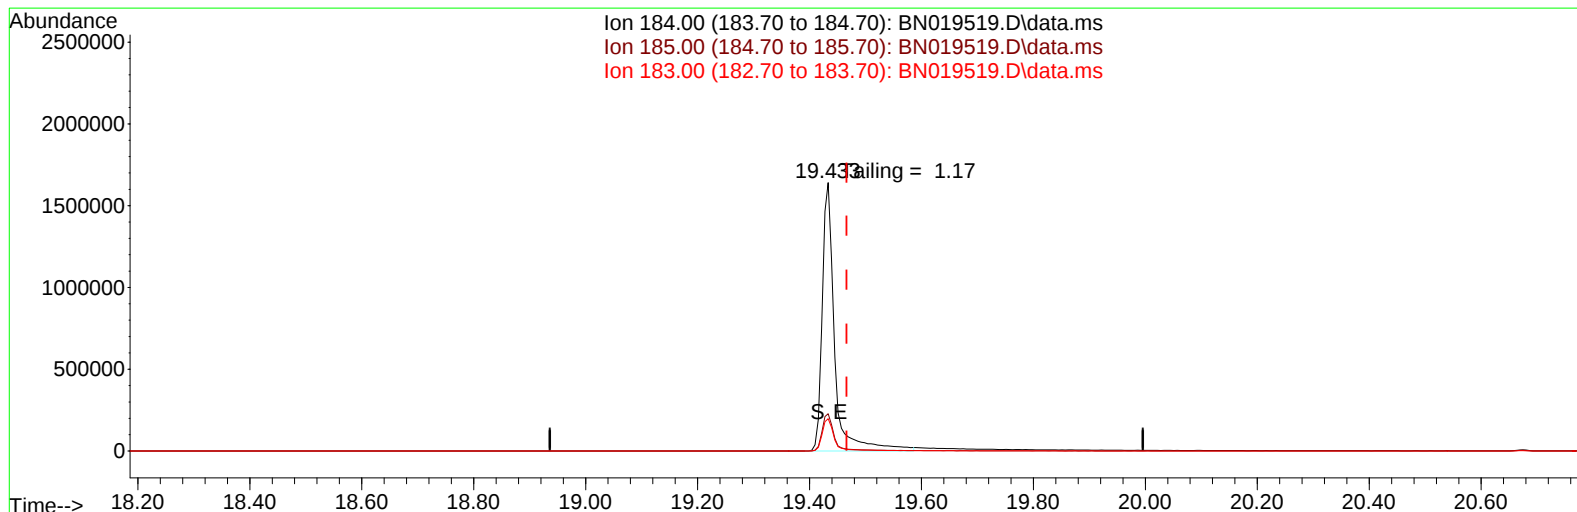

TIC: BN019519.D\data.ms

(77) Benzidine

19.433min (-0.033) 0.00 ng

response 2684062

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.88
183.00	13.20	12.05
0.00	0.00	0.00