

Data Path : Z:\HPCHEM1\BNA N\DATA\BN042418\
 Data File : BN000875.D
 Acq On : 25 Apr 2018 05:31
 Operator : JU/SJ
 Sample : J2444-21
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Apr 25 08:38:08 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN042418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 25 08:30:17 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	142204	20.00	ng/ul	0.00
2) Naphthalene-d8	10.39	136	600508	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.25	164	296539	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.00	188	596966	20.00	ng/ul	0.00
17) Chrysene-d12	21.20	240	579059	20.00	ng/ul	0.00
22) Perylene-d12	23.39	264	592312	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	13.94	160	661914	23.24	ng/ul	0.00
10) Fluorene-d10	15.25	176	455985	23.99	ng/ul	0.00
14) Anthracene-d10	17.10	188	651873	23.88	ng/ul	0.00
18) Pyrene-d10	19.40	212	695367	23.44	ng/ul	0.00
25) Benzo(a)pyrene-d12	23.25	264	733039	26.20	ng/ul	0.00
Target Compounds				Ovalue		
13) Phenanthrene	17.04	178	60058	1.845	ng/ul	99
15) Anthracene	17.04	178	60058	1.839	ng/ul	99
16) Fluoranthene	19.06	202	127656	3.864	ng/ul	95
19) Pyrene	19.43	202	105495	2.836	ng/ul#	90
20) Benzo(a)anthracene	21.19	228	65584	1.895	ng/ul	96
21) Chrysene	21.24	228	73338	2.254	ng/ul	96
23) Benzo(b)fluoranthene	22.74	252	131099	3.895	ng/ul#	91
24) Benzo(k)fluoranthene	22.74	252	131124	3.981	ng/ul#	91
26) Benzo(a)pyrene	23.29	252	61788	1.921	ng/ul#	86
27) Indeno(1,2,3-cd)pyrene	25.55	276	50026	1.287	ng/ul#	90
29) Benzo(g,h,i)perylene	26.22	276	48376	1.489	ng/ul#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA N\DATA\BN042418\
Data File : BN000875.D
Acq On : 25 Apr 2018 05:31
Operator : JU/SJ
Sample : J2444-21
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Apr 25 08:38:08 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN042418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 25 08:30:17 2018
Response via : Initial Calibration

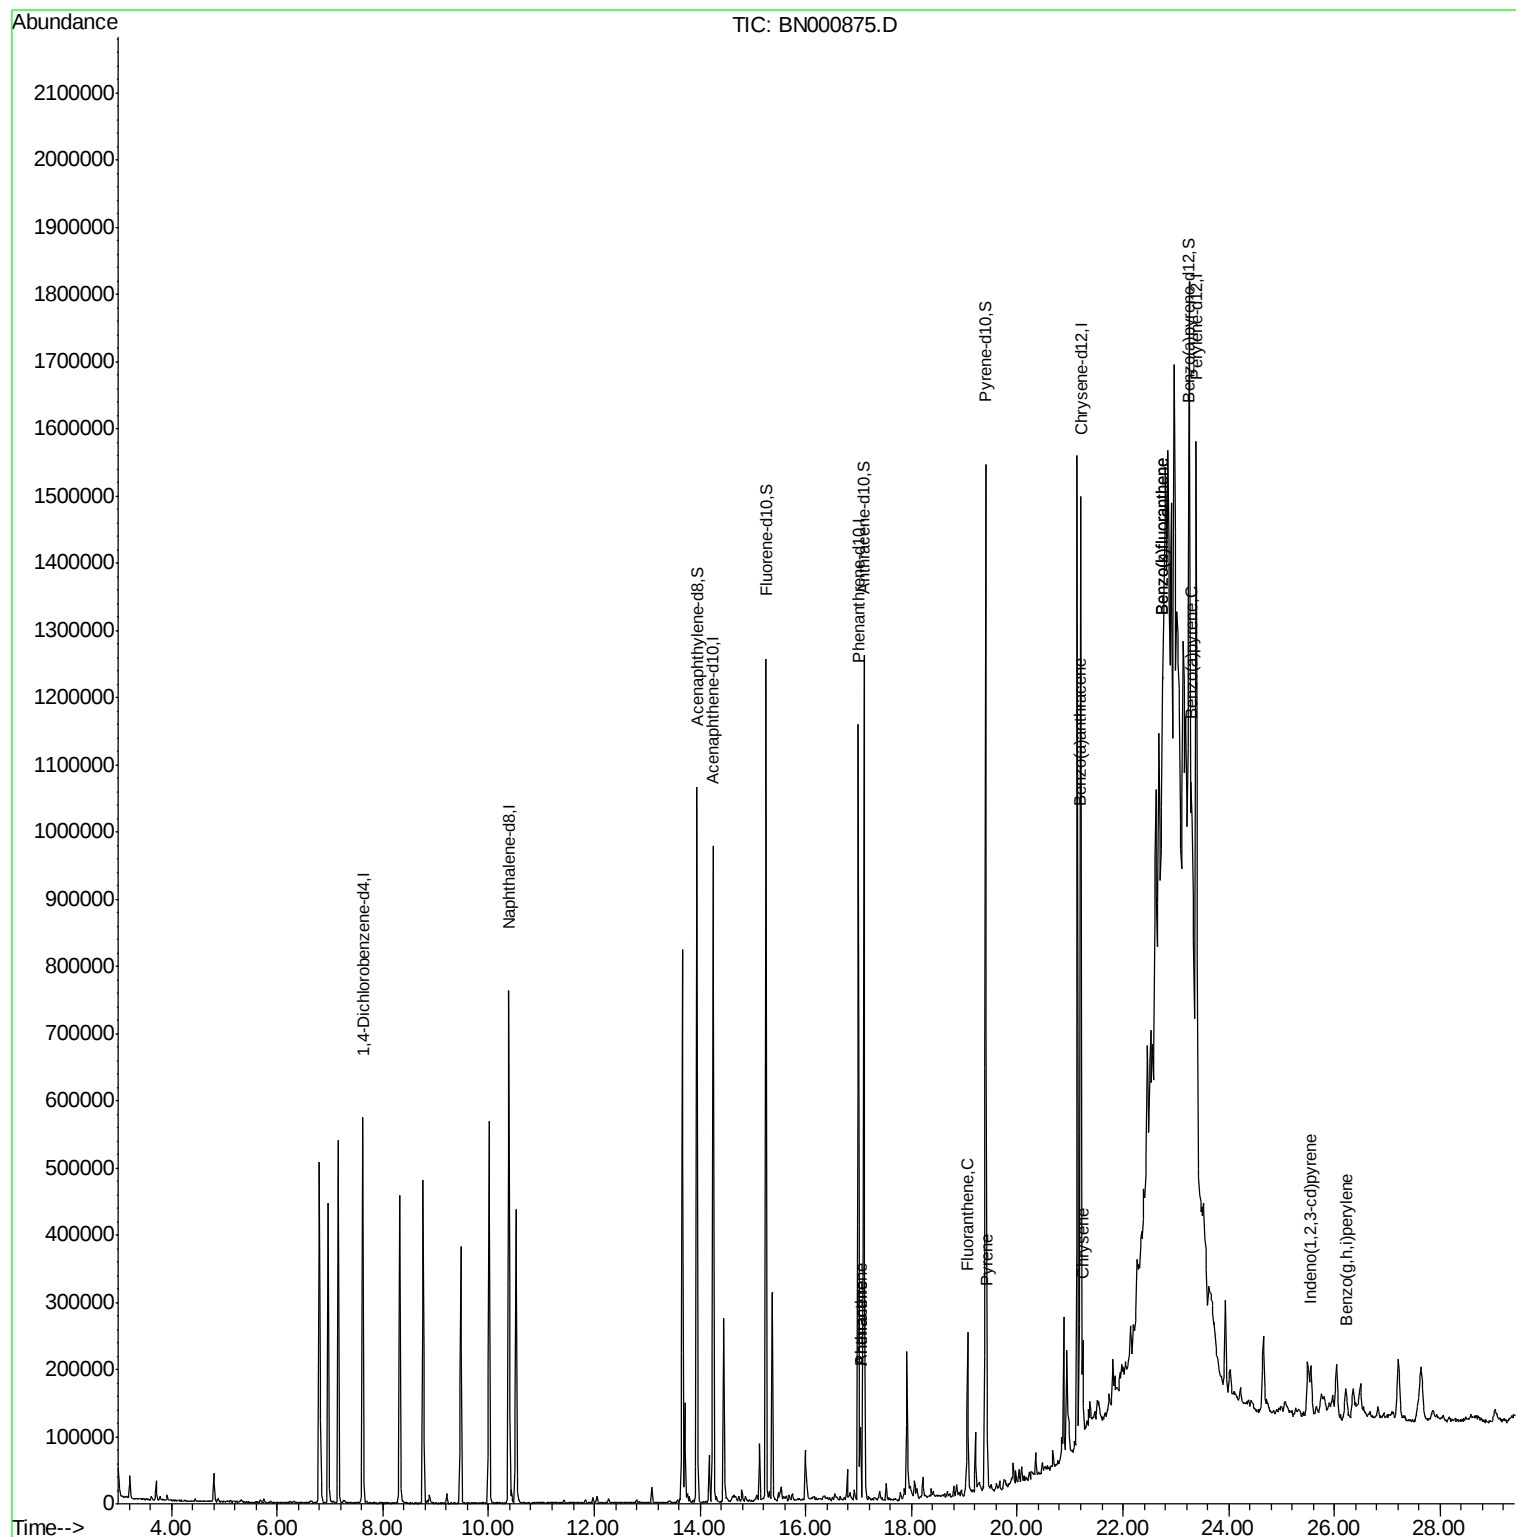

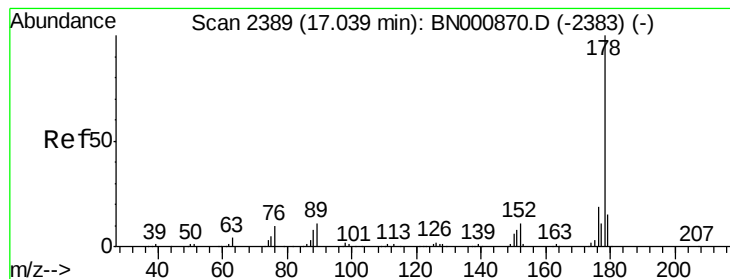

#13

Phenanthrene

Concen: 1.845 ng/ul

RT: 17.04 min Scan# 2389

Delta R.T. -0.00 min

Lab File: BN000875.D

Acq: 25 Apr 2018 05:31


Instrument :

BNA_N

ClientSampled :

Tot Ion:178 Resp: 60058

Ion	Ratio	Lower	Upper
178	100		
179	14.9	12.3	18.5
176	18.5	15.1	22.7



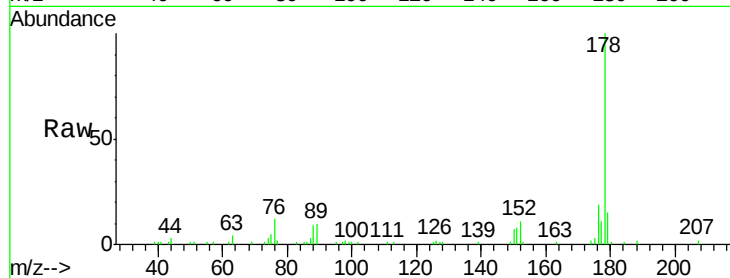


Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

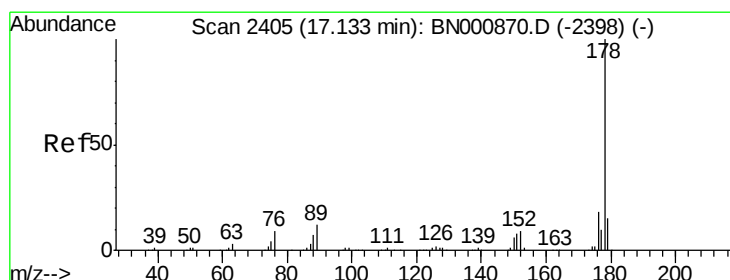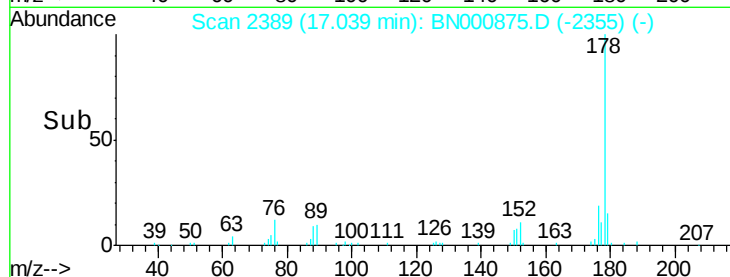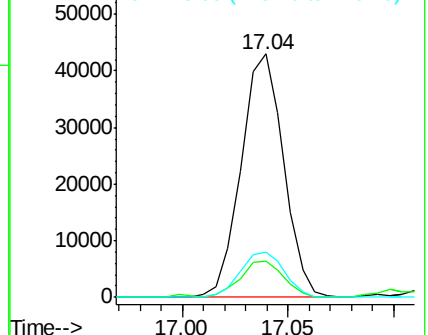

#15

Anthracene

Concen: 1.839 ng/ul

RT: 17.04 min Scan# 2389


Delta R.T. -0.09 min

Lab File: BN000875.D

Acq: 25 Apr 2018 05:31

Tgt Ion:178 Resp: 60058

Ion	Ratio	Lower	Upper
178	100		
179	14.9	11.8	17.8
176	18.5	15.2	22.8


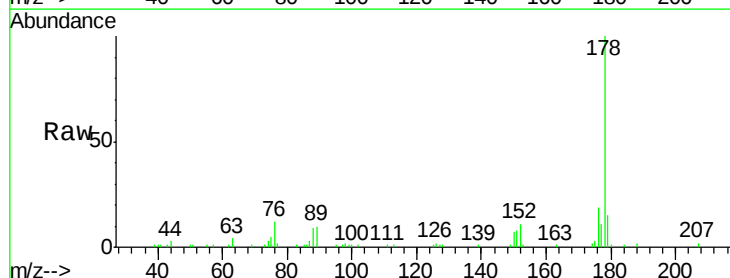



Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E



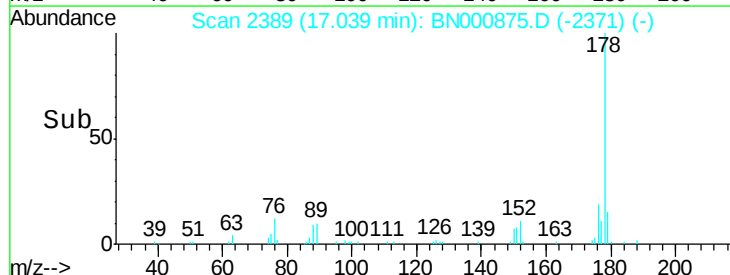
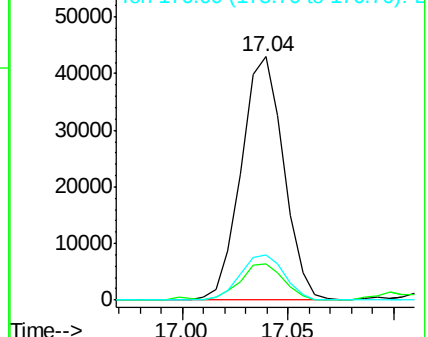




#16
Fluoranthene
 Concen: 3.864 ng/ul
 RT: 19.06 min Scan# 2733
 Delta R.T. -0.00 min
 Lab File: BN000875.D
 Acq: 25 Apr 2018 05:31




Instrument :
 BNA_N
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
202	100		
101	14.7	9.9	14.9
100	10.9	7.4	11.0

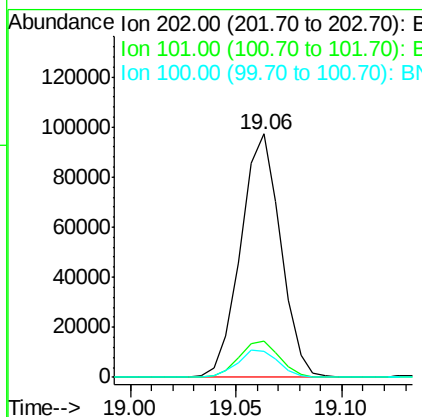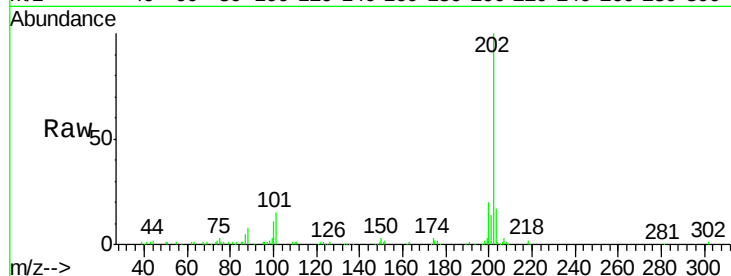

#19
Pyrene
 Concen: 2.836 ng/ul
 RT: 19.43 min Scan# 2795
 Delta R.T. -0.00 min
 Lab File: BN000875.D
 Acq: 25 Apr 2018 05:31

Tgt Ion	Ratio	Lower	Upper
202	100		
101	17.1	11.0	16.4#
100	14.3	8.1	12.1#

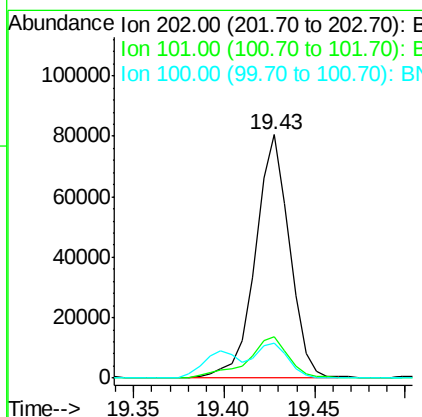

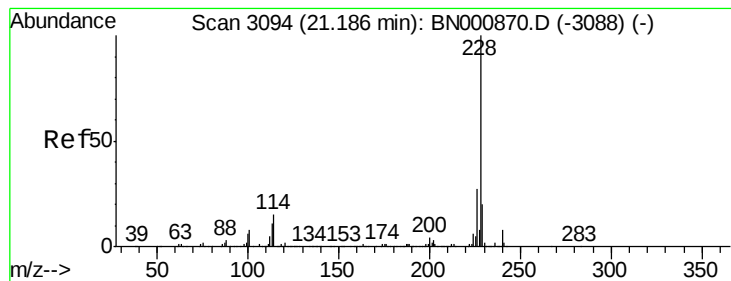

#20

Benzo(a)anthracene

Concen: 1.895 ng/ul

RT: 21.19 min Scan# 3094

Delta R.T. -0.00 min

Lab File: BN000875.D

Acq: 25 Apr 2018 05:31

Instrument :

BNA_N

ClientSampleId :


Tot Ion:228 Resp: 65584

Ion Ratio Lower Upper

228 100

229 21.5 15.7 23.5




226 28.4 21.1 31.7



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

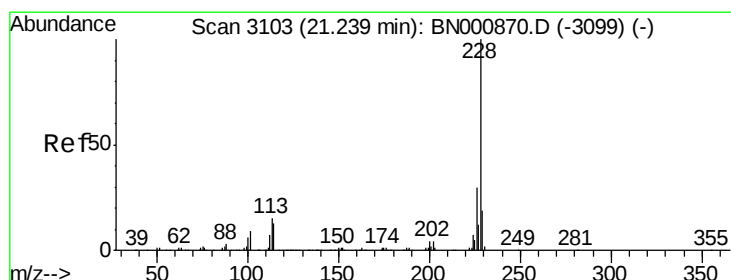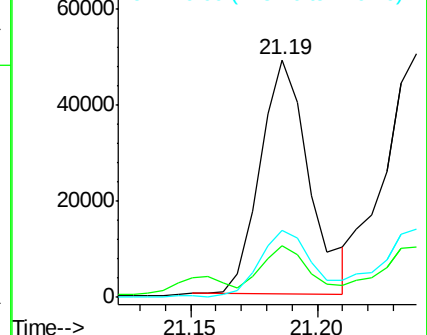

#21

Chrysene

Concen: 2.254 ng/ul

RT: 21.24 min Scan# 3103

Delta R.T. -0.00 min

Lab File: BN000875.D

Acq: 25 Apr 2018 05:31


Tgt Ion:228 Resp: 73338

Ion Ratio Lower Upper

228 100

226 28.1 24.5 36.7



229 20.9 15.8 23.8




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

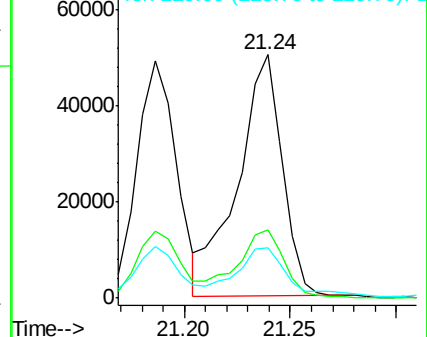



#23

Benzo(b)fluoranthene

Concen: 3.895 ng/ul

RT: 22.74 min Scan# 3358

Delta R.T. -0.00 min

Lab File: BN000875.D

Acq: 25 Apr 2018 05:31

Instrument :

BNA_N

ClientSampleId :





Tot Ion:252 Resp: 131099

Ion Ratio Lower Upper

252 100

253 23.4 18.0 27.0

125 19.3 8.0 12.0#

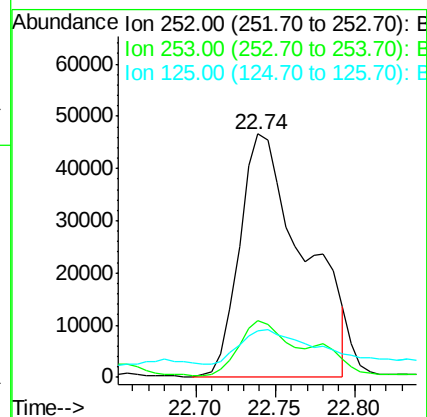

#24

Benzo(k)fluoranthene

Concen: 3.981 ng/ul

RT: 22.74 min Scan# 3358

Delta R.T. -0.05 min

Lab File: BN000875.D

Acq: 25 Apr 2018 05:31




Tgt Ion:252 Resp: 131124


Ion Ratio Lower Upper

252 100

253 23.4 18.0 27.0

125 19.3 8.1 12.1#

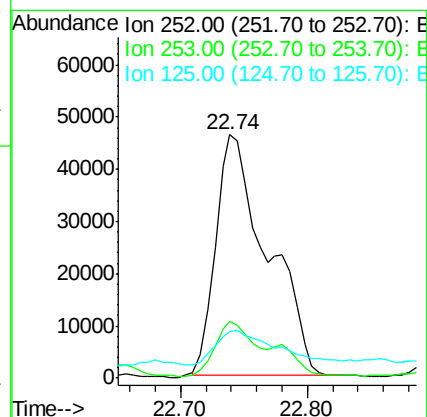

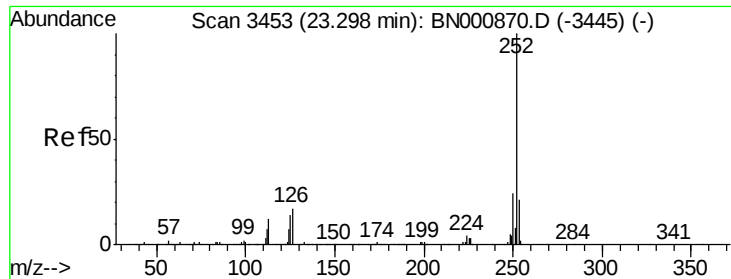

#26

Benzo(a)pyrene

Concen: 1.921 ng/ul

RT: 23.29 min Scan# 3452

Delta R.T. -0.01 min

Lab File: BN000875.D

Acq: 25 Apr 2018 05:31

Instrument :

BNA_N

ClientSampleId :


Tot Ion:252 Resp: 61788

Ion Ratio Lower Upper

252 100

253 23.6 17.2 25.8

125 23.3 8.2 12.4#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

Time-->




Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

Time-->



#27

Indeno(1,2,3-cd)pyrene

Concen: 1.287 ng/ul

RT: 25.55 min Scan# 3836

Delta R.T. -0.01 min

Lab File: BN000875.D

Acq: 25 Apr 2018 05:31


Tgt Ion:276 Resp: 50026

Ion Ratio Lower Upper

276 100

138 25.9 14.4 21.6#

277 23.9 18.0 27.0




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

Time-->




Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

Time-->

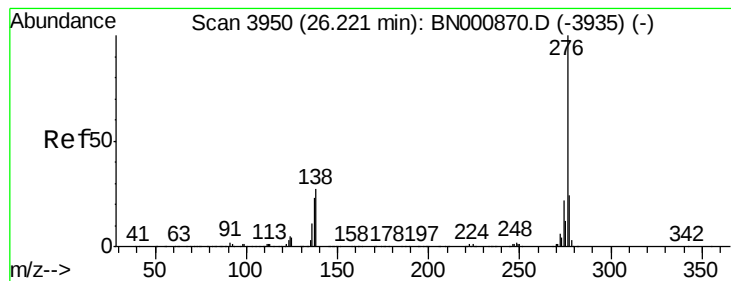

#29

Benzo(a,h,i)perylene

Concen: 1.489 ng/ul

RT: 26.22 min Scan# 3949

Delta R.T. -0.01 min

Lab File: BN000875.D

Acq: 25 Apr 2018 05:31

Instrument :

BNA_N

ClientSampleId :


Tot Ion:276 Resp: 48376

Ion Ratio Lower Upper

276 100

138 27.9 15.3 22.9#

277 23.1 19.0 28.4

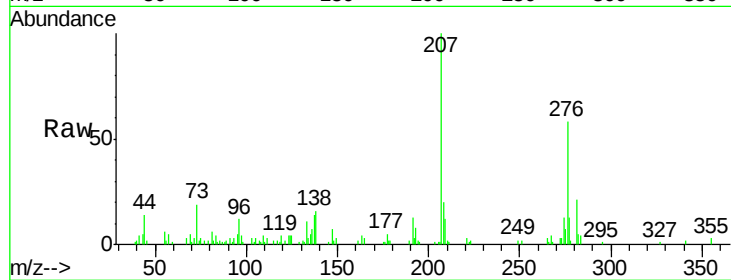

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

