

Data Path : Z:\HPCHEM1\BNA N\DATA\BN042418\
 Data File : BN000852.D
 Acq On : 24 Apr 2018 16:14
 Operator : JU/SJ
 Sample : J2443-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DARR6

Quant Time: Apr 25 07:44:20 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN042418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 24 13:09:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	115757	20.00	ng/ul	0.00
2) Naphthalene-d8	10.39	136	501773	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.25	164	261805	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.00	188	536073	20.00	ng/ul	0.00
17) Chrysene-d12	21.20	240	515003	20.00	ng/ul	0.00
22) Perylene-d12	23.39	264	533687	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	13.94	160	736602	29.30	ng/ul	0.00
10) Fluorene-d10	15.25	176	523923	31.22	ng/ul	0.00
14) Anthracene-d10	17.10	188	748222	30.52	ng/ul	0.00
18) Pyrene-d10	19.40	212	804270	30.48	ng/ul	0.00
25) Benzo(a)pyrene-d12	23.25	264	864540	34.29	ng/ul	0.00
Target Compounds						
16) Fluoranthene	19.06	202	35331	1.191	ng/ul#	Ovalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA N\DATA\BN042418\
Data File : BN000852.D
Acq On : 24 Apr 2018 16:14
Operator : JU/SJ
Sample : J2443-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DARR6

Quant Time: Apr 25 07:44:20 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN042418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 24 13:09:24 2018
Response via : Initial Calibration

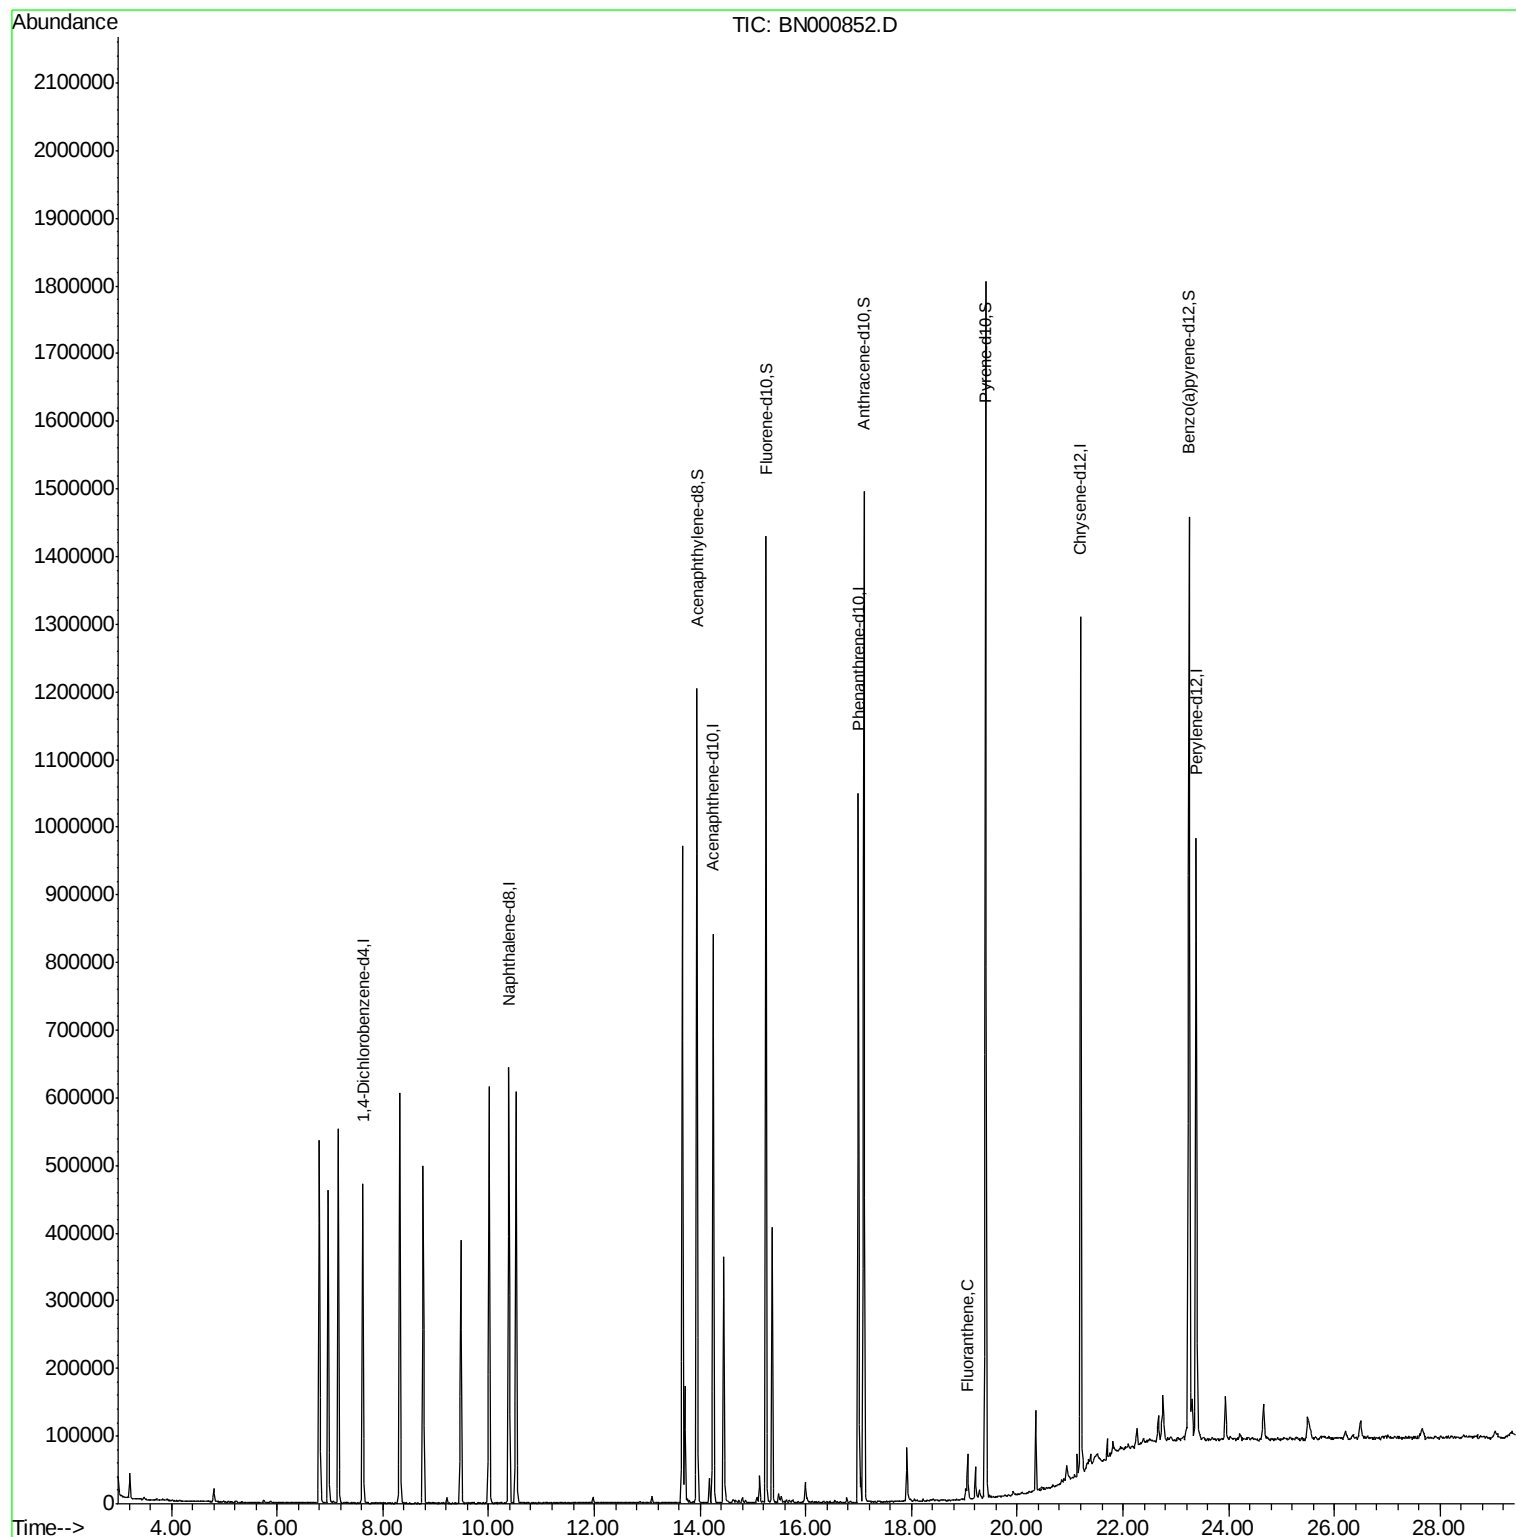

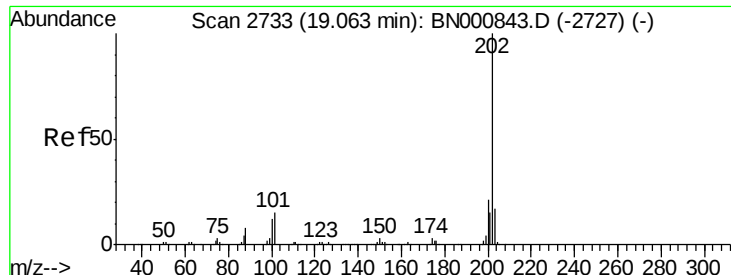

#16

Fluoranthene

Concen: 1.191 ng/ul

RT: 19.06 min Scan# 2733

Delta R.T. -0.00 min

Lab File: BN000852.D

Acq: 24 Apr 2018 16:14

Instrument :

BNA_N

ClientSampleId :

DARR6


Tot Ion:202 Resp: 35331

Ion Ratio Lower Upper

202 100

101 13.0 9.9 14.9

100 11.2 7.4 11.0#

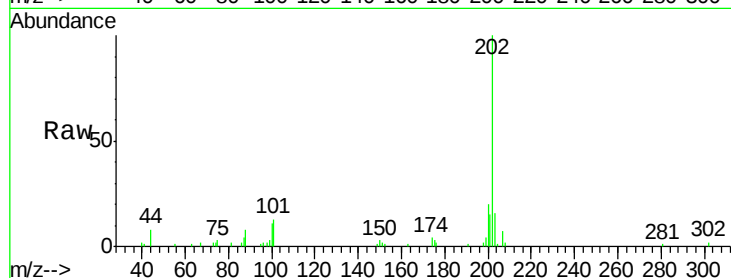

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

