

Data Path : Z:\HPCHEM1\BNA N\DATA\BN042418\
 Data File : BN000876.D
 Acq On : 25 Apr 2018 06:05
 Operator : JU/SJ
 Sample : J2444-22
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAS26

Quant Time: Apr 25 08:38:20 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN042418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 25 08:30:17 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	188654	20.00	ng/ul	0.00
2) Naphthalene-d8	10.39	136	840376	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.25	164	420734	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.00	188	797868	20.00	ng/ul	0.00
17) Chrysene-d12	21.20	240	608301	20.00	ng/ul	0.00
22) Perylene-d12	23.39	264	633938	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	13.94	160	980116	24.26	ng/ul	0.00
10) Fluorene-d10	15.25	176	663014	24.58	ng/ul	0.00
14) Anthracene-d10	17.10	188	890208	24.40	ng/ul	0.00
18) Pyrene-d10	19.40	212	836732	26.85	ng/ul	0.00
25) Benzo(a)pyrene-d12	23.25	264	813260	27.16	ng/ul	0.00
Target Compounds						
23) Benzo(b)fluoranthene	22.74	252	36405	1.010	ng/ul#	Ovalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA N\DATA\BN042418\
Data File : BN000876.D
Acq On : 25 Apr 2018 06:05
Operator : JU/SJ
Sample : J2444-22
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DAS26

Quant Time: Apr 25 08:38:20 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN042418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 25 08:30:17 2018
Response via : Initial Calibration

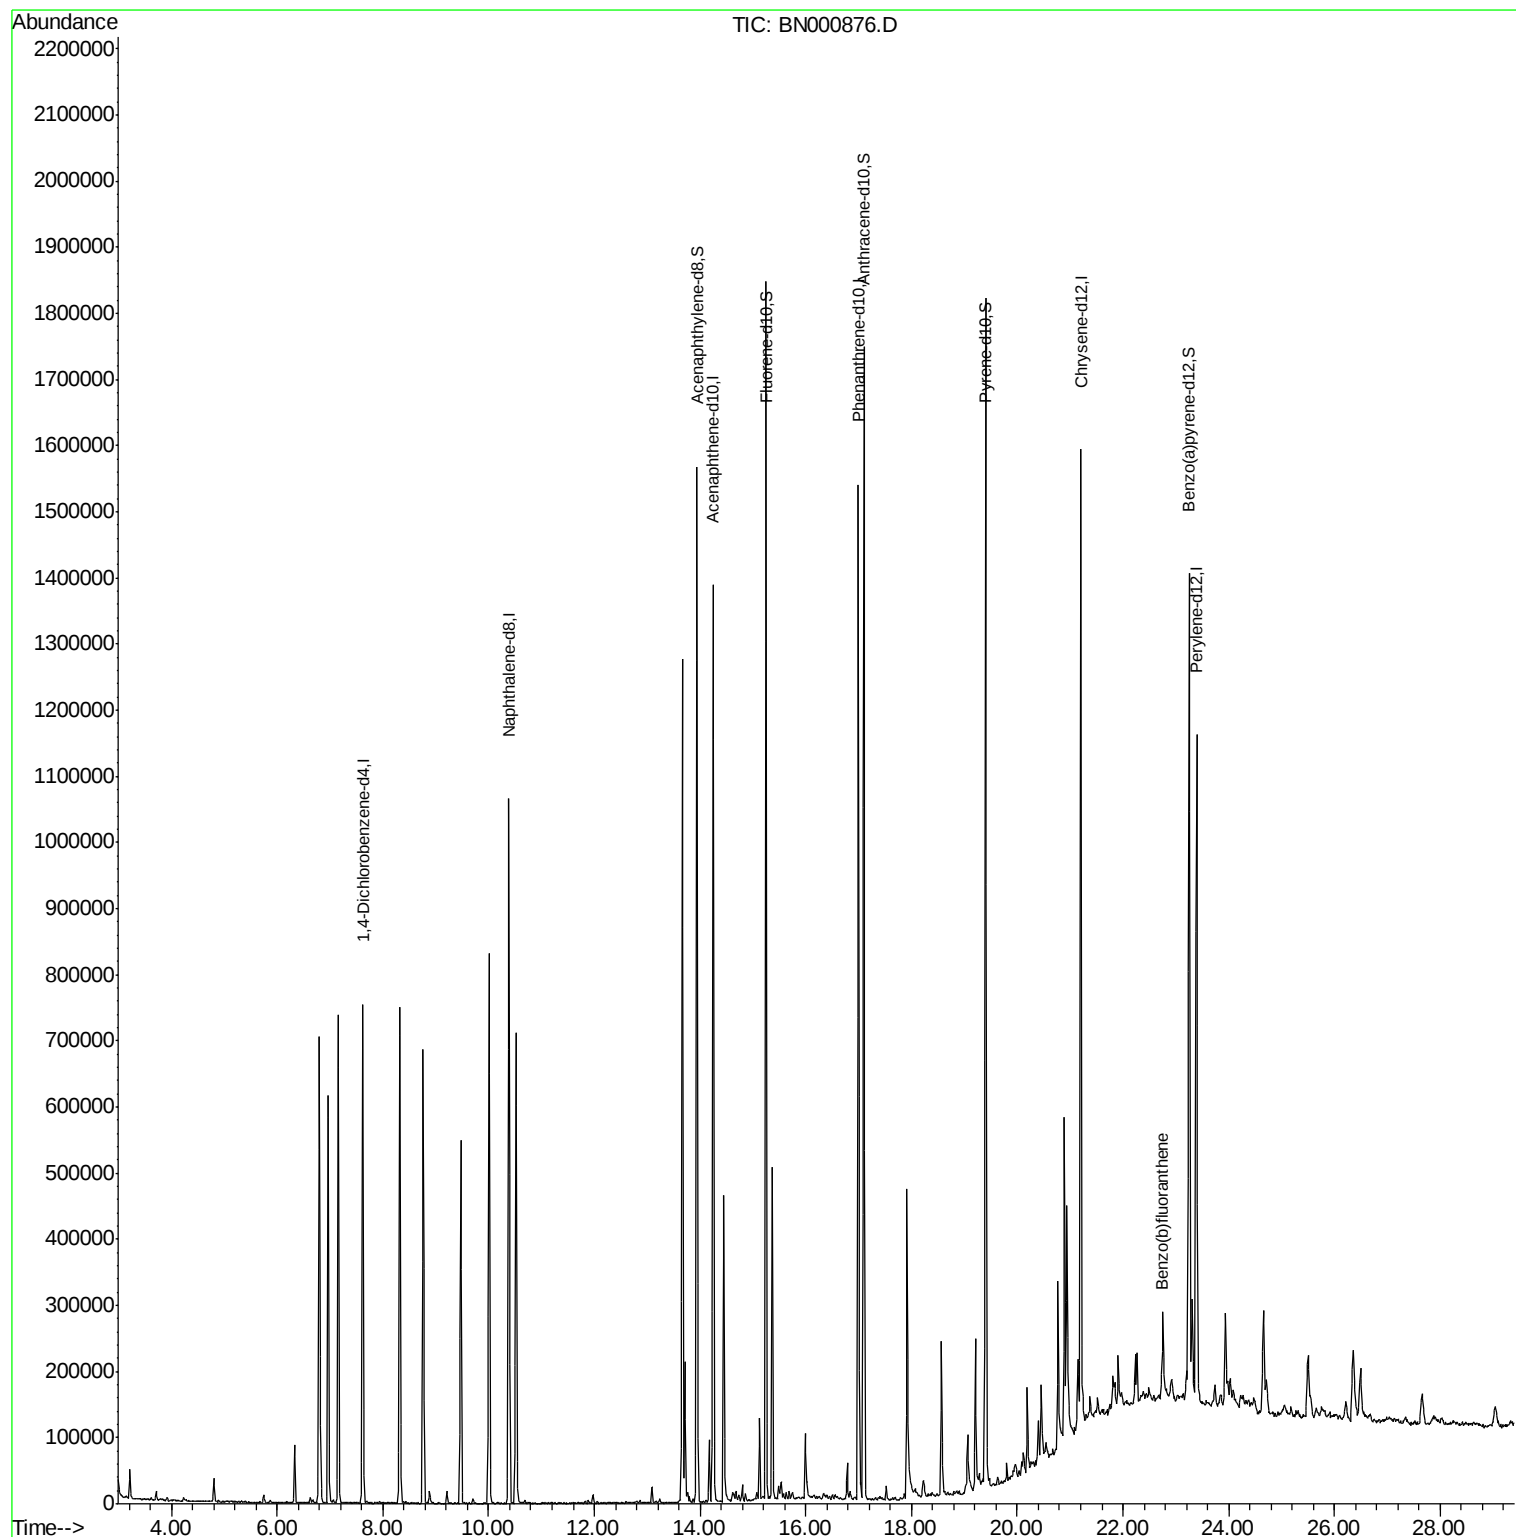

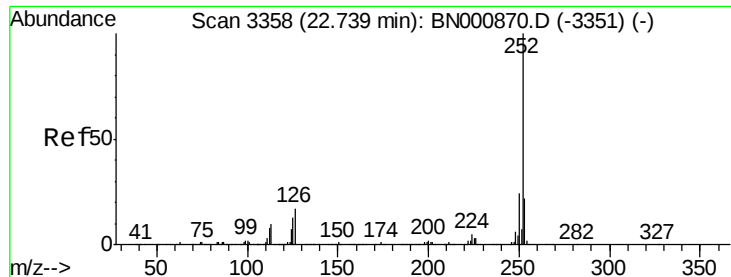

#23

Benzo(b)fluoranthene

Concen: 1.010 ng/ul

RT: 22.74 min Scan# 3358

Delta R.T. -0.00 min

Lab File: BN000876.D

Acq: 25 Apr 2018 06:05

Instrument :

BNA_N

ClientSampleId :

DAS26

Tot Ion:252 Resp: 36405

Ion Ratio Lower Upper

252 100

253 24.8 18.0 27.0

125 18.0 8.0 12.0#

