

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
 Data File : BN014398.D
 Acq On : 24 Apr 2021 12:09
 Operator : CG/JU
 Sample : M2065-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG572

Quant Time: Apr 26 01:48:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 23 12:06:34 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	138591	20.00	ng/ul	0.00
20) Naphthalene-d8	10.46	136	580141	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.32	164	338075	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.06	188	685674	20.00	ng/ul	0.00
79) Chrysene-d12	21.26	240	667615	20.00	ng/ul	0.00
88) Perylene-d12	23.49	264	675209	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.21	96	7910	2.17	ng/uL	0.00
4) Pyridine-d5	3.62	84	37458	3.88	ng/ul	0.01
7) Phenol-d5	6.85	99	171689	14.82	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.02	67	116555	16.80	ng/ul	0.00
11) 2-Chlorophenol-d4	7.22	132	151760	16.65	ng/ul	0.00
15) 4-Methylphenol-d8	8.38	113	139706	15.91	ng/ul	0.00
21) Nitrobenzene-d5	8.83	128	79030	18.85	ng/ul	0.00
24) 2-Nitrophenol-d4	9.55	143	65188	15.88	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.08	165	130598	14.77	ng/ul	0.00
31) 4-Chloroaniline-d4	10.59	131	185162	14.11	ng/ul	0.00
46) Dimethylphthalate-d6	13.73	166	436141	17.81	ng/ul	0.00
49) Acenaphthylene-d8	14.01	160	566119	19.21	ng/ul	0.00
54) 4-Nitrophenol-d4	14.52	143	35421	7.46	ng/ul	0.00
60) Fluorene-d10	15.32	176	380631	17.58	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.43	200	20431	5.57	ng/ul	0.00
73) Anthracene-d10	17.16	188	558792	17.46	ng/ul	0.00
81) Pyrene-d10	19.46	212	624968	19.28	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.35	264	624826	17.44	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.77	163	54366	2.138	ng/ul	Ovalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014398.D
Acq On : 24 Apr 2021 12:09
Operator : CG/JU
Sample : M2065-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG572

Quant Time: Apr 26 01:48:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 23 12:06:34 2021
Response via : Initial Calibration

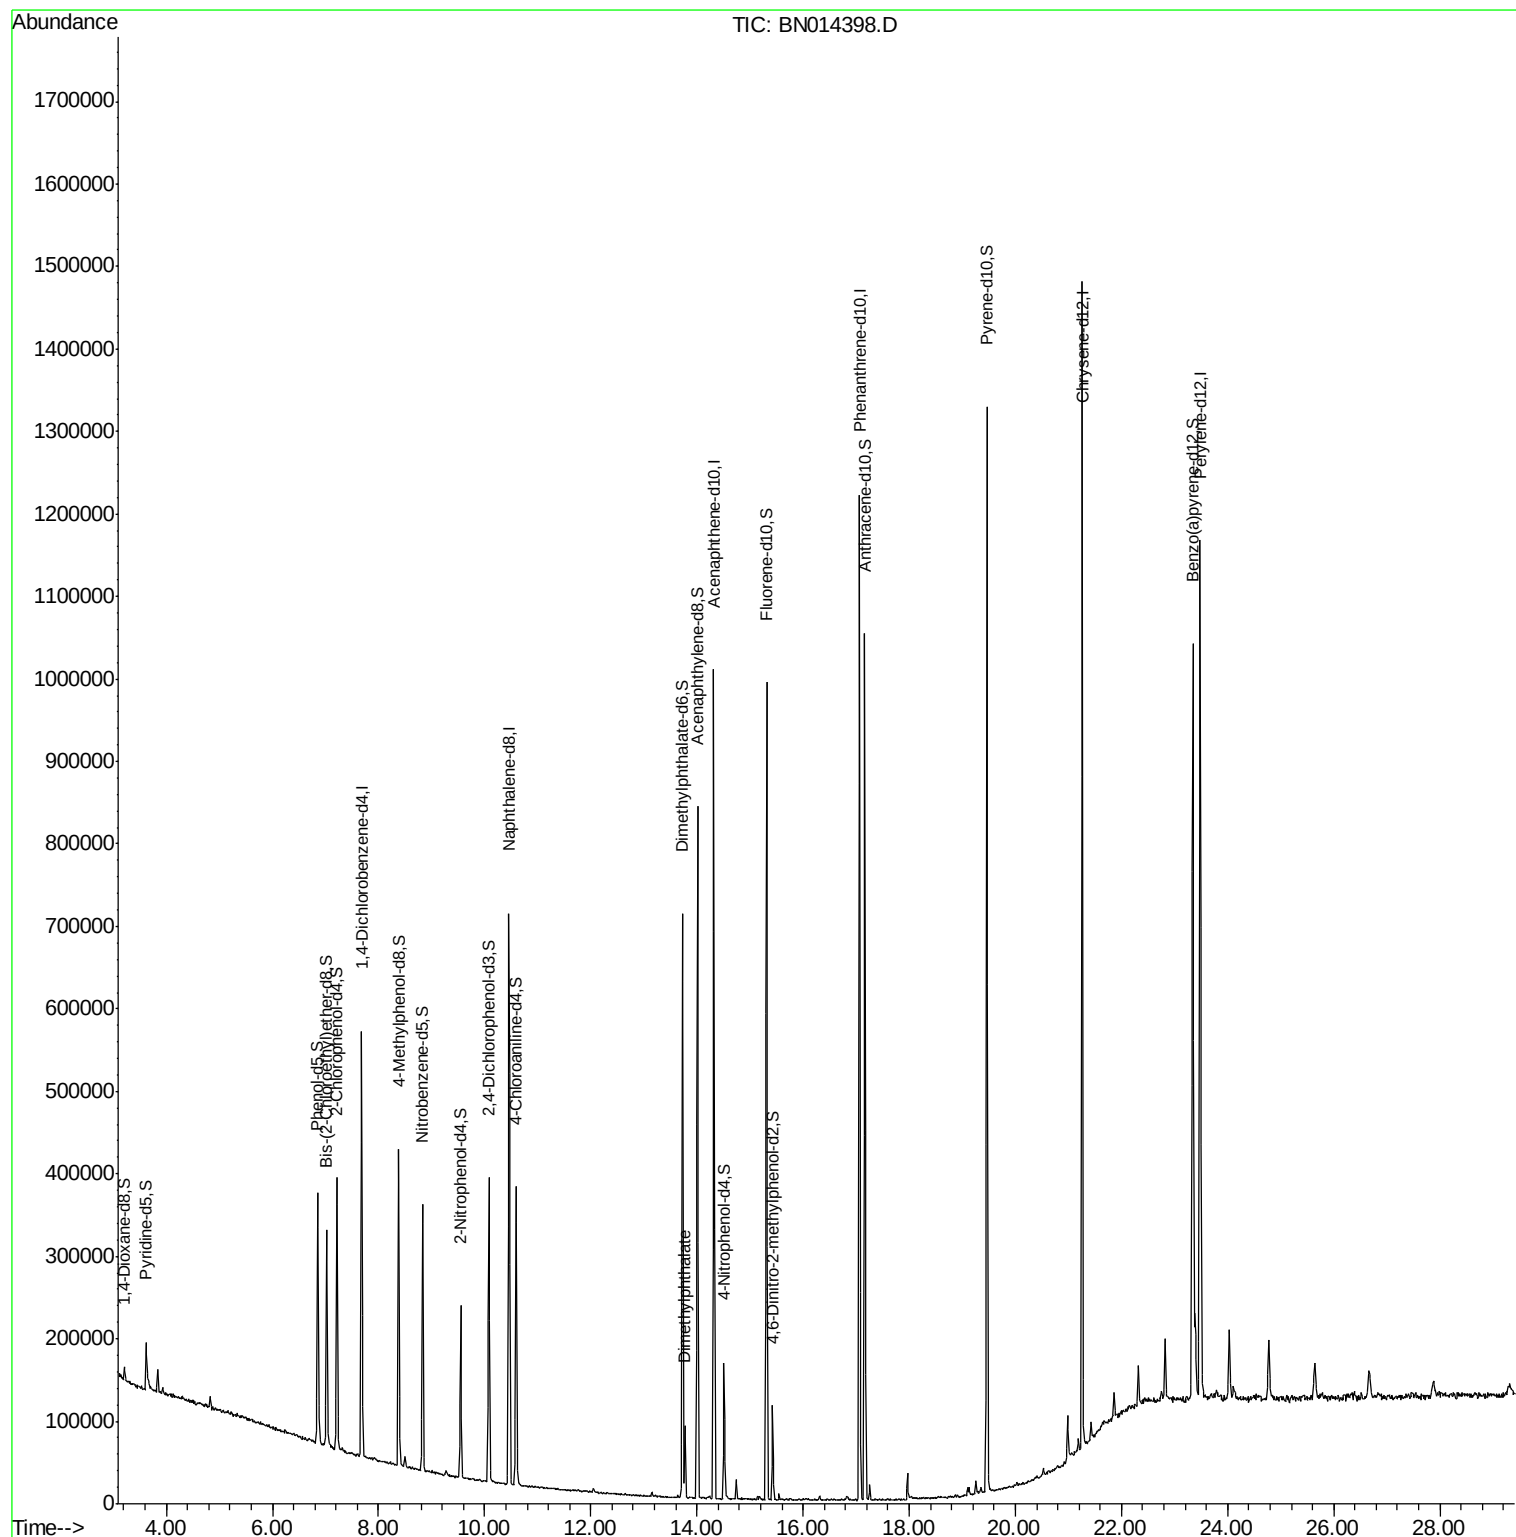

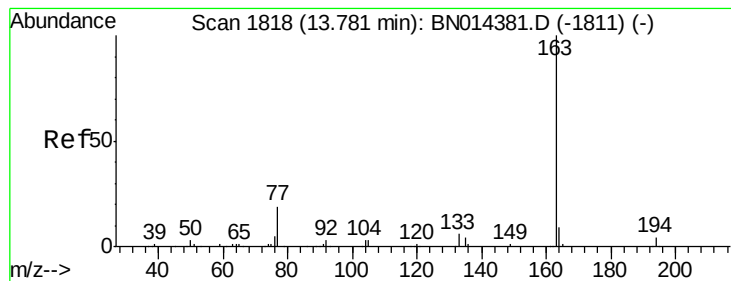

#47

Dimethylphthalate

Concen: 2.138 ng/ul

RT: 13.77 min Scan# 1817

Delta R.T. -0.01 min

Lab File: BN014398.D

Acq: 24 Apr 2021 12:09

Instrument :

BNA_N

ClientSampleId :

BG572


Tot Ion:163 Resp: 54366

Ion Ratio Lower Upper

163 100

194 3.9 3.3 4.9

164 10.0 7.8 11.8

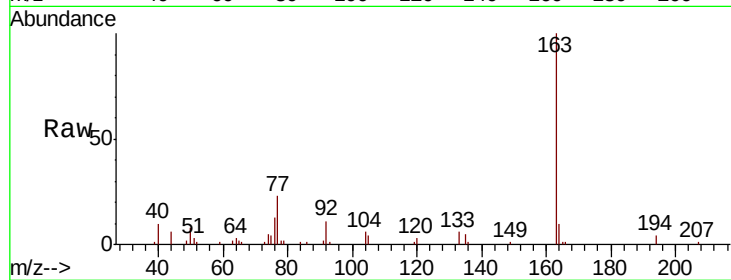

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

