

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
 Data File : BN014420.D
 Acq On : 25 Apr 2021 01:48
 Operator : CG/JU
 Sample : M2065-09
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG562

Quant Time: Apr 26 01:53:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 23 12:06:34 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	125264	20.00	ng/ul	0.00
20) Naphthalene-d8	10.46	136	534876	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.32	164	308849	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.06	188	673764	20.00	ng/ul	0.00
79) Chrysene-d12	21.26	240	741248	20.00	ng/ul	0.00
88) Perylene-d12	23.48	264	675743	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.21	96	6756	2.05	ng/uL	0.00
4) Pyridine-d5	3.63	84	18994	2.18	ng/ul	0.02
7) Phenol-d5	6.85	99	136413	13.03	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.02	67	96809	15.44	ng/ul	0.00
11) 2-Chlorophenol-d4	7.22	132	120434	14.62	ng/ul	0.00
15) 4-Methylphenol-d8	8.38	113	106845	13.46	ng/ul	0.00
21) Nitrobenzene-d5	8.83	128	67127	17.37	ng/ul	0.00
24) 2-Nitrophenol-d4	9.55	143	48820	12.90	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.08	165	107334	13.16	ng/ul	0.00
31) 4-Chloroaniline-d4	10.59	131	143854	11.89	ng/ul	0.00
46) Dimethylphthalate-d6	13.73	166	384815	17.20	ng/ul	0.00
49) Acenaphthylene-d8	14.01	160	503286	18.70	ng/ul	0.00
54) 4-Nitrophenol-d4	14.51	143	21882	5.04	ng/ul	0.00
60) Fluorene-d10	15.32	176	352801	17.84	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.43	200	11332	3.14	ng/ul	0.00
73) Anthracene-d10	17.16	188	528777	16.81	ng/ul	0.00
81) Pyrene-d10	19.46	212	601442	16.71	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.34	264	586112	16.35	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.77	163	27402	1.180	ng/ul	100
86) Bis(2-ethylhexyl)phthalate	21.19	149	40557	1.565	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014420.D
Acq On : 25 Apr 2021 01:48
Operator : CG/JU
Sample : M2065-09
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG562

Quant Time: Apr 26 01:53:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 23 12:06:34 2021
Response via : Initial Calibration




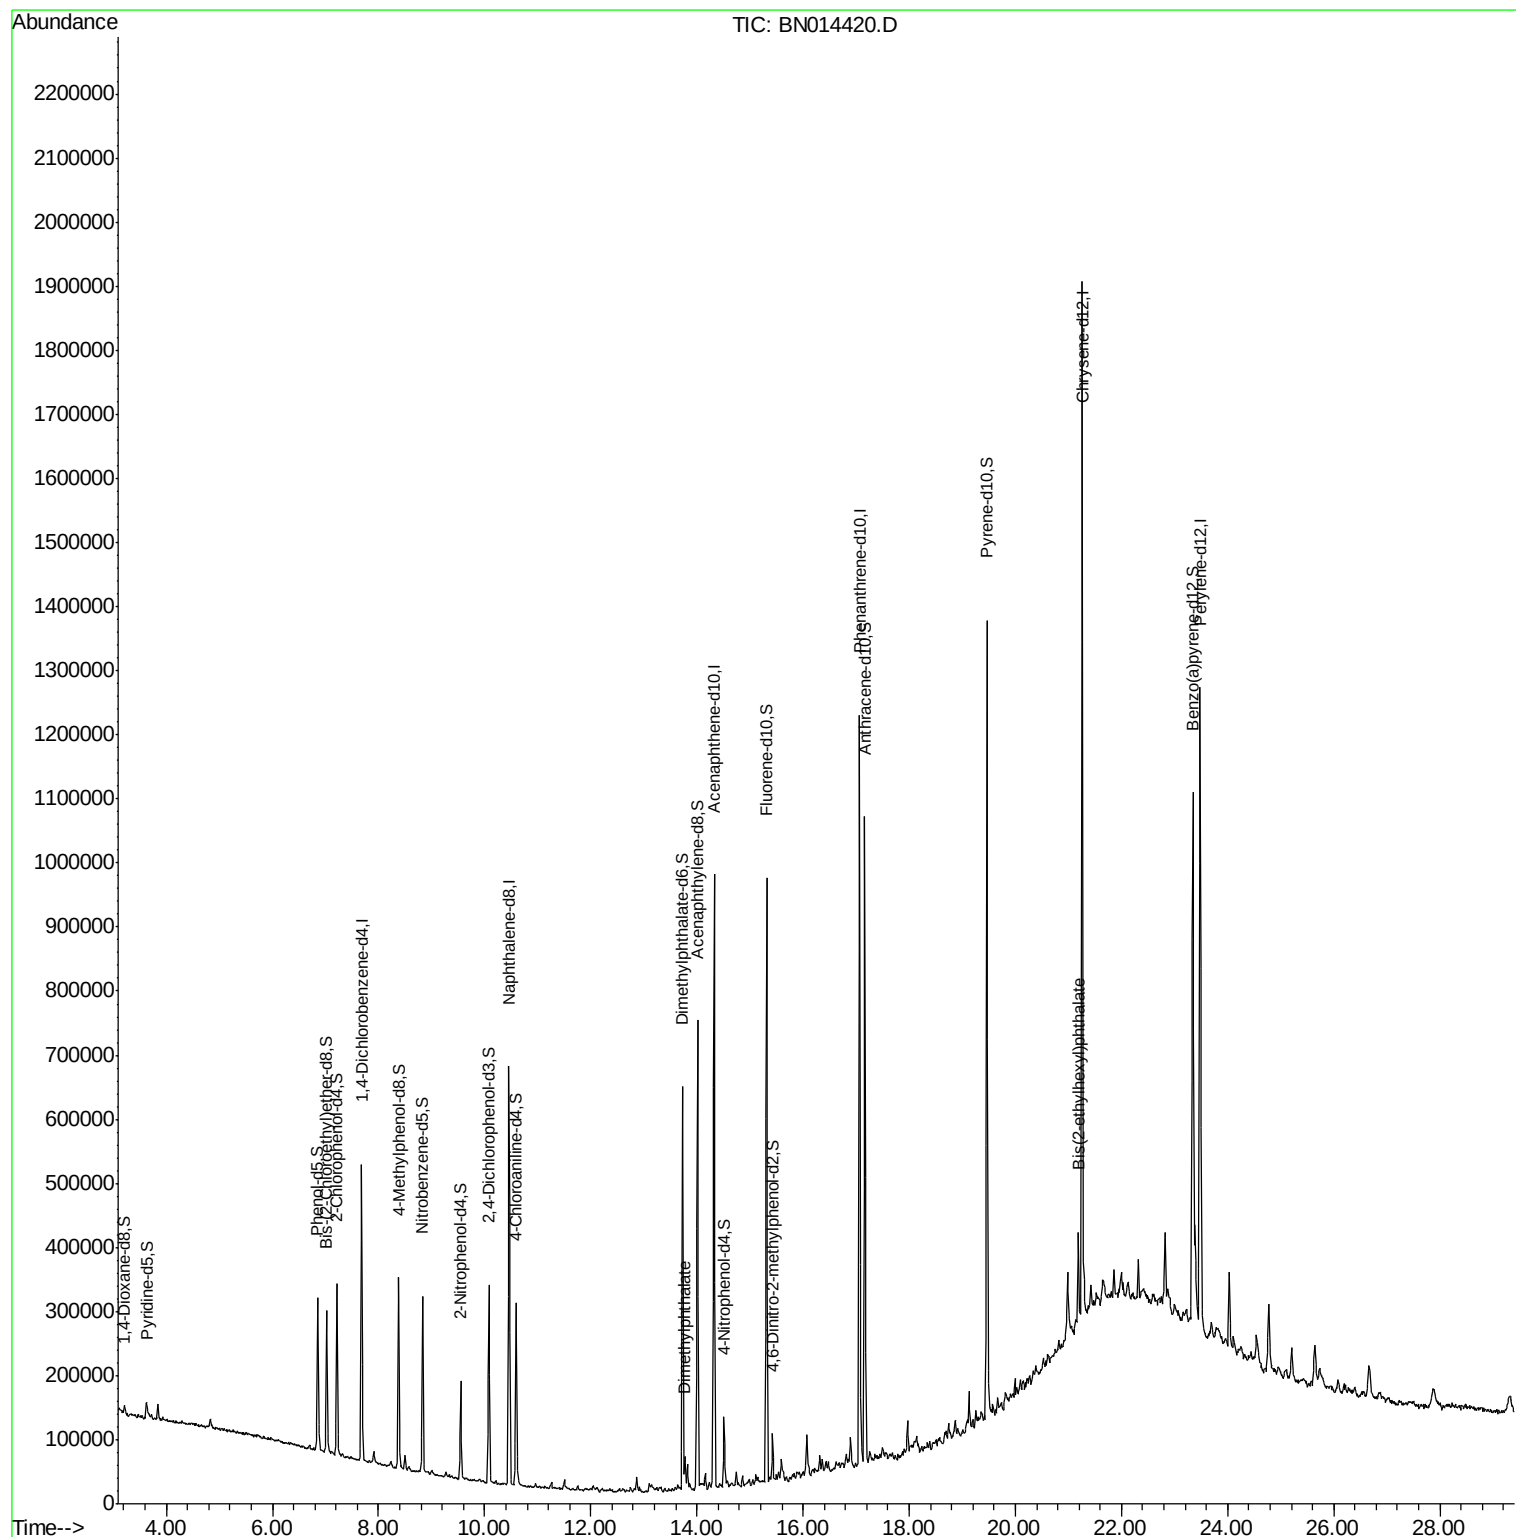


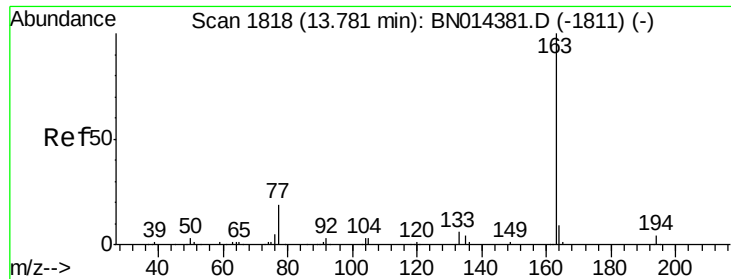

#47
 Dimethylphthalate
 Concen: 1.180 ng/ul
 RT: 13.77 min Scan# 1817
 Delta R.T. -0.01 min
 Lab File: BN014420.D
 Acq: 25 Apr 2021 01:48

Instrument :
 BNA_N
 ClientSampled :
 BG562

Tot Ion:163 Resp: 27402
 Ion Ratio Lower Upper
 163 100
 194 4.0 3.3 4.9
 164 9.9 7.8 11.8

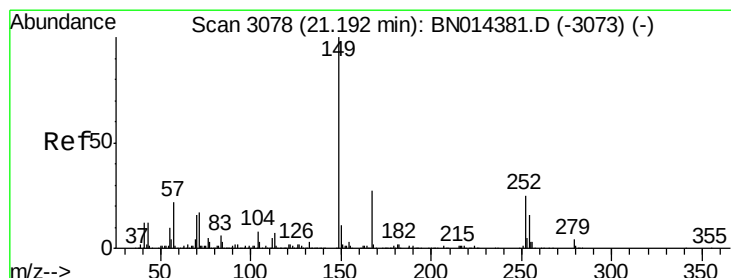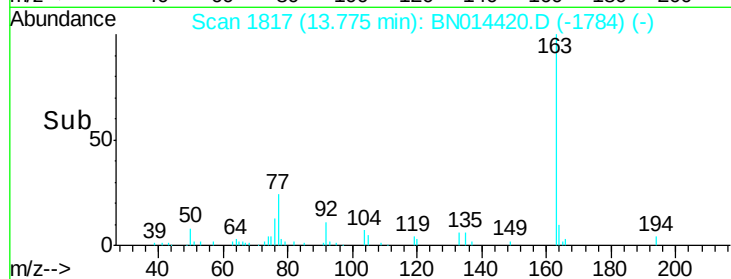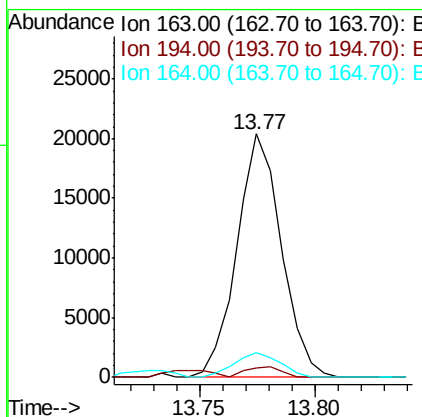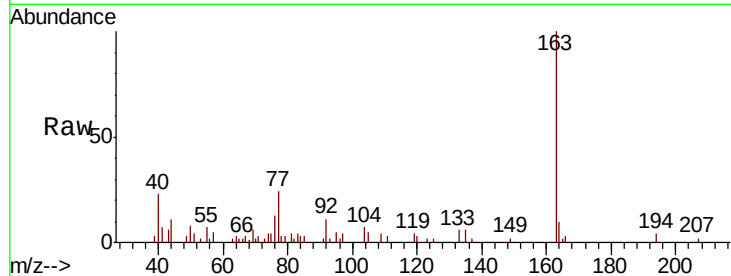

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.565 ng/ul
 RT: 21.19 min Scan# 3077
 Delta R.T. -0.01 min
 Lab File: BN014420.D
 Acq: 25 Apr 2021 01:48

Tgt Ion:149 Resp: 40557
 Ion Ratio Lower Upper
 149 100
 167 26.5 22.0 33.0
 279 3.5 3.0 4.6

