

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
 Data File : BN014425.D
 Acq On : 25 Apr 2021 04:46
 Operator : CG/JU
 Sample : M2065-13
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG566

Quant Time: Apr 26 01:53:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 23 12:06:34 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	127965	20.00	ng/ul	0.00
20) Naphthalene-d8	10.46	136	547021	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.32	164	320540	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.07	188	661589	20.00	ng/ul	0.00
79) Chrysene-d12	21.26	240	723693	20.00	ng/ul	0.00
88) Perylene-d12	23.49	264	707619	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	6071	1.81	ng/uL	0.00
4) Pyridine-d5	3.62	84	26809	3.01	ng/ul	0.01
7) Phenol-d5	6.85	99	128291	11.99	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.02	67	86012	13.43	ng/ul	0.00
11) 2-Chlorophenol-d4	7.22	132	114466	13.60	ng/ul	0.00
15) 4-Methylphenol-d8	8.38	113	106167	13.09	ng/ul	0.00
21) Nitrobenzene-d5	8.83	128	61935	15.67	ng/ul	0.00
24) 2-Nitrophenol-d4	9.55	143	47848	12.36	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.08	165	103806	12.45	ng/ul	0.00
31) 4-Chloroaniline-d4	10.59	131	143060	11.56	ng/ul	0.00
46) Dimethylphthalate-d6	13.73	166	357283	15.39	ng/ul	0.00
49) Acenaphthylene-d8	14.01	160	455511	16.31	ng/ul	0.00
54) 4-Nitrophenol-d4	14.51	143	26091	5.79	ng/ul	0.00
60) Fluorene-d10	15.32	176	305907	14.90	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.43	200	12203	3.45	ng/ul	0.00
73) Anthracene-d10	17.16	188	493272	15.97	ng/ul	0.00
81) Pyrene-d10	19.46	212	566894	16.14	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.34	264	586814	15.63	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.77	163	61909	2.568	ng/ul	Ovalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014425.D
Acq On : 25 Apr 2021 04:46
Operator : CG/JU
Sample : M2065-13
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG566

Quant Time: Apr 26 01:53:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 23 12:06:34 2021
Response via : Initial Calibration

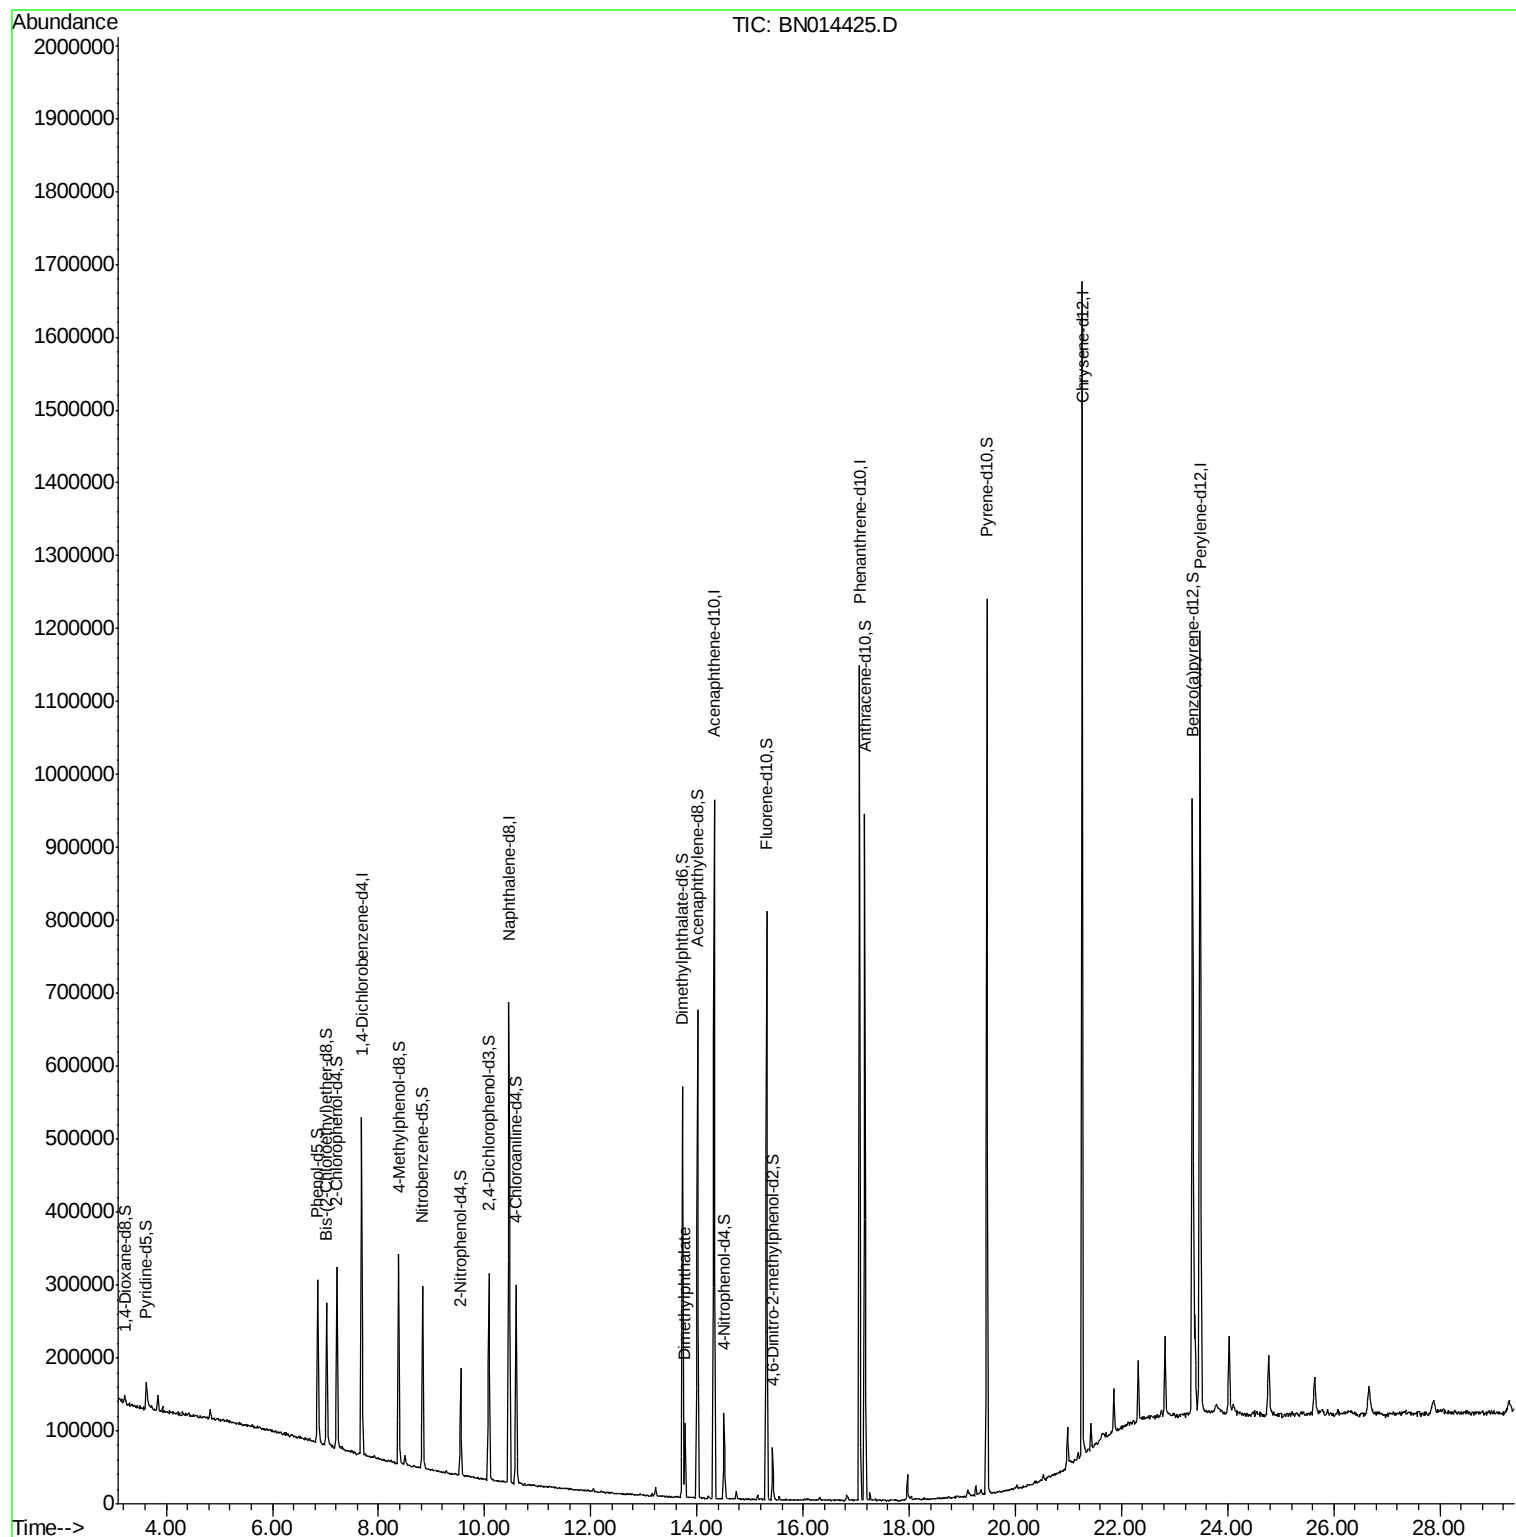

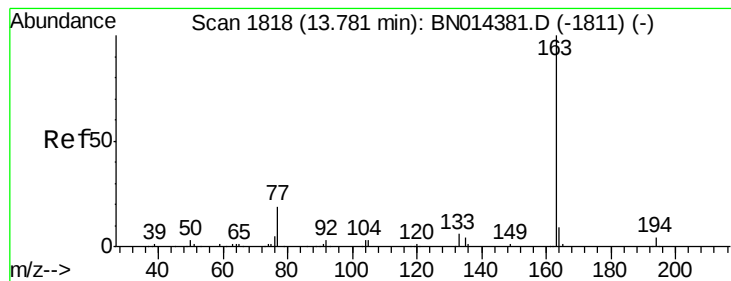

#47

Dimethylphthalate

Concen: 2.568 ng/ul

RT: 13.77 min Scan# 1817

Delta R.T. -0.01 min

Lab File: BN014425.D

Acq: 25 Apr 2021 04:46

Instrument :

BNA_N

ClientSampleId :

BG566


Tot Ion:163 Resp: 61909

Ion Ratio Lower Upper

163 100

194 4.1 3.3 4.9

164 10.4 7.8 11.8

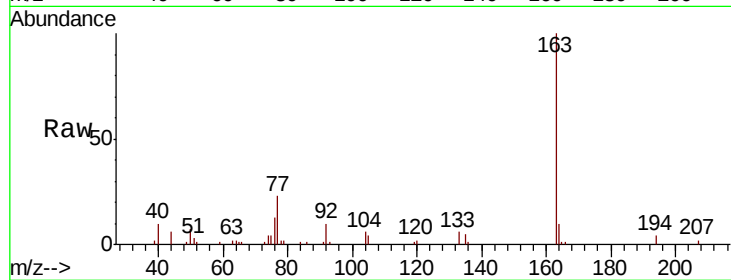

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

