

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
 Data File : BN014427.D
 Acq On : 25 Apr 2021 06:33
 Operator : CG/JU
 Sample : M2065-16
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG569

Quant Time: Apr 26 01:54:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 23 12:06:34 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	127505	20.00	ng/ul	0.00
20) Naphthalene-d8	10.46	136	550658	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.32	164	310989	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.06	188	664413	20.00	ng/ul	0.00
79) Chrysene-d12	21.26	240	715671	20.00	ng/ul	0.00
88) Perylene-d12	23.48	264	697339	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.21	96	9755	2.91	ng/uL	0.00
4) Pyridine-d5	3.61	84	100748	11.35	ng/ul	0.00
7) Phenol-d5	6.85	99	218237	20.47	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.02	67	139498	21.85	ng/ul	0.00
11) 2-Chlorophenol-d4	7.22	132	188818	22.52	ng/ul	0.00
15) 4-Methylphenol-d8	8.38	113	181417	22.45	ng/ul	0.00
21) Nitrobenzene-d5	8.83	128	103939	26.12	ng/ul	0.00
24) 2-Nitrophenol-d4	9.55	143	81879	21.01	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.08	165	178783	21.30	ng/ul	0.00
31) 4-Chloroaniline-d4	10.59	131	243577	19.56	ng/ul	0.00
46) Dimethylphthalate-d6	13.73	166	564913	25.07	ng/ul	0.00
49) Acenaphthylene-d8	14.01	160	794186	29.30	ng/ul	0.00
54) 4-Nitrophenol-d4	14.51	143	59742	13.67	ng/ul	0.00
60) Fluorene-d10	15.31	176	519279	26.07	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.43	200	28134	7.91	ng/ul	0.00
73) Anthracene-d10	17.16	188	826671	26.66	ng/ul	0.00
81) Pyrene-d10	19.46	212	985723	28.37	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.34	264	1030580	27.86	ng/ul	0.00

Target Compounds


					Ovalue
8) Phenol	6.88	94	19094	1.666 ng/ul	95
47) Dimethylphthalate	13.77	163	40023	1.711 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014427.D
Acq On : 25 Apr 2021 06:33
Operator : CG/JU
Sample : M2065-16
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG569

Quant Time: Apr 26 01:54:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 23 12:06:34 2021
Response via : Initial Calibration

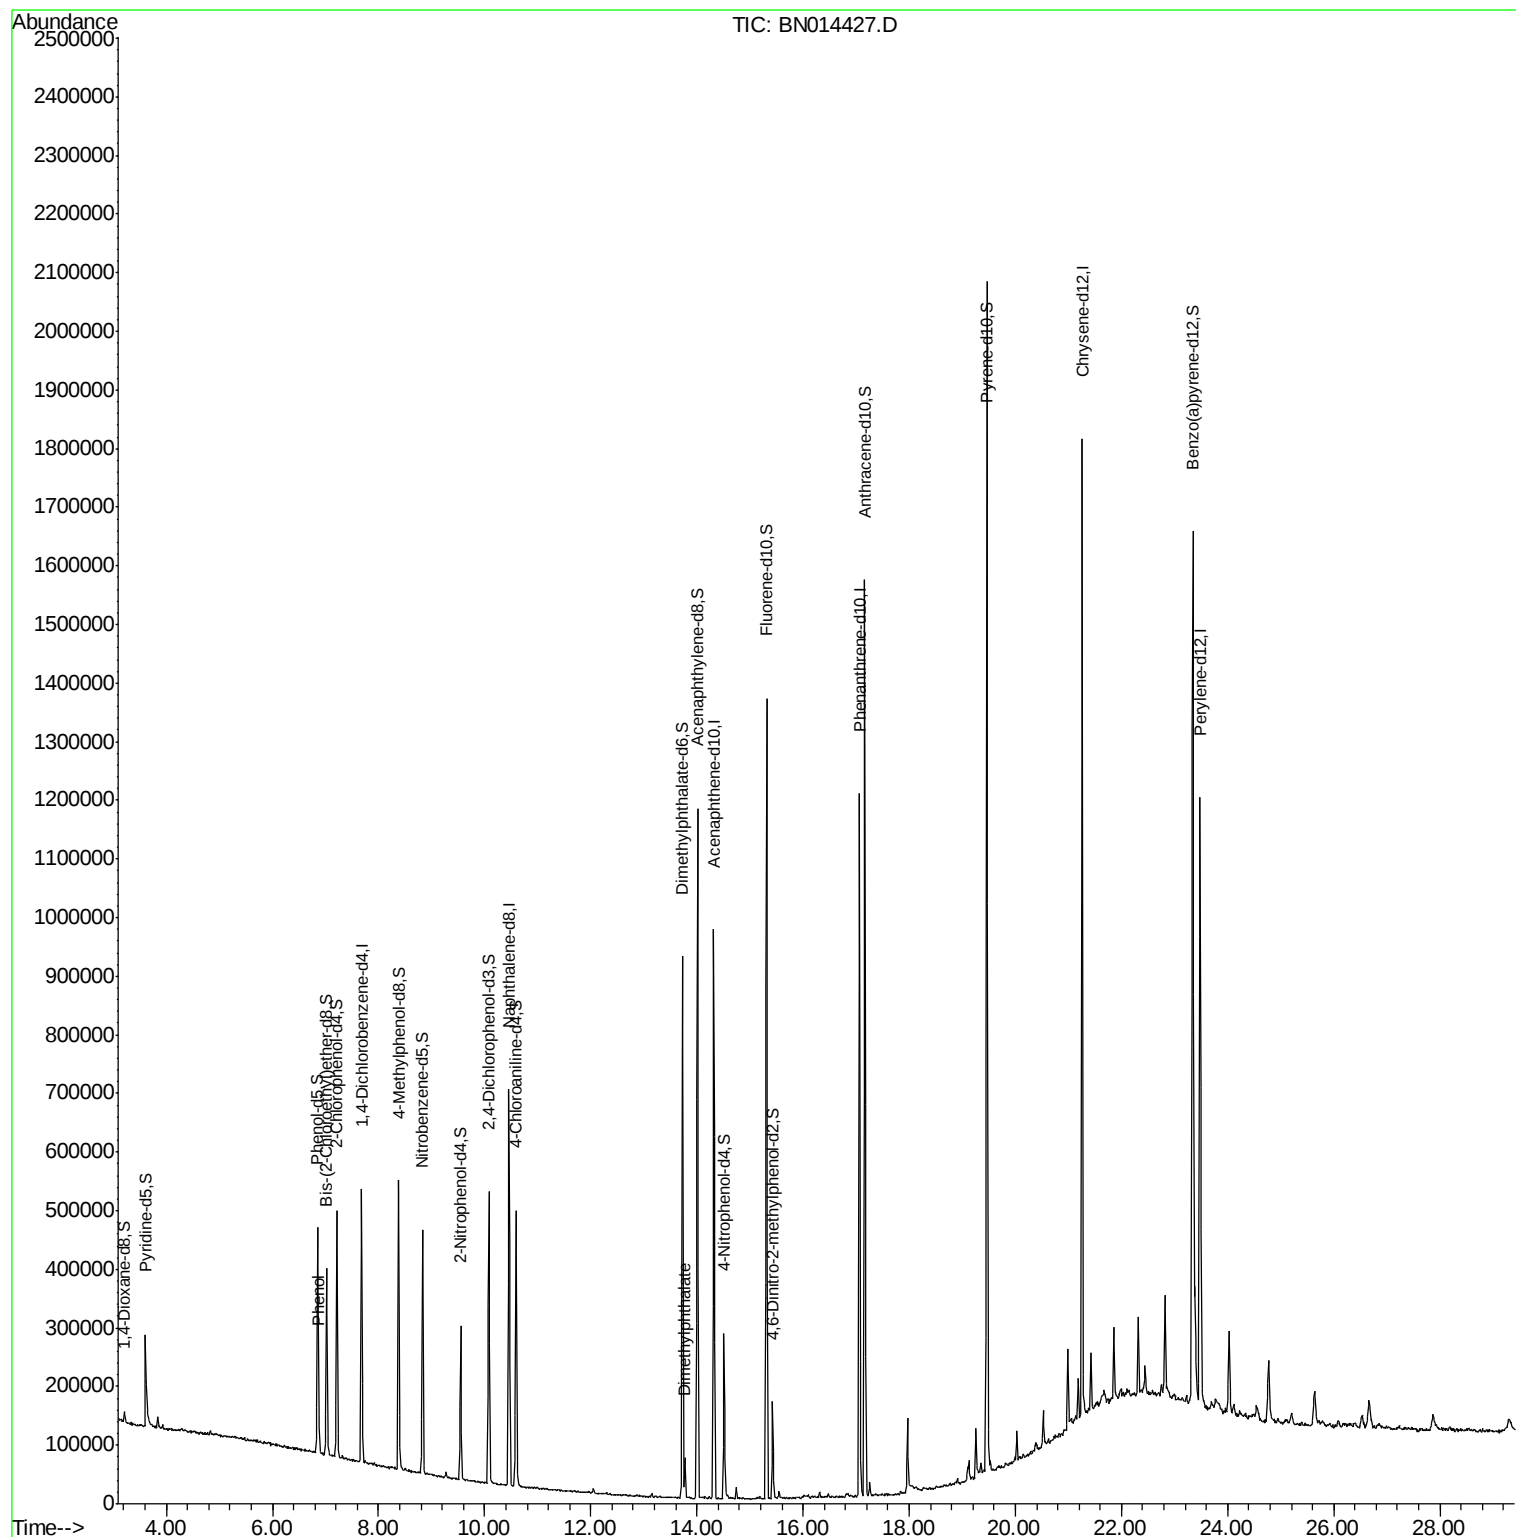

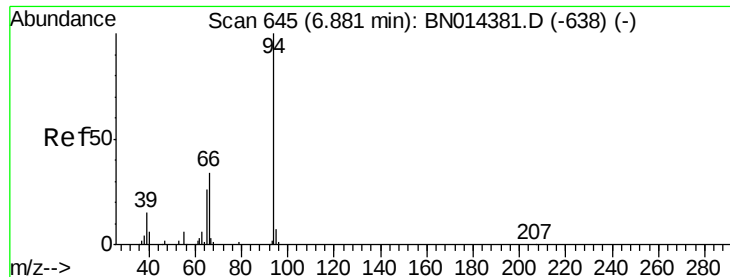





#8

Phenol

Concen: 1.666 ng/ul
 RT: 6.88 min Scan# 644
 Delta R.T. -0.01 min
 Lab File: BN014427.D
 Acq: 25 Apr 2021 06:33

Instrument :
 BNA_N
 ClientSampleId :
 BG569

Tot Ion: 94 Resp: 19094
 Ion Ratio Lower Upper
 94 100
 65 28.0 22.5 33.7
 66 41.2 29.0 43.6

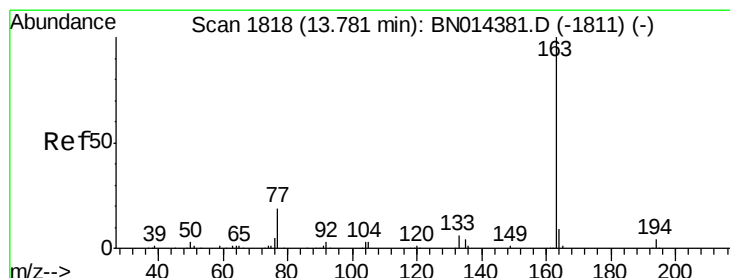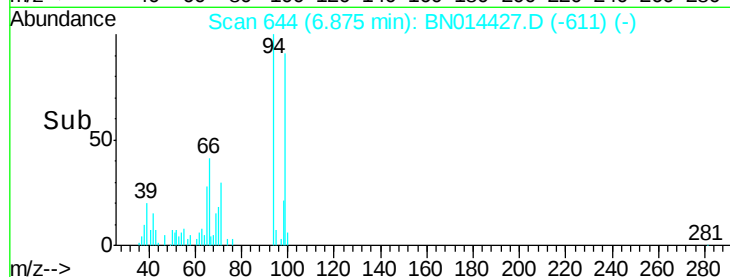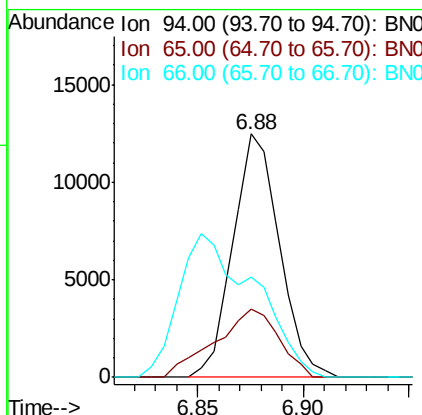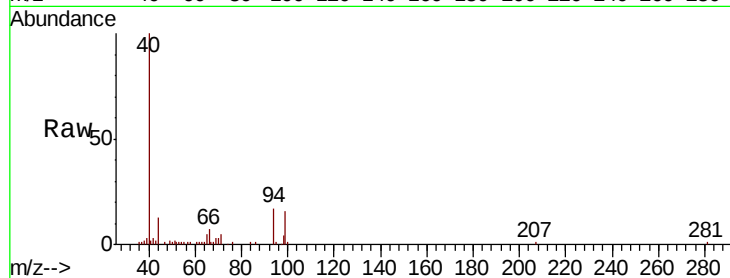

#47

Dimethylphthalate

Concen: 1.711 ng/ul
 RT: 13.77 min Scan# 1817
 Delta R.T. -0.01 min
 Lab File: BN014427.D
 Acq: 25 Apr 2021 06:33

Tgt Ion: 163 Resp: 40023
 Ion Ratio Lower Upper
 163 100
 194 3.9 3.3 4.9
 164 10.2 7.8 11.8

