

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_N\DATA\BN042421\  
 Data File : BN014398.D  
 Acq On : 24 Apr 2021 12:09  
 Operator : CG/JU  
 Sample : M2065-19  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 BG572

Quant Time: Apr 26 01:48:53 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SFAM-EPA-BN041521.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Fri Apr 23 12:06:34 2021  
 Response via : Initial Calibration


| Internal Standards             | R.T.  | QIon | Response | Conc  | Units | Dev(Min)      |
|--------------------------------|-------|------|----------|-------|-------|---------------|
| 1) 1,4-Dichlorobenzene-d4      | 7.68  | 152  | 138591   | 20.00 | ng/ul | 0.00          |
| 20) Naphthalene-d8             | 10.46 | 136  | 580141   | 20.00 | ng/ul | 0.00          |
| 38) Acenaphthene-d10           | 14.32 | 164  | 338075   | 20.00 | ng/ul | 0.00          |
| 64) Phenanthrene-d10           | 17.06 | 188  | 685674   | 20.00 | ng/ul | 0.00          |
| 79) Chrysene-d12               | 21.26 | 240  | 667615   | 20.00 | ng/ul | 0.00          |
| 88) Perylene-d12               | 23.49 | 264  | 675209   | 20.00 | ng/ul | 0.00          |
| System Monitoring Compounds    |       |      |          |       |       |               |
| 3) 1,4-Dioxane-d8              | 3.21  | 96   | 7910     | 2.17  | ng/uL | 0.00          |
| 4) Pyridine-d5                 | 3.62  | 84   | 37458    | 3.88  | ng/ul | 0.01          |
| 7) Phenol-d5                   | 6.85  | 99   | 171689   | 14.82 | ng/ul | 0.00          |
| 9) Bis-(2-Chloroethyl)ether-d  | 7.02  | 67   | 116555   | 16.80 | ng/ul | 0.00          |
| 11) 2-Chlorophenol-d4          | 7.22  | 132  | 151760   | 16.65 | ng/ul | 0.00          |
| 15) 4-Methylphenol-d8          | 8.38  | 113  | 139706   | 15.91 | ng/ul | 0.00          |
| 21) Nitrobenzene-d5            | 8.83  | 128  | 79030    | 18.85 | ng/ul | 0.00          |
| 24) 2-Nitrophenol-d4           | 9.55  | 143  | 65188    | 15.88 | ng/ul | 0.00          |
| 28) 2,4-Dichlorophenol-d3      | 10.08 | 165  | 130598   | 14.77 | ng/ul | 0.00          |
| 31) 4-Chloroaniline-d4         | 10.59 | 131  | 185162   | 14.11 | ng/ul | 0.00          |
| 46) Dimethylphthalate-d6       | 13.73 | 166  | 436141   | 17.81 | ng/ul | 0.00          |
| 49) Acenaphthylene-d8          | 14.01 | 160  | 566119   | 19.21 | ng/ul | 0.00          |
| 54) 4-Nitrophenol-d4           | 14.52 | 143  | 35421    | 7.46  | ng/ul | 0.00          |
| 60) Fluorene-d10               | 15.32 | 176  | 380631   | 17.58 | ng/ul | 0.00          |
| 65) 4,6-Dinitro-2-methylphenol | 15.43 | 200  | 20431    | 5.57  | ng/ul | 0.00          |
| 73) Anthracene-d10             | 17.16 | 188  | 558792   | 17.46 | ng/ul | 0.00          |
| 81) Pyrene-d10                 | 19.46 | 212  | 624968   | 19.28 | ng/ul | 0.00          |
| 92) Benzo(a)pyrene-d12         | 23.35 | 264  | 624826   | 17.44 | ng/ul | 0.00          |
| Target Compounds               |       |      |          |       |       |               |
| 47) Dimethylphthalate          | 13.77 | 163  | 54366    | 2.138 | ng/ul | Ovalue<br>100 |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_N\DATA\BN042421\  
Data File : BN014398.D  
Acq On : 24 Apr 2021 12:09  
Operator : CG/JU  
Sample : M2065-19  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
BG572

Quant Time: Apr 26 01:48:53 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SFAM-EPA-BN041521.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Fri Apr 23 12:06:34 2021  
Response via : Initial Calibration

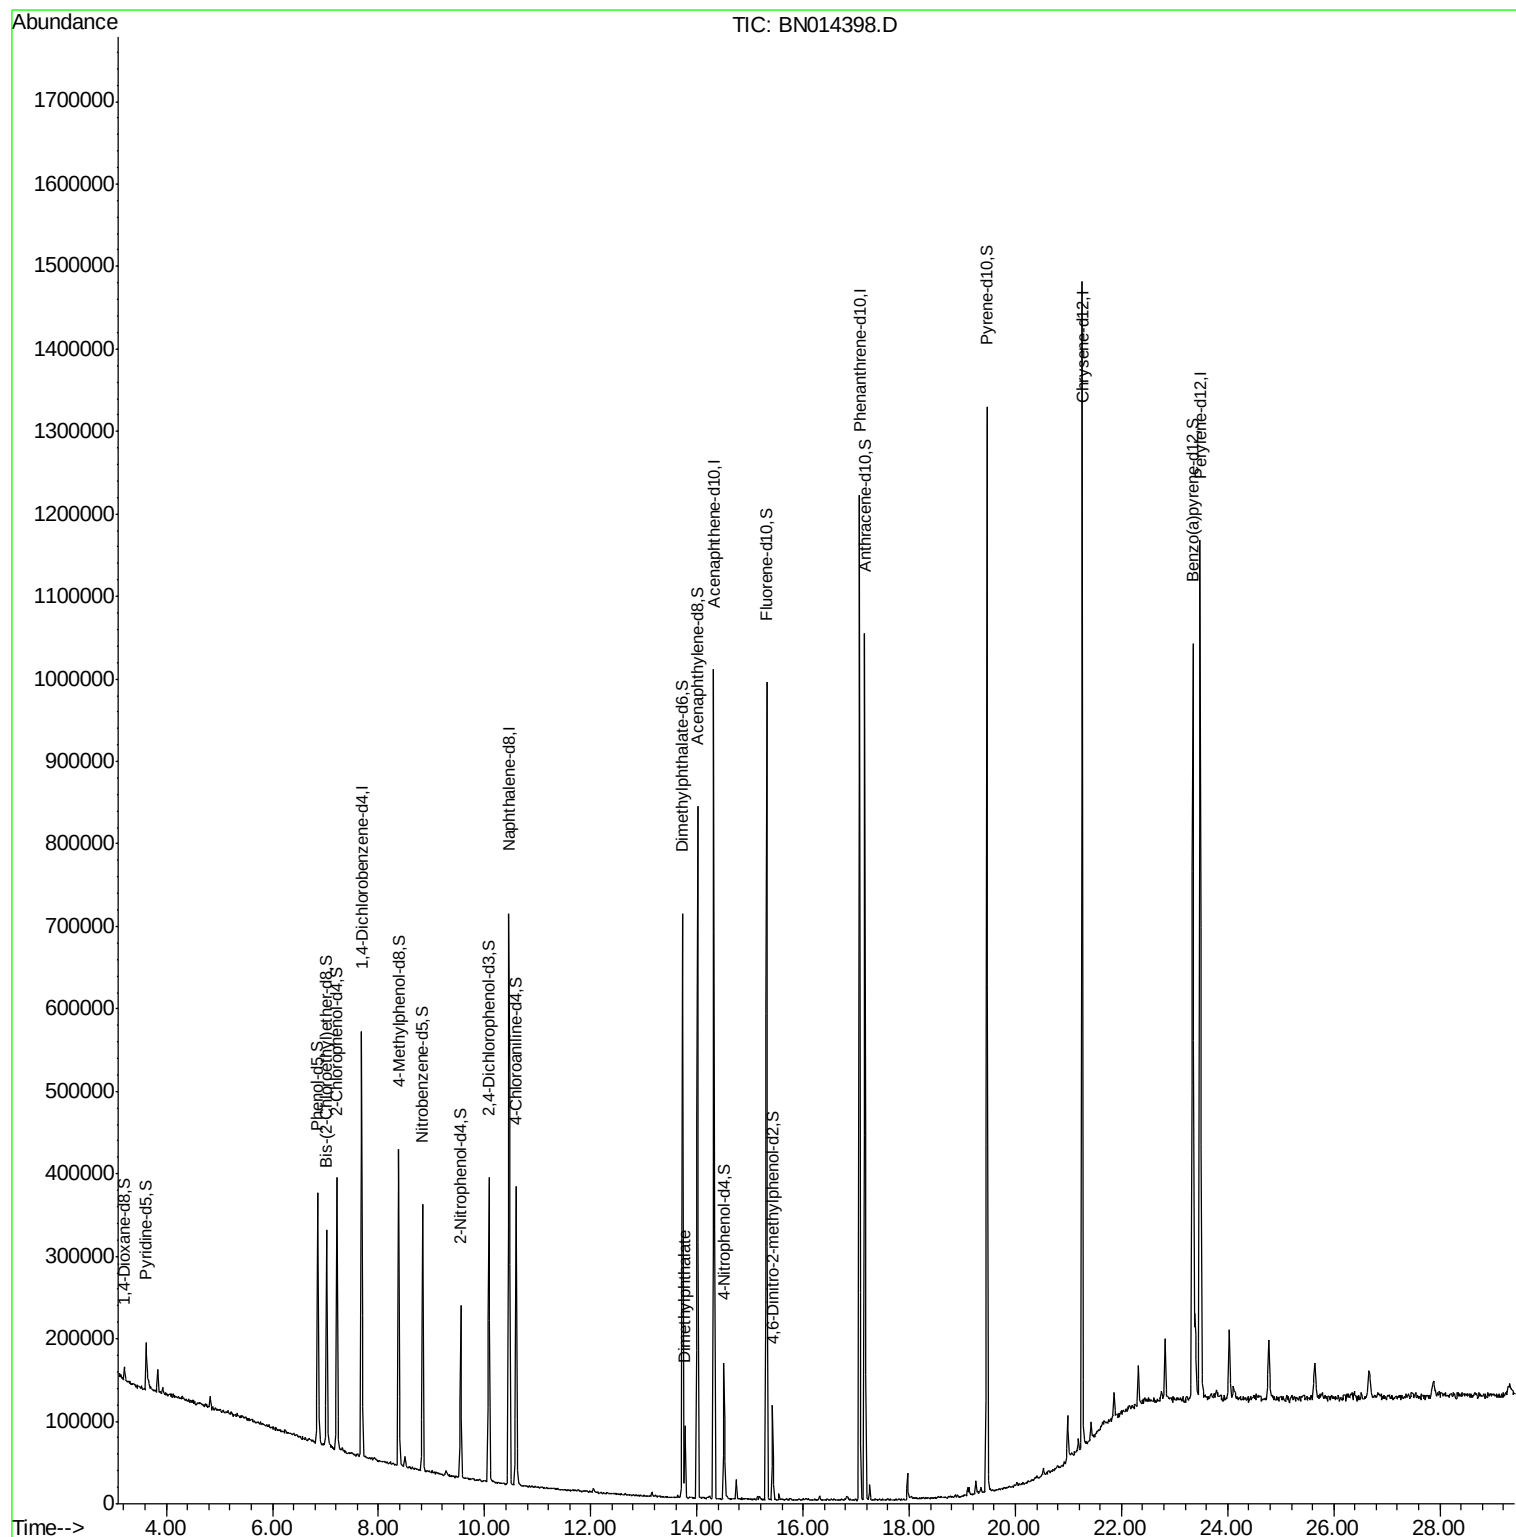


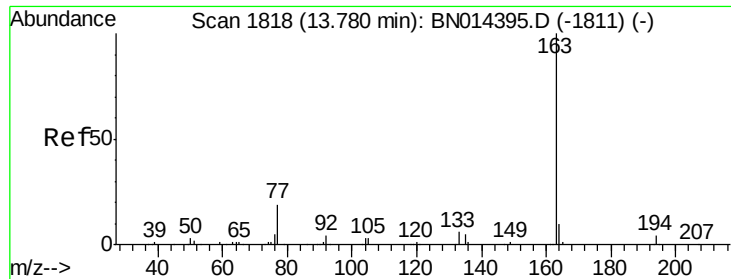

#47  
 Dimethylphthalate  
 Concen: 2.138 ng/ul  
 RT: 13.77 min Scan# 1817  
 Delta R.T. -0.01 min  
 Lab File: BN014398.D  
 Acq: 24 Apr 2021 12:09

Instrument :  
 BNA\_N  
 ClientSampleId :  
 BG572

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 163     | 100   |       |       |
| 194     | 3.9   | 3.3   | 4.9   |
| 164     | 10.0  | 7.8   | 11.8  |

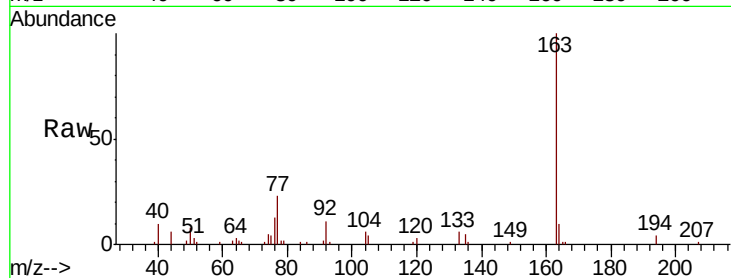

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

