

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
 Data File : BN014417.D
 Acq On : 25 Apr 2021 00:00
 Operator : CG/JU
 Sample : M2065-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG4Z8

Manual Integrations
 APPROVED

mohammad
 4/26/2021 11:42:58 AM

Quant Time: Apr 26 03:34:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 23 12:06:34 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	119096	20.00	ng/ul	0.00
20) Naphthalene-d8	10.46	136	492613	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.32	164	273399	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.06	188	605974	20.00	ng/ul	0.00
79) Chrysene-d12	21.26	240	663950	20.00	ng/ul	0.00
88) Perylene-d12	23.49	264	622774	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	5585	1.78	ng/uL	0.00
4) Pyridine-d5	3.63	84	22497m	2.71	ng/ul	0.02
7) Phenol-d5	6.85	99	113682	11.42	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.02	67	81502	13.67	ng/ul	0.00
11) 2-Chlorophenol-d4	7.22	132	97269	12.42	ng/ul	0.00
15) 4-Methylphenol-d8	8.38	113	88574	11.74	ng/ul	0.00
21) Nitrobenzene-d5	8.83	128	54019	15.17	ng/ul	0.00
24) 2-Nitrophenol-d4	9.55	143	34979	10.03	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.08	165	80907	10.77	ng/ul	0.00
31) 4-Chloroaniline-d4	10.59	131	89630	8.05	ng/ul	0.00
46) Dimethylphthalate-d6	13.73	166	274691	13.87	ng/ul	0.00
49) Acenaphthylene-d8	14.01	160	379506	15.93	ng/ul	0.00
54) 4-Nitrophenol-d4	14.51	143	13377	3.48	ng/ul	0.00
60) Fluorene-d10	15.32	176	267749	15.29	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.43	200	7981	2.46	ng/ul	0.00
73) Anthracene-d10	17.16	188	405541	14.34	ng/ul	0.00
81) Pyrene-d10	19.46	212	470764	14.61	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.34	264	487180	14.75	ng/ul	0.00
Target Compounds						
72) Phenanthrene	17.11	178	66566	1.881	ng/ul	99
80) Fluoranthene	19.13	202	313312	7.693	ng/ul	99
82) Pyrene	19.49	202	246740	5.690	ng/ul	99
85) Benzo(a)anthracene	21.24	228	85429	1.991	ng/ul	95
87) Chrysene	21.30	228	132241	3.180	ng/ul	96
90) Benzo(b)fluoranthene	22.82	252	131754	3.162	ng/ul#	89
93) Benzo(a)pyrene	23.39	252	55288	1.500	ng/ul#	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014417.D
Acq On : 25 Apr 2021 00:00
Operator : CG/JU
Sample : M2065-01
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BG4Z8

Quant Time: Apr 26 03:34:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 23 12:06:34 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
4/26/2021 11:42:58 AM

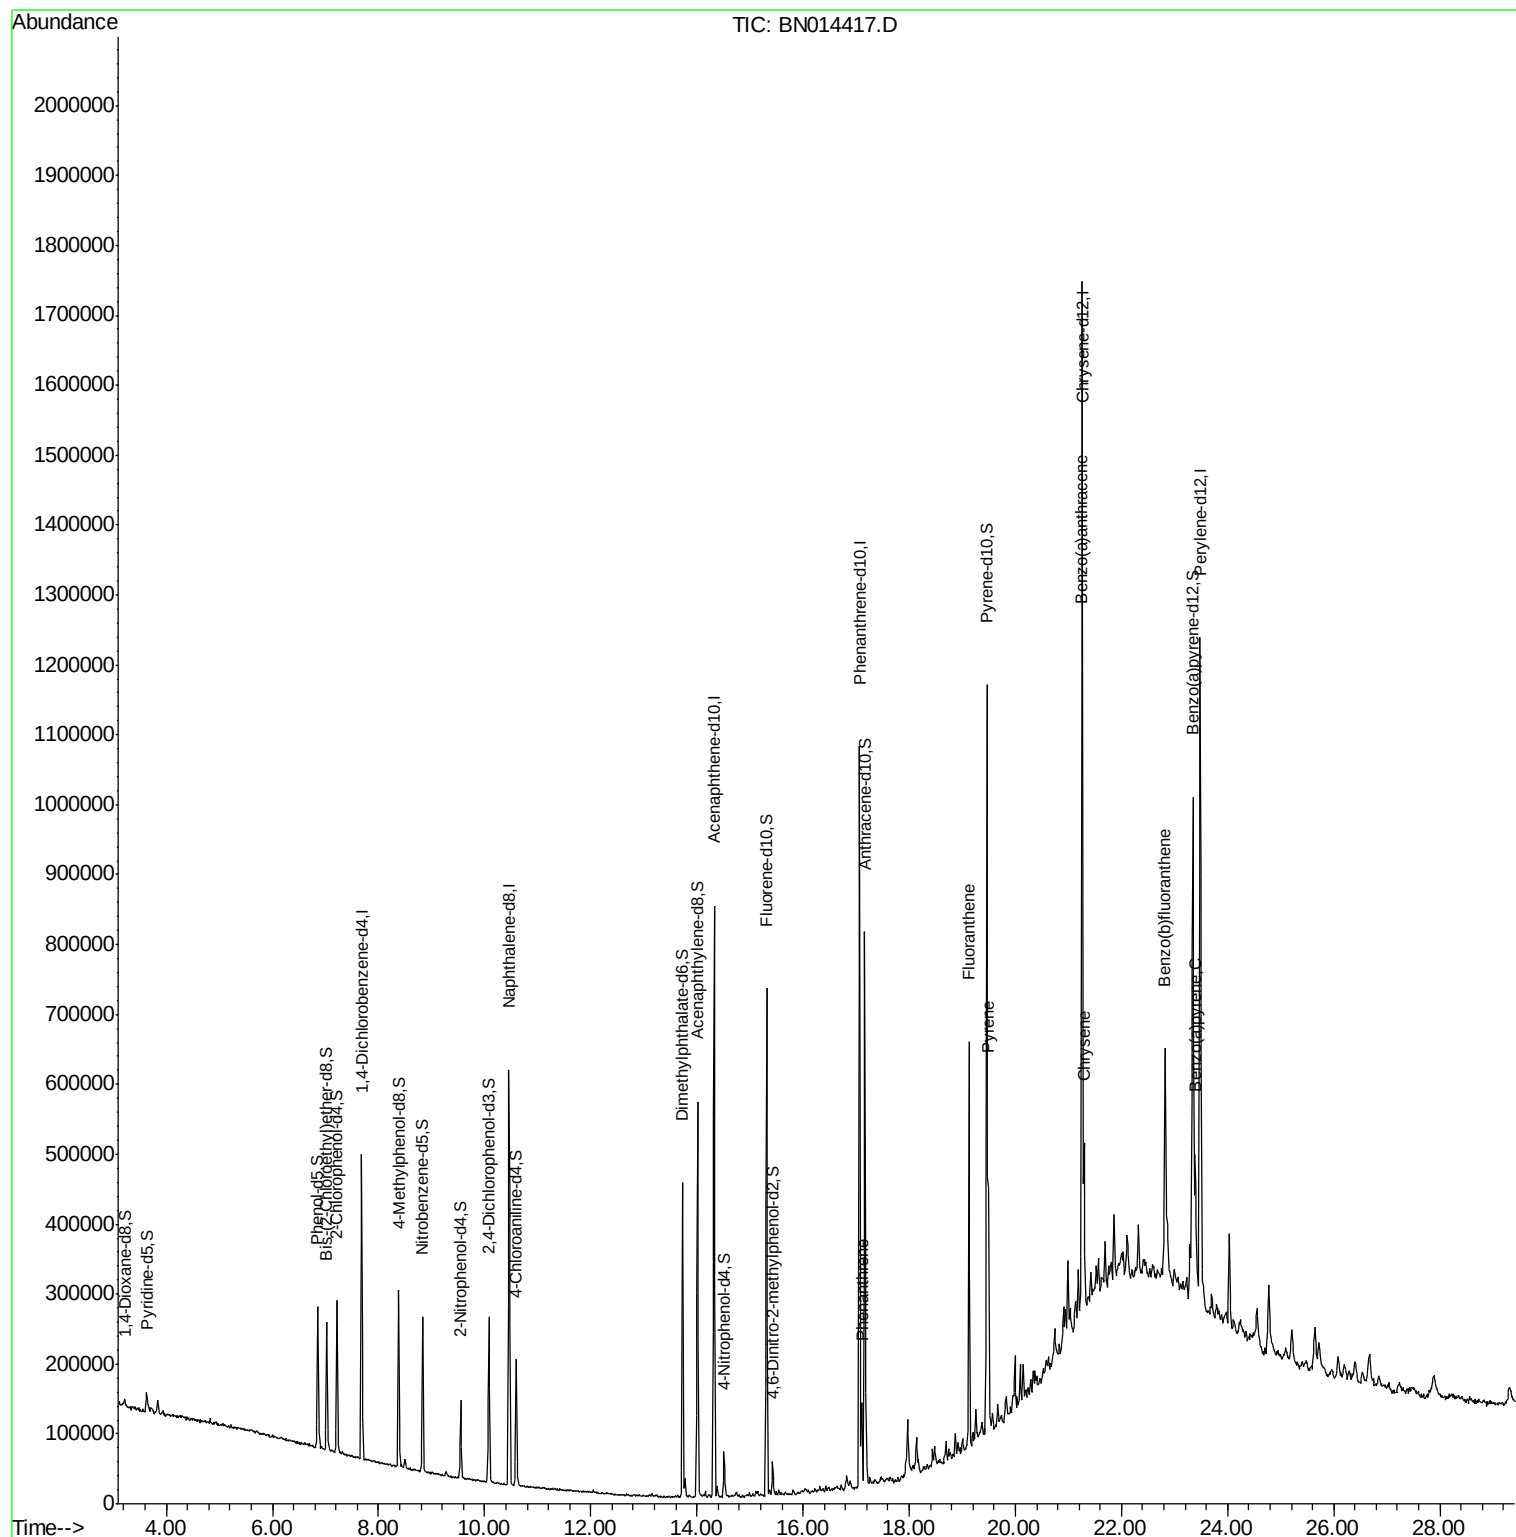

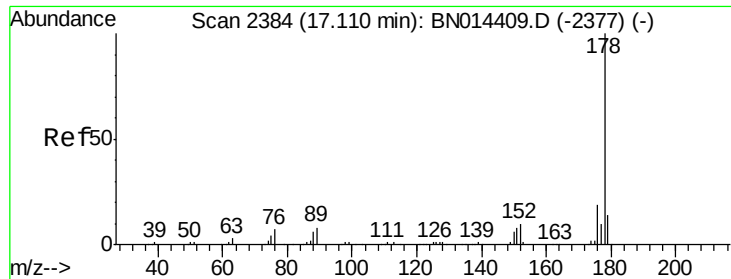

#72

Phenanthrene

Concen: 1.881 ng/ul

RT: 17.11 min Scan# 2384

Delta R.T. 0.00 min

Lab File: BN014417.D

Acq: 25 Apr 2021 00:00

Instrument :

BNA_N


ClientSampleId :

BG4Z8




Tot Ion:	178	Resp:	66566
Ion	Ratio	Lower	Upper
178	100		
179	14.8	12.2	18.4
176	18.9	15.0	22.4

Manual Integrations
APPROVED

mohammad
4/26/2021 11:42:58 AM

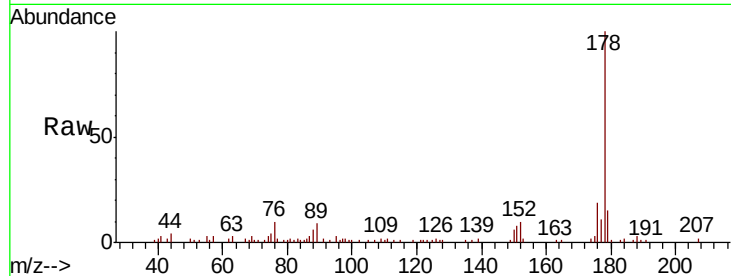

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

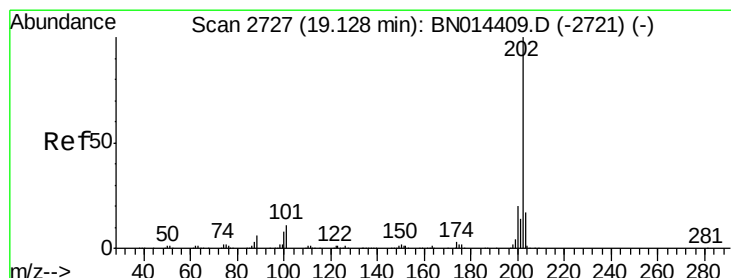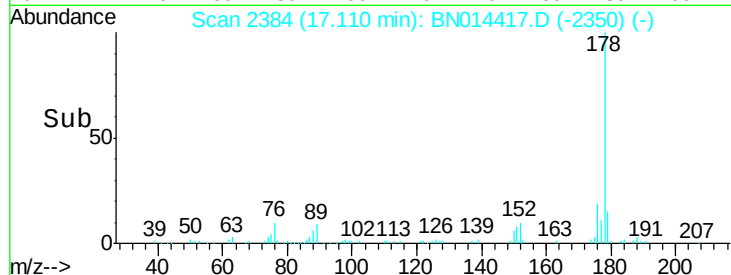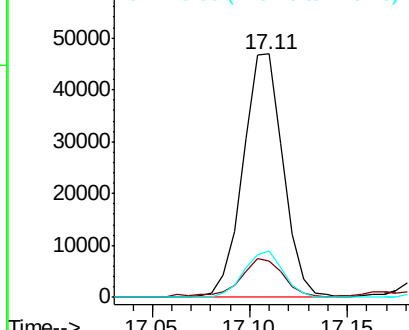

#80

Fluoranthene

Concen: 7.693 ng/ul


RT: 19.13 min Scan# 2727

Delta R.T. 0.00 min



Lab File: BN014417.D


Acq: 25 Apr 2021 00:00

Tgt Ion:	202	Resp:	313312
Ion	Ratio	Lower	Upper
202	100		
101	12.0	9.0	13.6
100	9.0	7.0	10.4

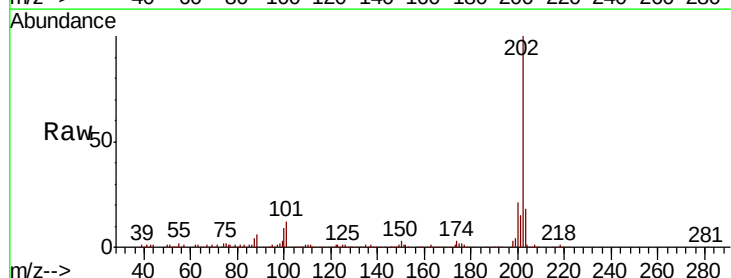

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

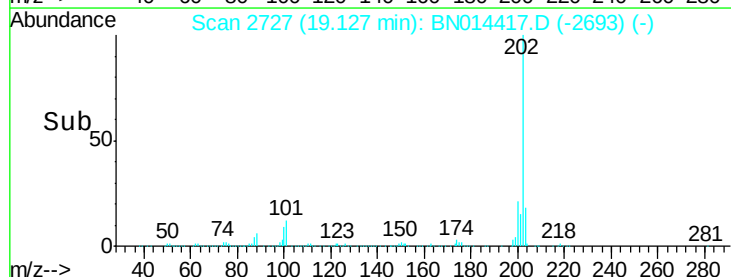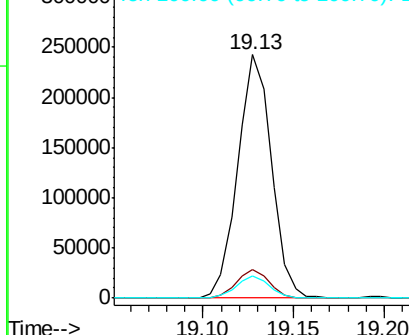

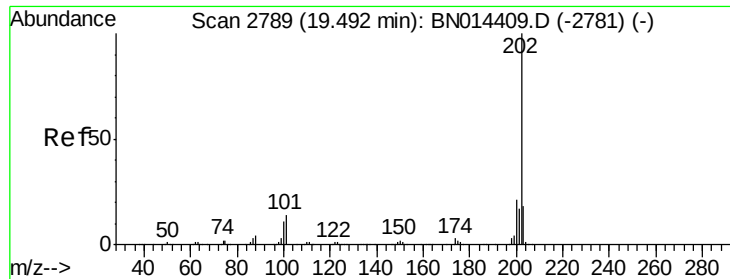





#82
Pvrene
Concen: 5.690 ng/ul
RT: 19.49 min Scan# 2789
Delta R.T. -0.01 min
Lab File: BN014417.D
Acq: 25 Apr 2021 00:00

Instrument :
BNA_N
ClientSampled :
BG4Z8

Tot Ion	Ratio	Lower	Upper
202	100		
101	13.8	10.5	15.7
100	11.0	8.7	13.1




Manual Integrations
APPROVED


mohammad
4/26/2021 11:42:58 AM

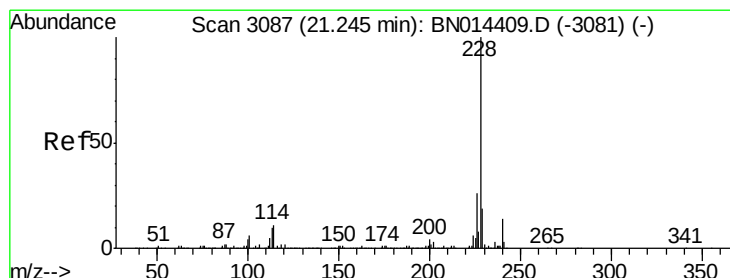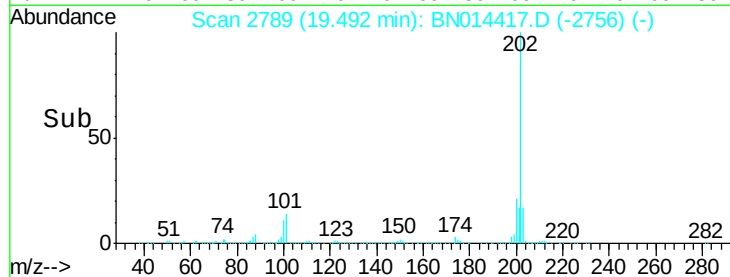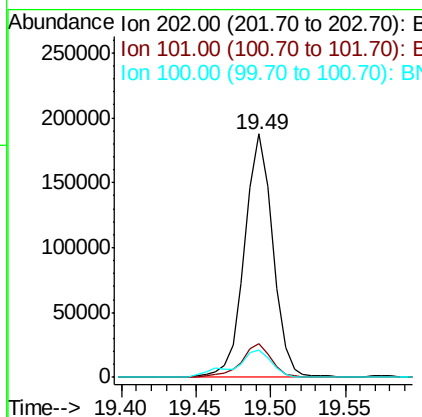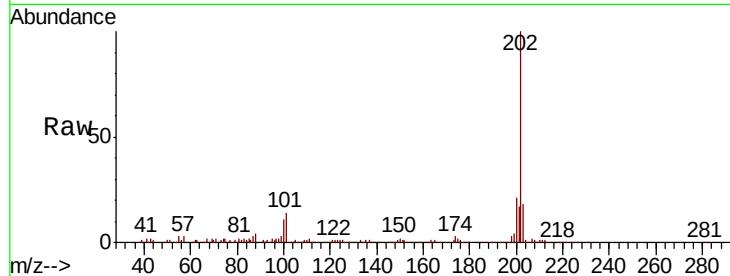

#85
Benzo(a)anthracene
Concen: 1.991 ng/ul
RT: 21.24 min Scan# 3087
Delta R.T. 0.00 min
Lab File: BN014417.D
Acq: 25 Apr 2021 00:00

Tgt Ion	Ratio	Lower	Upper
228	100		
229	21.5	15.4	23.2
226	30.0	21.8	32.8

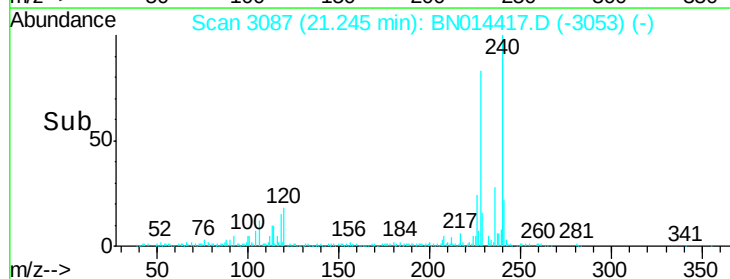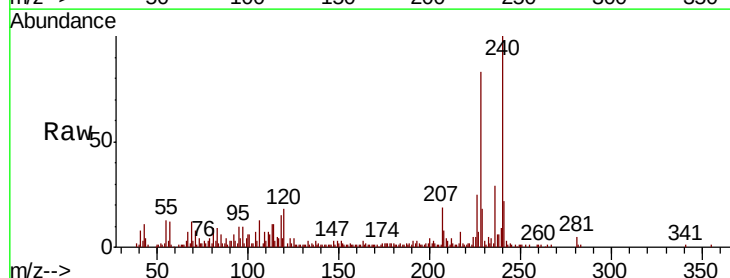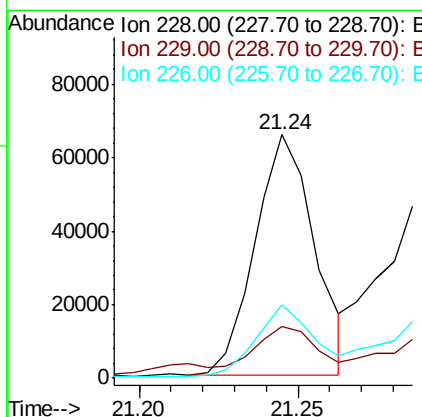

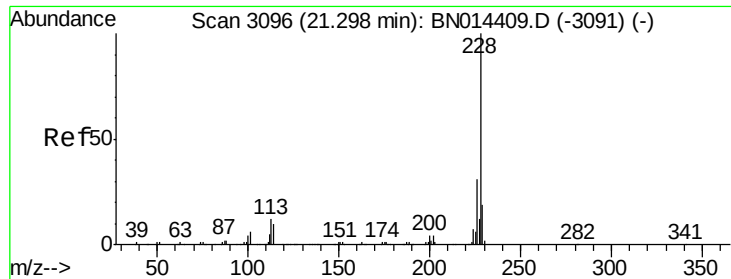

#87

Chrysene

Concen: 3.180 ng/ul

RT: 21.30 min Scan# 3096

Delta R.T. 0.00 min

Lab File: BN014417.D

Acq: 25 Apr 2021 00:00

Instrument :

BNA_N





ClientSampled :

BG4Z8

Tot Ion:	228	Resp:	132241
Ion Ratio	Lower	Upper	
228	100		
226	29.9	26.0	39.0
229	21.6	16.4	24.6

Manual Integrations
APPROVED

mohammad
4/26/2021 11:42:58 AM

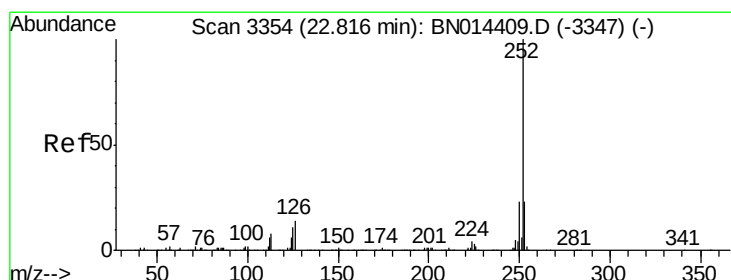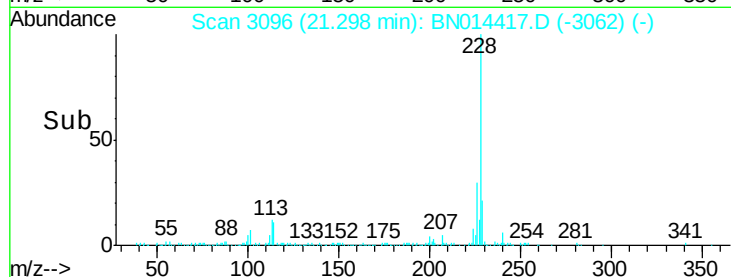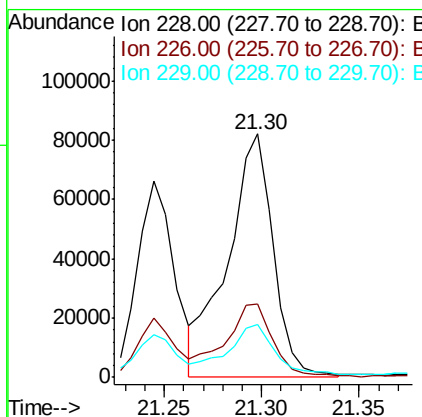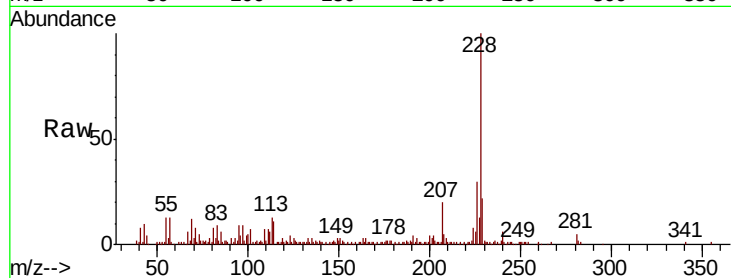

#90

Benzo(b)fluoranthene

Concen: 3.162 ng/ul




RT: 22.82 min Scan# 3355


Delta R.T. 0.00 min

Lab File: BN014417.D

Acq: 25 Apr 2021 00:00

Tgt Ion:	252	Resp:	131754
Ion Ratio	Lower	Upper	
252	100		
253	25.2	17.3	25.9
125	17.4	8.1	12.1#

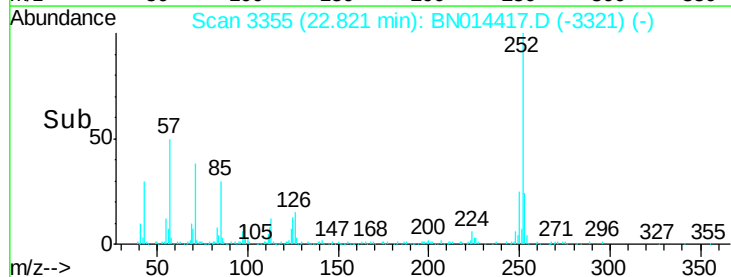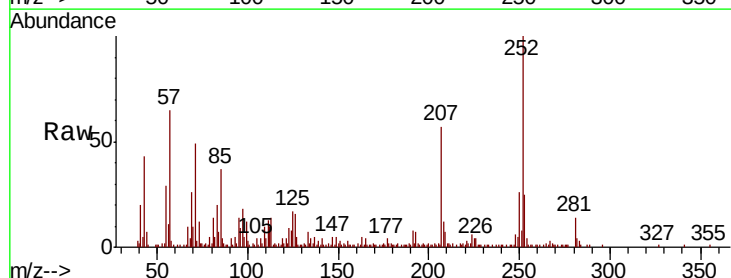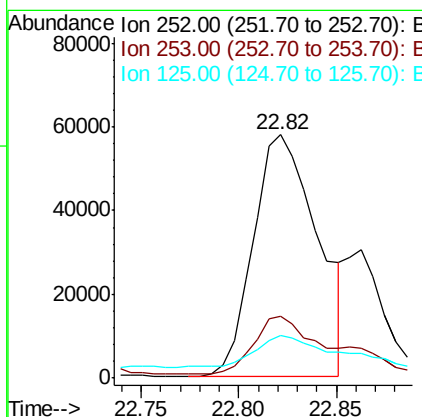

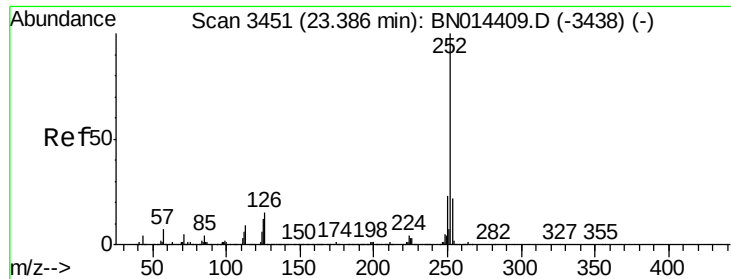

#93

Benzo(a)pyrene

Concen: 1.500 ng/ul

RT: 23.39 min Scan# 3451

Delta R.T. -0.01 min

Lab File: BN014417.D

Acq: 25 Apr 2021 00:00

Instrument :

BNA_N

ClientSampleId :

BG4Z8

Tot Ion:	252	Resp:	55288
Ion Ratio	Lower	Upper	
252	100		
253	23.2	17.4	26.2
125	20.7	9.3	13.9#

Manual Integrations
APPROVED

mohammad
4/26/2021 11:42:58 AM

