

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
 Data File : BN014419.D
 Acq On : 25 Apr 2021 01:12
 Operator : CG/JU
 Sample : M2065-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG564

Manual Integrations
 APPROVED

mohammad
 4/26/2021 11:43:03 AM

Quant Time: Apr 26 03:43:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 23 12:06:34 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	113236	20.00	ng/ul	0.00
20) Naphthalene-d8	10.46	136	481260	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.32	164	273592	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.06	188	587926	20.00	ng/ul	0.00
79) Chrysene-d12	21.26	240	644462	20.00	ng/ul	0.00
88) Perylene-d12	23.49	264	598209	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	5571	1.87	ng/uL	0.00
4) Pyridine-d5	3.63	84	16007m	2.03	ng/ul	0.02
7) Phenol-d5	6.85	99	109439	11.56	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.02	67	77489	13.67	ng/ul	0.00
11) 2-Chlorophenol-d4	7.22	132	96364	12.94	ng/ul	0.00
15) 4-Methylphenol-d8	8.38	113	89339	12.45	ng/ul	0.00
21) Nitrobenzene-d5	8.83	128	52329	15.05	ng/ul	0.00
24) 2-Nitrophenol-d4	9.55	143	36074	10.59	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.08	165	84668	11.54	ng/ul	0.00
31) 4-Chloroaniline-d4	10.59	131	109500	10.06	ng/ul	0.00
46) Dimethylphthalate-d6	13.73	166	296992	14.98	ng/ul	0.00
49) Acenaphthylene-d8	14.01	160	395960	16.61	ng/ul	0.00
54) 4-Nitrophenol-d4	14.51	143	12502	3.25	ng/ul	0.00
60) Fluorene-d10	15.32	176	274119	15.65	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.43	200	4820	1.53	ng/ul	0.00
73) Anthracene-d10	17.16	188	408662	14.89	ng/ul	0.00
81) Pyrene-d10	19.46	212	458907	14.67	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.34	264	473349	14.92	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.77	163	46626	2.266	ng/ul	Ovalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014419.D
Acq On : 25 Apr 2021 01:12
Operator : CG/JU
Sample : M2065-11
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BG564

Quant Time: Apr 26 03:43:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 23 12:06:34 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
4/26/2021 11:43:03 AM

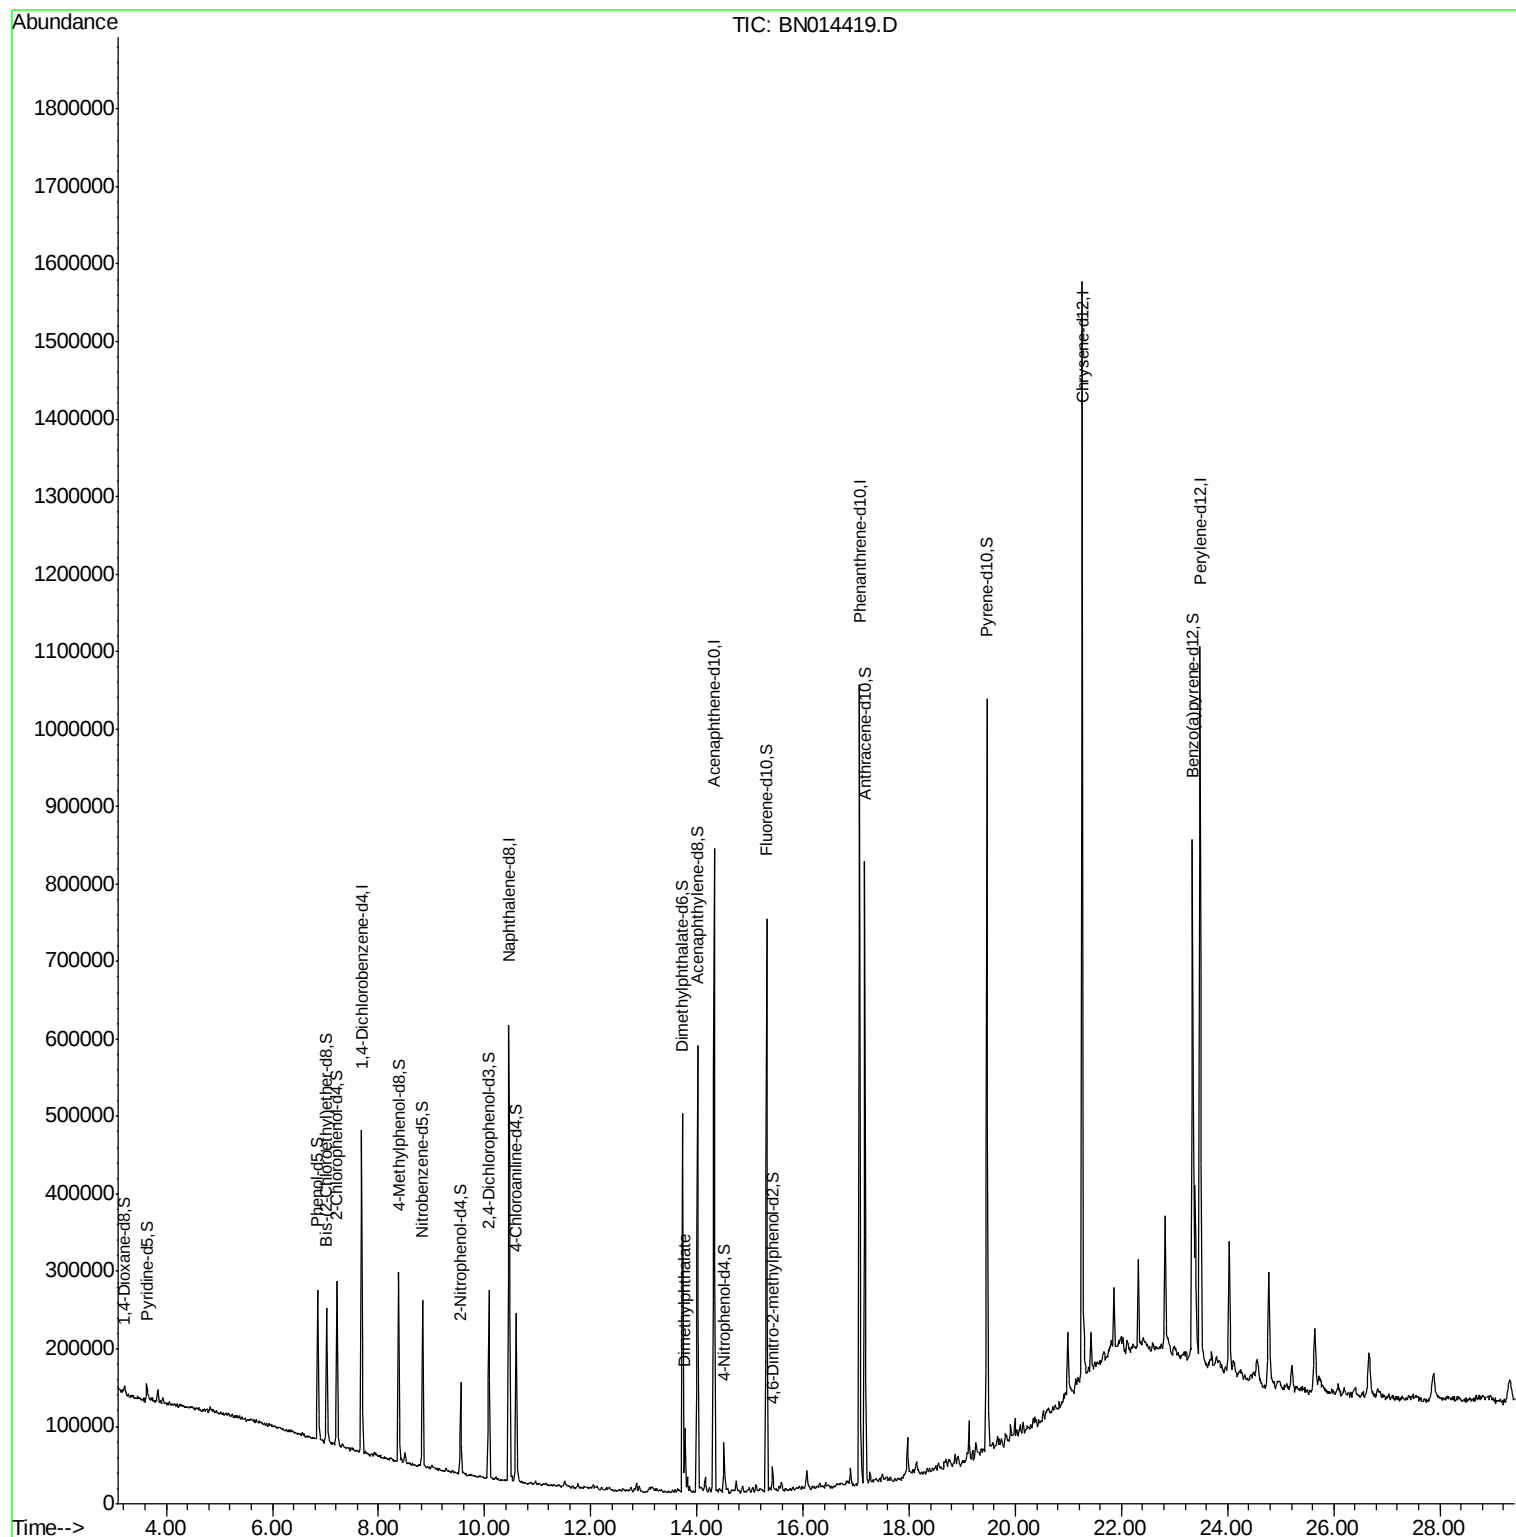

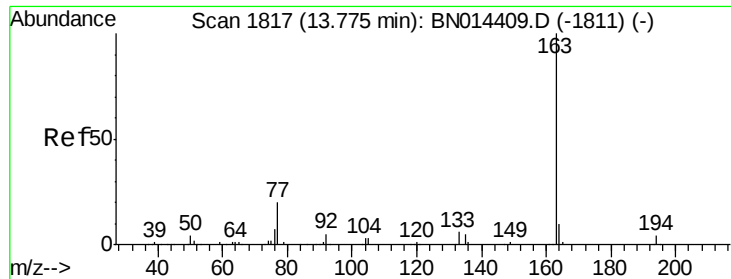

#47
 Dimethylphthalate
 Concen: 2.266 ng/ul
 RT: 13.77 min Scan# 1817
 Delta R.T. -0.01 min
 Lab File: BN014419.D
 Acq: 25 Apr 2021 01:12

Instrument :
 BNA_N
 ClientSampleID :
 BG564

Tot Ion:	163	Resp:	46626
Ion Ratio	Lower	Upper	
163	100		
194	4.2	3.3	4.9
164	9.8	7.8	11.8

Manual Integrations
 APPROVED

mohammad
 4/26/2021 11:43:03 AM

