

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
 Data File : BN014429.D
 Acq On : 25 Apr 2021 07:43
 Operator : CG/JU
 Sample : M2065-12
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG565

Manual Integrations
 APPROVED

mohammad
 4/26/2021 11:43:35 AM

Quant Time: Apr 26 04:44:06 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 23 12:06:34 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	108943	20.00	ng/ul	0.00
20) Naphthalene-d8	10.46	136	477588	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.32	164	275969	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.06	188	590428	20.00	ng/ul	0.00
79) Chrysene-d12	21.26	240	624130	20.00	ng/ul	0.00
88) Perylene-d12	23.49	264	611406	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.21	96	5359	1.87	ng/uL	0.00
4) Pyridine-d5	3.63	84	19688m	2.60	ng/ul	0.02
7) Phenol-d5	6.85	99	119393	13.11	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.02	67	78883	14.46	ng/ul	0.00
11) 2-Chlorophenol-d4	7.22	132	104932	14.65	ng/ul	0.00
15) 4-Methylphenol-d8	8.38	113	94058	13.62	ng/ul	0.00
21) Nitrobenzene-d5	8.83	128	57571	16.68	ng/ul	0.00
24) 2-Nitrophenol-d4	9.55	143	43215	12.79	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.08	165	96049	13.19	ng/ul	0.00
31) 4-Chloroaniline-d4	10.59	131	128054	11.86	ng/ul	0.00
46) Dimethylphthalate-d6	13.73	166	338267	16.92	ng/ul	0.00
49) Acenaphthylene-d8	14.01	160	449487	18.69	ng/ul	0.00
54) 4-Nitrophenol-d4	14.51	143	22890	5.90	ng/ul	0.00
60) Fluorene-d10	15.31	176	308922	17.48	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.43	200	11566	3.66	ng/ul	0.00
73) Anthracene-d10	17.16	188	473223	17.17	ng/ul	0.00
81) Pyrene-d10	19.46	212	534842	17.65	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.34	264	539383	16.63	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.78	163	51802	2.496	ng/ul	Ovalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014429.D
Acq On : 25 Apr 2021 07:43
Operator : CG/JU
Sample : M2065-12
Misc :
ALS Vial : 35 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BG565

Quant Time: Apr 26 04:44:06 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 23 12:06:34 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
4/26/2021 11:43:35 AM

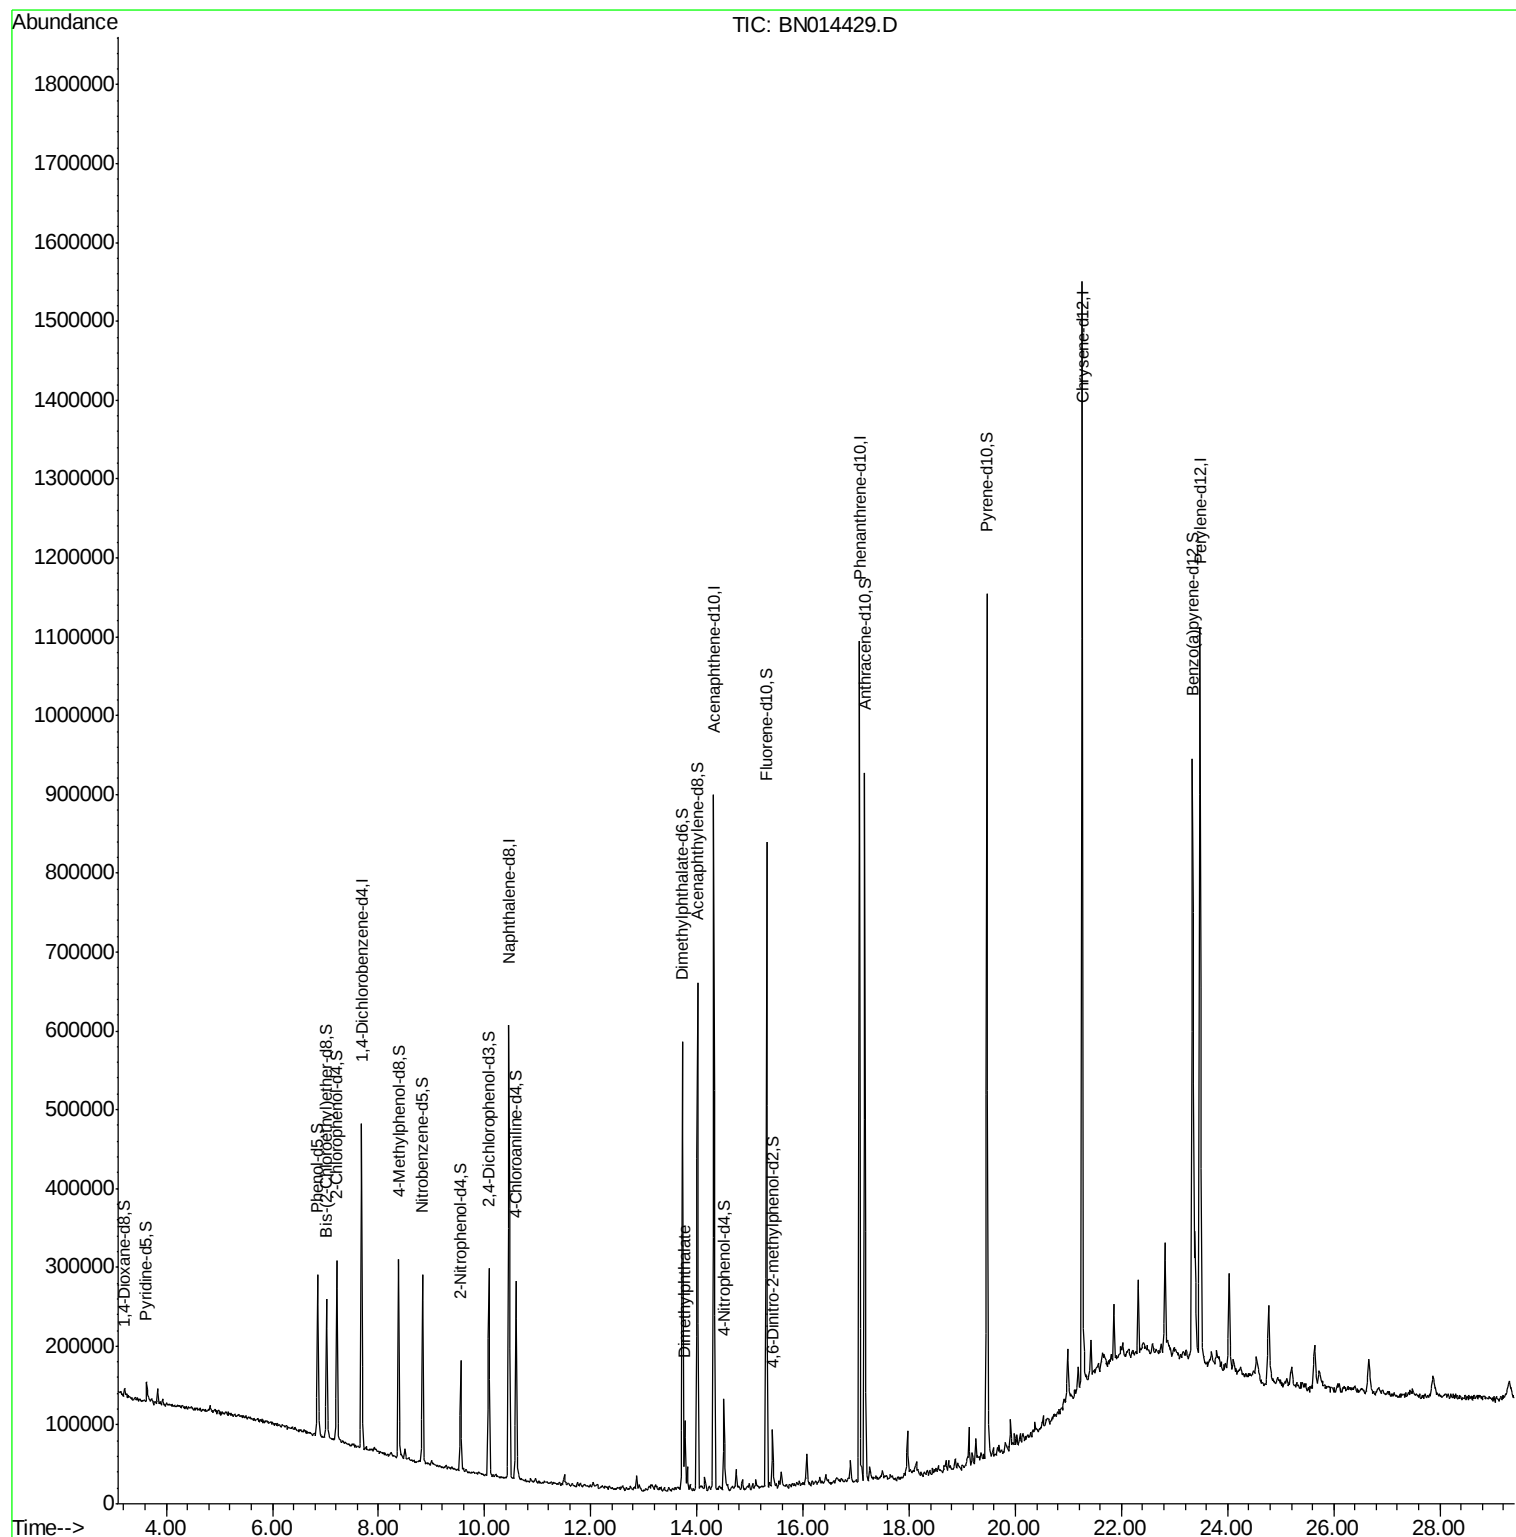

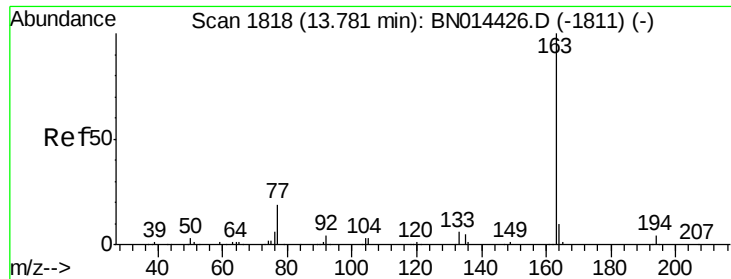

#47
 Dimethylphthalate
 Concen: 2.496 ng/ul
 RT: 13.78 min Scan# 1817
 Delta R.T. -0.01 min
 Lab File: BN014429.D
 Acq: 25 Apr 2021 07:43

Instrument :
 BNA_N
 ClientSampleId :
 BG565

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.3	4.9
164	10.1	7.8	11.8

Manual Integrations
 APPROVED

mohammad
 4/26/2021 11:43:35 AM

