

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
 Data File : BN014396.D
 Acq On : 24 Apr 2021 10:58
 Operator : CG/JU
 Sample : M2065-15
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG568

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.623	89	91	101	rBV2	35157	58046	2.65%	0.225%
2	6.852	634	640	653	rVB	269093	467651	21.34%	1.810%
3	7.022	664	669	677	rBV	223439	350692	16.00%	1.358%
4	7.216	696	702	712	rVB	290991	456949	20.85%	1.769%
5	7.681	775	781	790	rVB	535570	833696	38.04%	3.227%
6	7.752	790	793	799	rBV4	8042	15065	0.69%	0.058%
7	8.234	873	875	880	rVB4	13318	18886	0.86%	0.073%
8	8.381	893	900	907	rBV	303079	485404	22.15%	1.879%
9	8.434	907	909	914	rVV2	11387	17418	0.79%	0.067%
10	8.499	916	920	925	rVB2	23191	35223	1.61%	0.136%
11	8.563	925	931	934	rBV4	8271	16270	0.74%	0.063%
12	8.828	970	976	982	rVB	274650	431833	19.70%	1.672%
13	8.999	1000	1005	1007	rBV4	17467	27786	1.27%	0.108%
14	9.028	1008	1010	1017	rVB5	17435	31238	1.43%	0.121%
15	9.146	1027	1030	1037	rVB5	7356	12674	0.58%	0.049%
16	9.393	1067	1072	1076	rVV5	16081	28276	1.29%	0.109%
17	9.446	1078	1081	1086	rVB3	9306	13724	0.63%	0.053%
18	9.546	1087	1098	1105	rBV	179861	315640	14.40%	1.222%
19	9.646	1111	1115	1123	rVB8	19317	37296	1.70%	0.144%
20	10.081	1180	1189	1196	rBV	329327	544370	24.84%	2.107%
21	10.340	1227	1233	1235	rBV7	6635	12890	0.59%	0.050%
22	10.457	1244	1253	1260	rBV	721528	1229581	56.10%	4.760%
23	10.593	1270	1276	1282	rBV	259510	424539	19.37%	1.643%
24	10.869	1316	1323	1327	rBV6	11247	22598	1.03%	0.087%
25	10.957	1332	1338	1346	rBV5	20406	30359	1.39%	0.118%
26	11.146	1363	1370	1373	rBV8	14884	34337	1.57%	0.133%
27	11.234	1379	1385	1387	rBV6	8679	16742	0.76%	0.065%
28	11.299	1392	1396	1401	rVV5	8583	16554	0.76%	0.064%
29	11.404	1411	1414	1418	rVB5	10295	15091	0.69%	0.058%
30	11.499	1425	1430	1433	rBV2	27880	46384	2.12%	0.180%
31	11.652	1451	1456	1461	rBV4	13478	21695	0.99%	0.084%
32	11.757	1466	1474	1479	rBV5	20336	41177	1.88%	0.159%
33	11.904	1496	1499	1500	rVV3	9870	11974	0.55%	0.046%
34	11.922	1500	1502	1508	rVV7	11664	20883	0.95%	0.081%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
 Data File : BN014396.D
 Acq On : 24 Apr 2021 10:58
 Operator : CG/JU
 Sample : M2065-15
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG568

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

35	11.987	1508	1513	1517	rVV6	11466	24523	1.12%	0.095%
36	12.052	1518	1524	1526	rVV6	15944	31002	1.41%	0.120%
37	12.122	1528	1536	1543	rVB8	21275	66769	3.05%	0.258%
38	12.204	1545	1550	1557	rBV8	17833	39296	1.79%	0.152%
39	12.263	1557	1560	1564	rBV5	11698	14947	0.68%	0.058%
40	12.352	1570	1575	1579	rVV6	13835	24661	1.13%	0.095%
41	12.416	1583	1586	1591	rVB6	7316	12131	0.55%	0.047%
42	12.522	1600	1604	1611	rBV9	9940	23750	1.08%	0.092%
43	12.599	1614	1617	1620	rBV4	12619	16652	0.76%	0.064%
44	12.675	1624	1630	1635	rBV8	17973	36162	1.65%	0.140%
45	12.757	1637	1644	1650	rVB8	23965	47301	2.16%	0.183%
46	12.816	1650	1654	1658	rBV6	19576	32752	1.49%	0.127%
47	12.863	1658	1662	1666	rVV3	40747	59123	2.70%	0.229%
48	12.916	1666	1671	1677	rVB4	23468	40110	1.83%	0.155%
49	13.104	1695	1703	1705	rBV3	33916	57313	2.62%	0.222%
50	13.134	1706	1708	1713	rVV6	26128	43407	1.98%	0.168%
51	13.175	1713	1715	1718	rVV3	16162	19742	0.90%	0.076%
52	13.210	1718	1721	1724	rVV4	14875	22604	1.03%	0.088%
53	13.246	1724	1727	1731	rVV3	17925	25868	1.18%	0.100%
54	13.299	1732	1736	1737	rVV4	10370	14159	0.65%	0.055%
55	13.316	1737	1739	1745	rVB7	17538	27142	1.24%	0.105%
56	13.387	1745	1751	1760	rBV7	17116	38540	1.76%	0.149%
57	13.469	1761	1765	1768	rBV5	16417	22815	1.04%	0.088%
58	13.546	1773	1778	1782	rBV5	13097	22741	1.04%	0.088%
59	13.593	1782	1786	1789	rBV6	10522	16235	0.74%	0.063%
60	13.640	1789	1794	1798	rBV4	31671	55666	2.54%	0.215%
61	13.728	1804	1809	1815	rBV	633105	999992	45.63%	3.871%
62	13.775	1815	1817	1821	rVV	97527	120791	5.51%	0.468%
63	13.816	1821	1824	1828	rVV2	58615	77311	3.53%	0.299%
64	13.863	1828	1832	1838	rVB6	38115	71562	3.27%	0.277%
65	14.010	1848	1857	1863	rBV	725097	1129345	51.53%	4.372%
66	14.157	1878	1882	1889	rVB2	100654	171670	7.83%	0.665%
67	14.228	1889	1894	1898	rBV5	29508	50846	2.32%	0.197%
68	14.316	1900	1909	1917	rVV	1047241	1659304	75.71%	6.423%
69	14.381	1917	1920	1922	rBV3	13810	14171	0.65%	0.055%
70	14.510	1936	1942	1948	rBV	175580	290093	13.24%	1.123%
71	14.651	1961	1966	1968	rBV3	22543	34029	1.55%	0.132%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
 Data File : BN014396.D
 Acq On : 24 Apr 2021 10:58
 Operator : CG/JU
 Sample : M2065-15
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG568

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

72	14.781	1984	1988	1996	rVB6	30160	65314	2.98%	0.253%
73	14.863	1997	2002	2009	rBV9	37589	63446	2.89%	0.246%
74	14.951	2011	2017	2020	rBV6	29000	56512	2.58%	0.219%
75	14.987	2020	2023	2028	rVB4	39291	54769	2.50%	0.212%
76	15.045	2029	2033	2039	rBV7	31786	56937	2.60%	0.220%
77	15.116	2040	2045	2049	rBV2	52192	78173	3.57%	0.303%
78	15.316	2073	2079	2084	rVB	934816	1326029	60.50%	5.133%
79	15.369	2085	2088	2091	rBV4	28362	37933	1.73%	0.147%
80	15.428	2093	2098	2102	rBV	112809	144522	6.59%	0.559%
81	15.598	2123	2127	2135	rVB3	42108	79519	3.63%	0.308%
82	15.745	2149	2152	2157	rBV6	17113	34359	1.57%	0.133%
83	16.075	2205	2208	2213	rVB	78036	109231	4.98%	0.423%
84	16.428	2264	2268	2273	rBV4	47060	80804	3.69%	0.313%
85	16.898	2345	2348	2356	rVB4	67583	110678	5.05%	0.428%
86	17.063	2371	2376	2381	rBV	1249578	1743410	79.55%	6.749%
87	17.104	2381	2383	2387	rVB	83729	96847	4.42%	0.375%
88	17.163	2387	2393	2397	rBV	1065818	1493958	68.16%	5.783%
89	17.198	2397	2399	2404	rVB	177115	199160	9.09%	0.771%
90	17.263	2406	2410	2415	rBV6	37168	72766	3.32%	0.282%
91	17.969	2527	2530	2536	rVB4	86154	137934	6.29%	0.534%
92	18.069	2544	2547	2551	rBV	44973	63676	2.91%	0.246%
93	18.745	2659	2662	2665	rBV2	36923	48853	2.23%	0.189%
94	18.869	2679	2683	2687	rBV	75820	100088	4.57%	0.387%
95	19.128	2723	2727	2732	rVB	215287	274534	12.53%	1.063%
96	19.463	2779	2784	2788	rBV2	1297551	1819917	83.04%	7.045%
97	19.992	2871	2874	2878	rVB	82987	99637	4.55%	0.386%
98	21.263	3084	3090	3094	rBV	1517442	2094303	95.56%	8.107%
99	23.345	3438	3444	3449	rBV	838417	1500285	68.45%	5.808%
100	23.486	3462	3468	3485	rVB2	1129729	2191691	100.00%	8.484%


Sum of corrected areas: 25832751

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
Data File : BN014396.D
Acq On : 24 Apr 2021 10:58
Operator : CG/JU
Sample : M2065-15
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG568

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

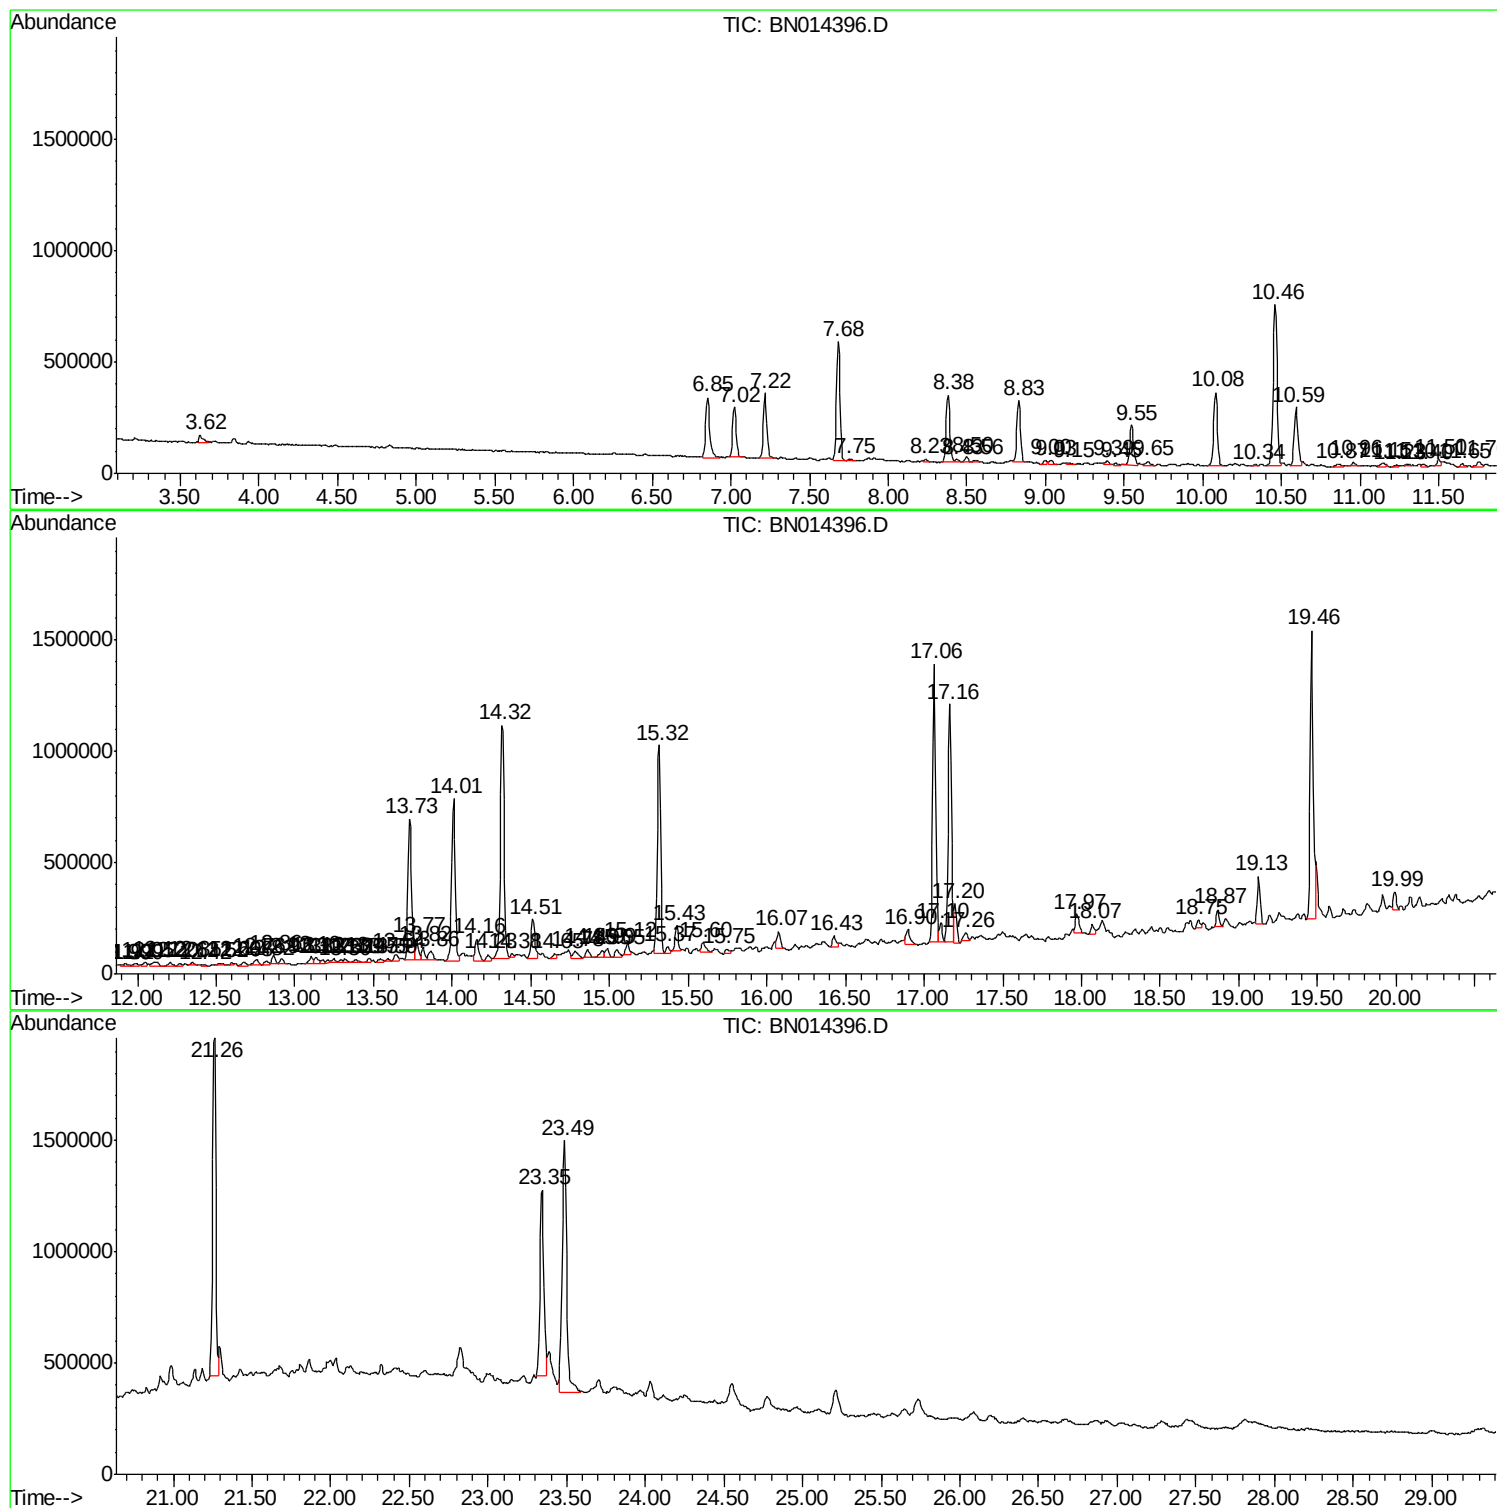

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014396.D
Acq On : 24 Apr 2021 10:58
Operator : CG/JU
Sample : M2065-15
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
BG568

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.16	2.07 ng/ul	171670	Acenaphthene-d10	14.32
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1	Decahydro-4,4,8,9,10-pentamethyl...	208 C15H28	080655-44-3	43
2	4H-1,3,2-Dioxaborin, 4-ethenyl-2...	208 C12H21B02	074630-04-9	25
3	Pvrimido(5,4-e)-as-triazine-5,7(...	193 C7H7N5O2	000084-82-2	16
4	Pyrazole, 5-methyl-3-(5-nitro-2-...	193 C8H7N3O3	016239-90-0	14
5	s-Triazine, 2-amino-4-(piperidin...	276 C14H24N6	021868-43-9	14

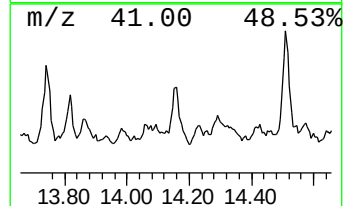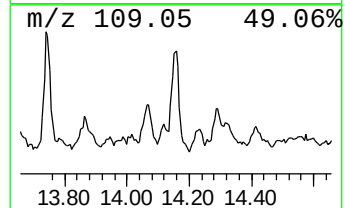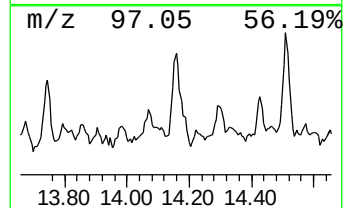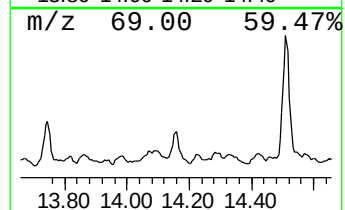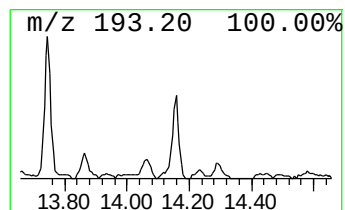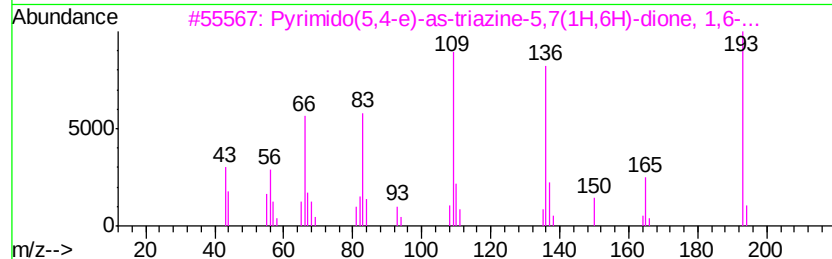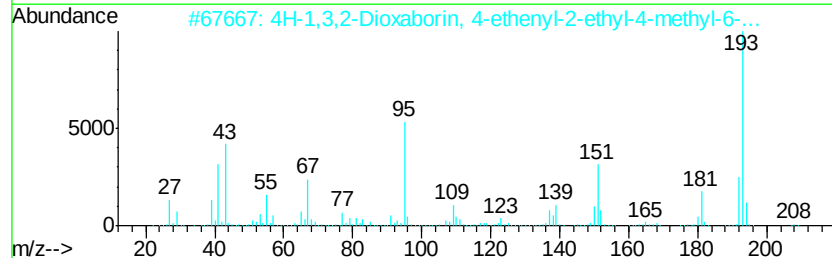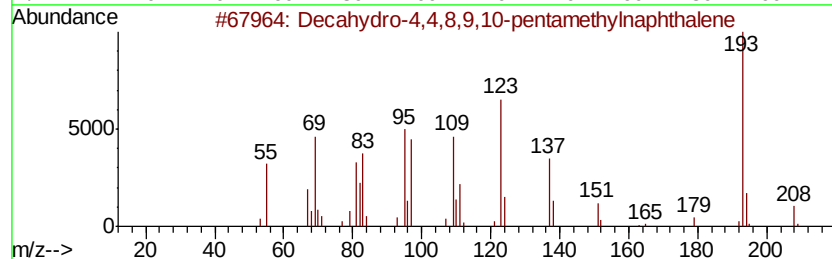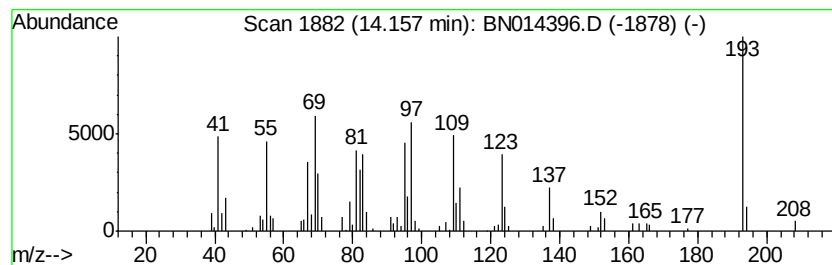

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014396.D
Acq On : 24 Apr 2021 10:58
Operator : CG/JU
Sample : M2065-15
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG568

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	14.16	2.1	ng/ul	171670	3	14.32	1659300	20.0