

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
 Data File : BN014398.D
 Acq On : 24 Apr 2021 12:09
 Operator : CG/JU
 Sample : M2065-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG572

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.623	89	91	101	rBV	57930	104781	5.51%	0.461%
2	6.852	635	640	651	rVB	305304	500509	26.32%	2.200%
3	7.022	664	669	678	rVB	260428	408003	21.46%	1.794%
4	7.216	697	702	710	rVB	329594	521825	27.44%	2.294%
5	7.681	776	781	789	rVB	515644	803051	42.23%	3.530%
6	8.381	894	900	912	rVB	384198	600877	31.60%	2.642%
7	8.828	970	976	986	rVB	323849	535639	28.17%	2.355%
8	9.546	1092	1098	1106	rBV	208936	336836	17.72%	1.481%
9	10.081	1183	1189	1199	rBV	368498	585344	30.78%	2.573%
10	10.457	1246	1253	1261	rVB	691890	1170800	61.58%	5.147%
11	10.593	1270	1276	1285	rBV	361238	585368	30.79%	2.573%
12	12.052	1520	1524	1531	rVB3	5340	9605	0.51%	0.042%
13	13.157	1707	1712	1717	rBV2	5532	7774	0.41%	0.034%
14	13.222	1719	1723	1727	rVB4	1599	2334	0.12%	0.010%
15	13.640	1792	1794	1799	rVB3	2886	2985	0.16%	0.013%
16	13.728	1803	1809	1814	rVV	707456	928291	48.82%	4.081%
17	13.775	1814	1817	1823	rVB	88010	116307	6.12%	0.511%
18	14.010	1850	1857	1865	rBV	838774	1184742	62.31%	5.208%
19	14.216	1886	1892	1893	rBV5	2127	3100	0.16%	0.014%
20	14.234	1893	1895	1902	rVB3	4064	5030	0.26%	0.022%
21	14.316	1903	1909	1918	rBV	1005782	1509074	79.37%	6.634%
22	14.510	1936	1942	1957	rBV	165566	249654	13.13%	1.098%
23	14.740	1977	1981	1985	rVB2	23328	25789	1.36%	0.113%
24	15.145	2044	2050	2053	rBV3	4804	7481	0.39%	0.033%
25	15.187	2053	2057	2063	rVB3	3871	4492	0.24%	0.020%
26	15.316	2072	2079	2086	rBV	991442	1399704	73.61%	6.153%
27	15.428	2093	2098	2105	rVB	114647	149628	7.87%	0.658%
28	15.551	2115	2119	2123	rBV	7696	9917	0.52%	0.044%
29	15.598	2123	2127	2129	rVV3	1650	2725	0.14%	0.012%
30	15.916	2178	2181	2185	rVB2	1466	2093	0.11%	0.009%
31	15.992	2189	2194	2197	rBV4	1696	2422	0.13%	0.011%
32	16.092	2210	2211	2216	rVB2	2461	2821	0.15%	0.012%
33	16.316	2245	2249	2252	rBV2	5720	7155	0.38%	0.031%
34	16.463	2271	2274	2278	rVB4	1507	2389	0.13%	0.011%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
 Data File : BN014398.D
 Acq On : 24 Apr 2021 12:09
 Operator : CG/JU
 Sample : M2065-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG572

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
 Title : SVOA CALIBRATION

35	16.828	2331	2336	2337	rBV2	4219	5116	0.27%	0.022%
36	17.063	2370	2376	2383	rBV	1219453	1670104	87.83%	7.342%
37	17.163	2387	2393	2402	rVV	1050096	1434488	75.44%	6.306%
38	17.257	2406	2409	2414	rVB3	18834	22479	1.18%	0.099%
39	17.357	2424	2426	2430	rBV2	2000	2688	0.14%	0.012%
40	17.587	2461	2465	2468	rVB4	1745	2330	0.12%	0.010%
41	17.751	2490	2493	2496	rBV3	2219	2421	0.13%	0.011%
42	17.969	2525	2530	2535	rBV2	32679	45024	2.37%	0.198%
43	18.045	2541	2543	2546	rVB2	3688	3394	0.18%	0.015%
44	18.081	2546	2549	2552	rBV4	1425	2140	0.11%	0.009%
45	18.545	2623	2628	2630	rBV3	3133	4166	0.22%	0.018%
46	18.745	2657	2662	2663	rBV3	2128	3193	0.17%	0.014%
47	18.869	2679	2683	2686	rBV5	2876	3714	0.20%	0.016%
48	18.910	2688	2690	2694	rVB3	2161	2726	0.14%	0.012%
49	19.098	2718	2722	2724	rBV	11183	14075	0.74%	0.062%
50	19.128	2725	2727	2730	rVB2	9393	8946	0.47%	0.039%
51	19.257	2745	2749	2753	rBV3	15954	18107	0.95%	0.080%
52	19.351	2762	2765	2770	rVB	7265	7163	0.38%	0.031%
53	19.463	2778	2784	2793	rBV	1315130	1711866	90.03%	7.526%
54	19.986	2871	2873	2877	rBV5	3601	5532	0.29%	0.024%
55	20.980	3039	3042	3050	rBV3	50588	81262	4.27%	0.357%
56	21.263	3084	3090	3098	rBV	1415460	1877009	98.72%	8.252%
57	21.427	3115	3118	3121	rBV3	22692	28095	1.48%	0.124%
58	21.863	3189	3192	3196	rVB4	28163	33857	1.78%	0.149%
59	22.322	3267	3270	3274	rBV2	44448	53702	2.82%	0.236%
60	22.822	3352	3355	3361	rVB2	69436	99051	5.21%	0.435%
61	23.345	3437	3444	3449	rBV	910888	1620187	85.21%	7.123%
62	23.486	3461	3468	3480	rVB	1038954	1901416	100.00%	8.359%
63	24.033	3556	3561	3568	rVB	82010	155990	8.20%	0.686%
64	24.774	3683	3687	3696	rVB3	68695	137917	7.25%	0.606%


Sum of corrected areas: 22746703

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042421\
Data File : BN014398.D
Acq On : 24 Apr 2021 12:09
Operator : CG/JU
Sample : M2065-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG572

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

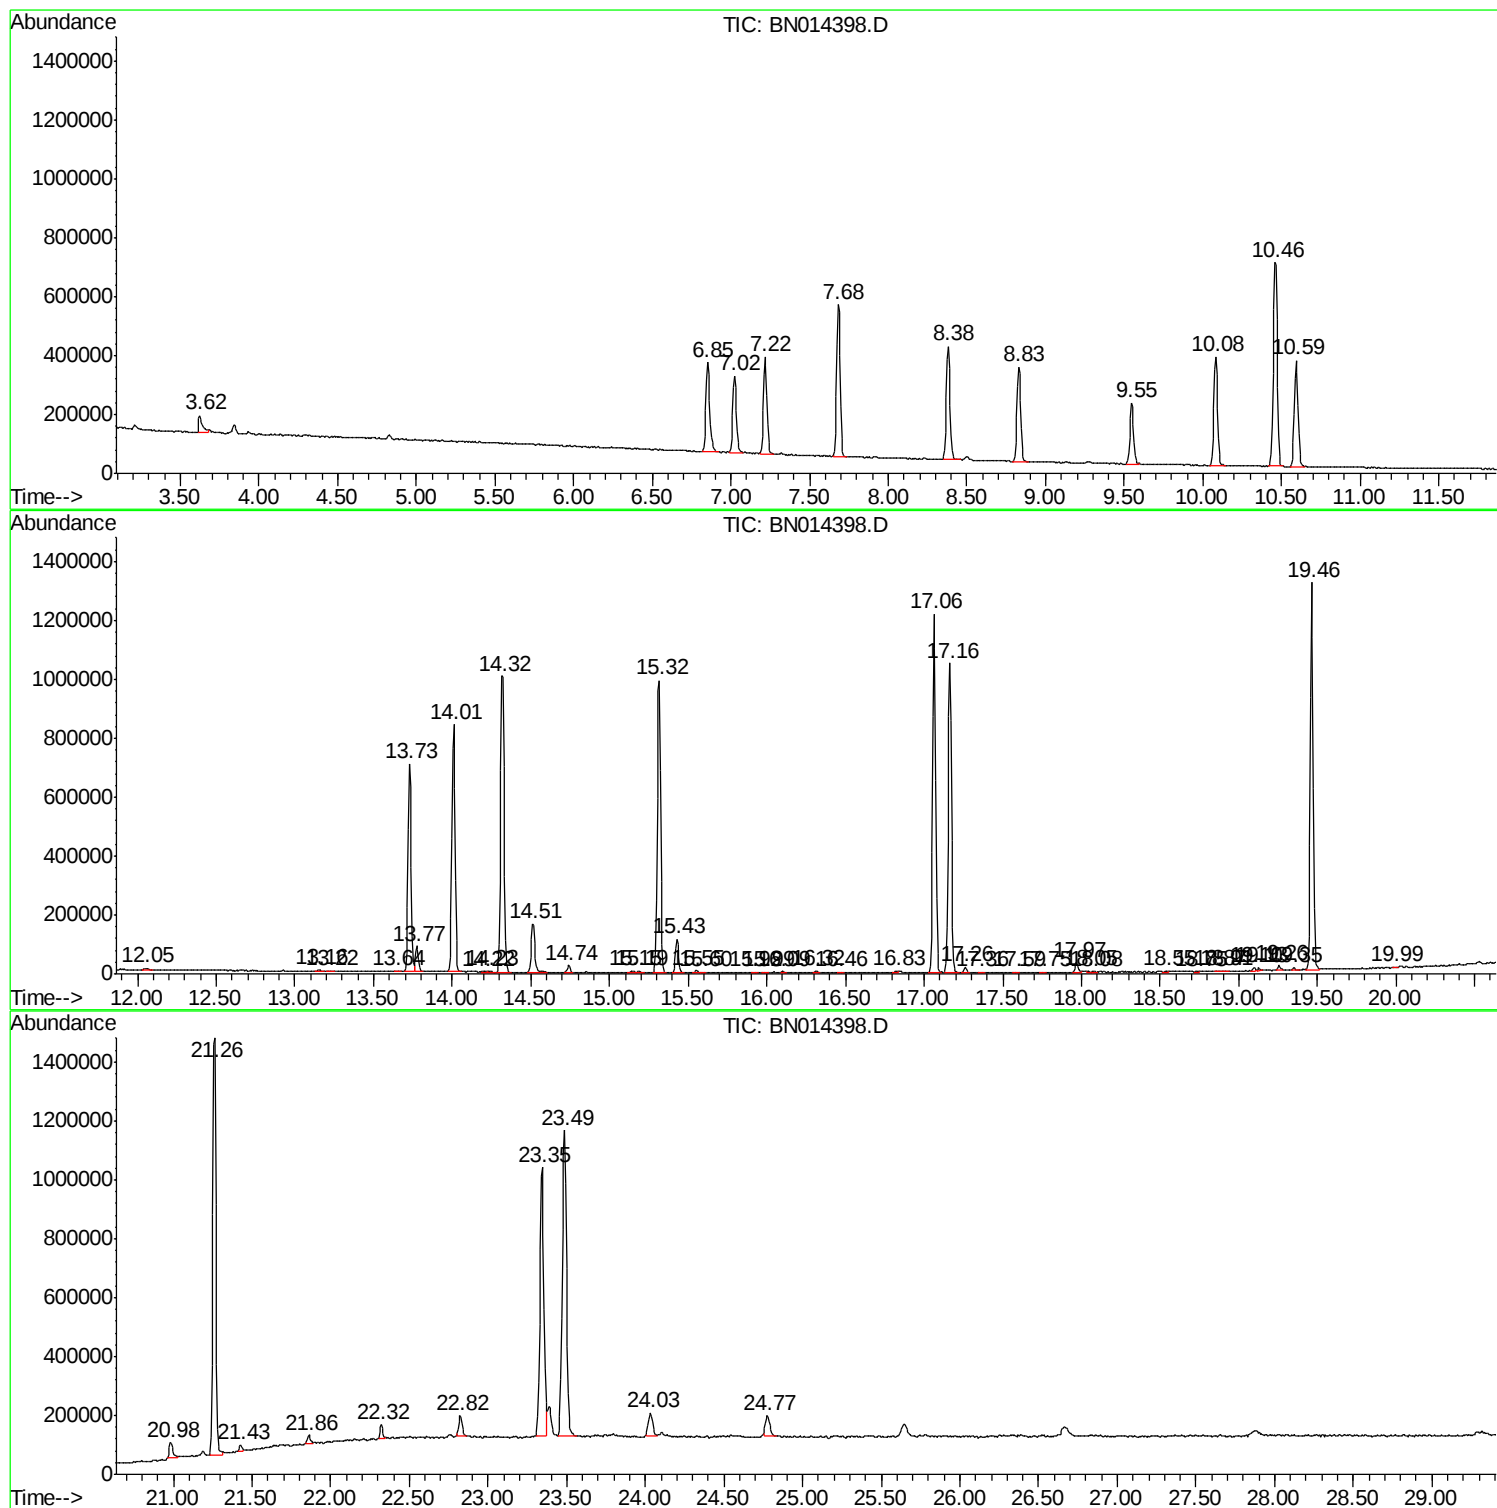

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014398.D
Acq On : 24 Apr 2021 12:09
Operator : CG/JU
Sample : M2065-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG572

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042421\
Data File : BN014398.D
Acq On : 24 Apr 2021 12:09
Operator : CG/JU
Sample : M2065-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG572

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN041521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc